

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
 Data File : VV031051.D
 Acq On : 16 May 2023 14:29
 Operator : SY/MD
 Sample : 02790-08DL 200X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0NY2DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031051.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	86	rVB	61364	70428	14.57%	1.633%
2	1.535	146	154	165	rBV	59021	70981	14.68%	1.646%
3	2.063	309	318	330	rBV	130724	188002	38.89%	4.358%
4	2.455	431	440	449	rBV	14629	25667	5.31%	0.595%
5	3.828	852	867	897	rBV4	56015	209797	43.40%	4.864%
6	4.259	985	1001	1022	rBV2	95891	237724	49.18%	5.511%
7	4.966	1205	1221	1250	rBV5	184997	483368	100.00%	11.206%
8	5.542	1389	1400	1425	rBV	146148	310299	64.20%	7.193%
9	5.841	1480	1493	1515	rBV	191157	392782	81.26%	9.106%
10	5.998	1528	1542	1558	rBV3	111824	234646	48.54%	5.440%
11	6.921	1819	1829	1845	rBV2	45163	85593	17.71%	1.984%
12	7.252	1920	1932	1950	rBV	199843	362072	74.91%	8.394%
13	7.564	2019	2029	2042	rBV2	27203	54444	11.26%	1.262%
14	8.037	2165	2176	2206	rBV	155795	383598	79.36%	8.893%
15	8.792	2400	2411	2432	rBV	223082	382608	79.15%	8.870%
16	10.162	2824	2837	2852	rBV2	81667	134333	27.79%	3.114%
17	11.194	3145	3158	3177	rBV	217101	354762	73.39%	8.224%
18	11.570	3262	3275	3292	rBV	196809	325730	67.39%	7.551%
19	12.201	3464	3471	3483	rVB9	3751	6779	1.40%	0.157%




Sum of corrected areas: 4313613

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
Data File : VV031051.D
Acq On : 16 May 2023 14:29
Operator : SY/MD
Sample : 02790-08DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CONY2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

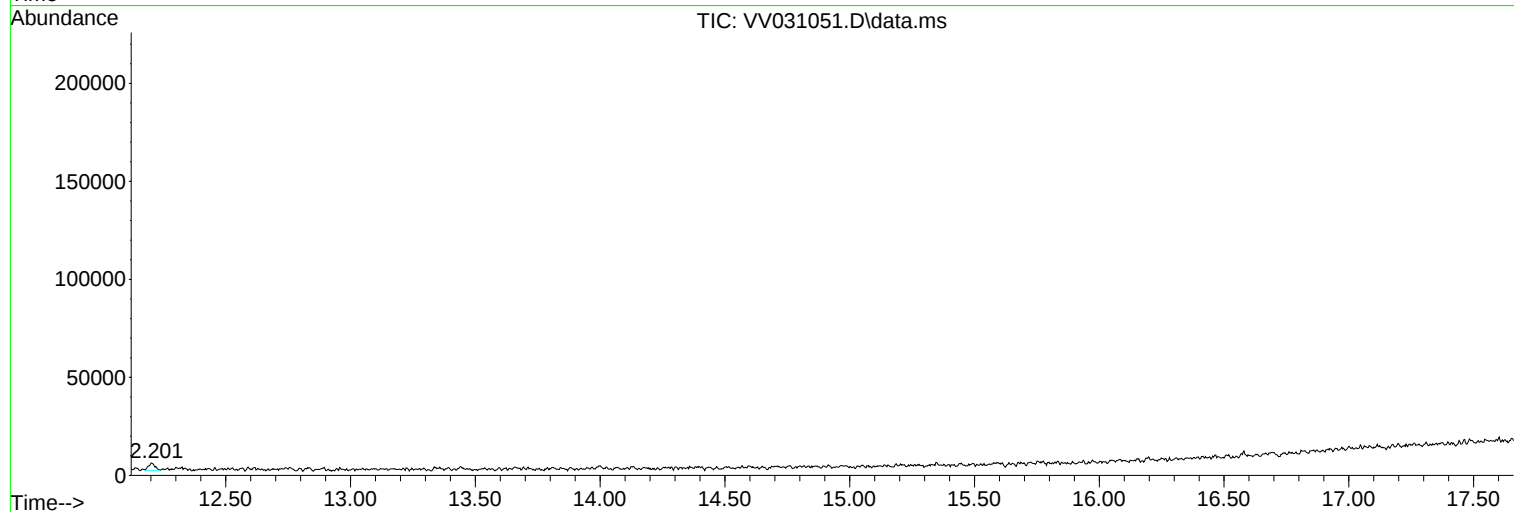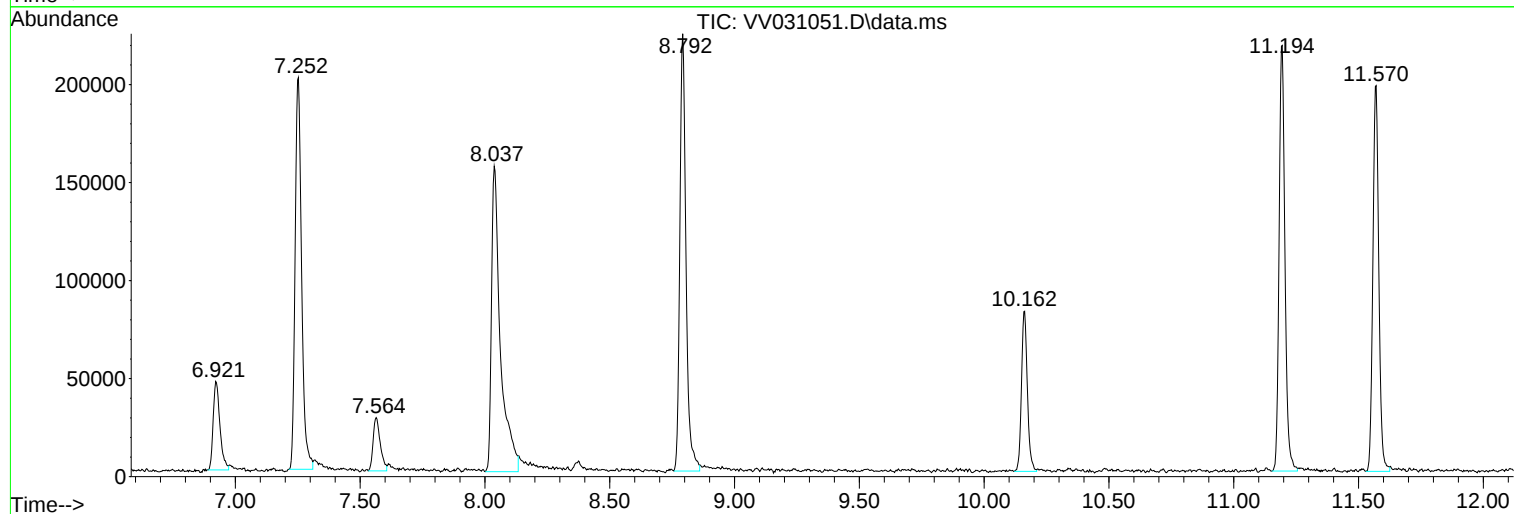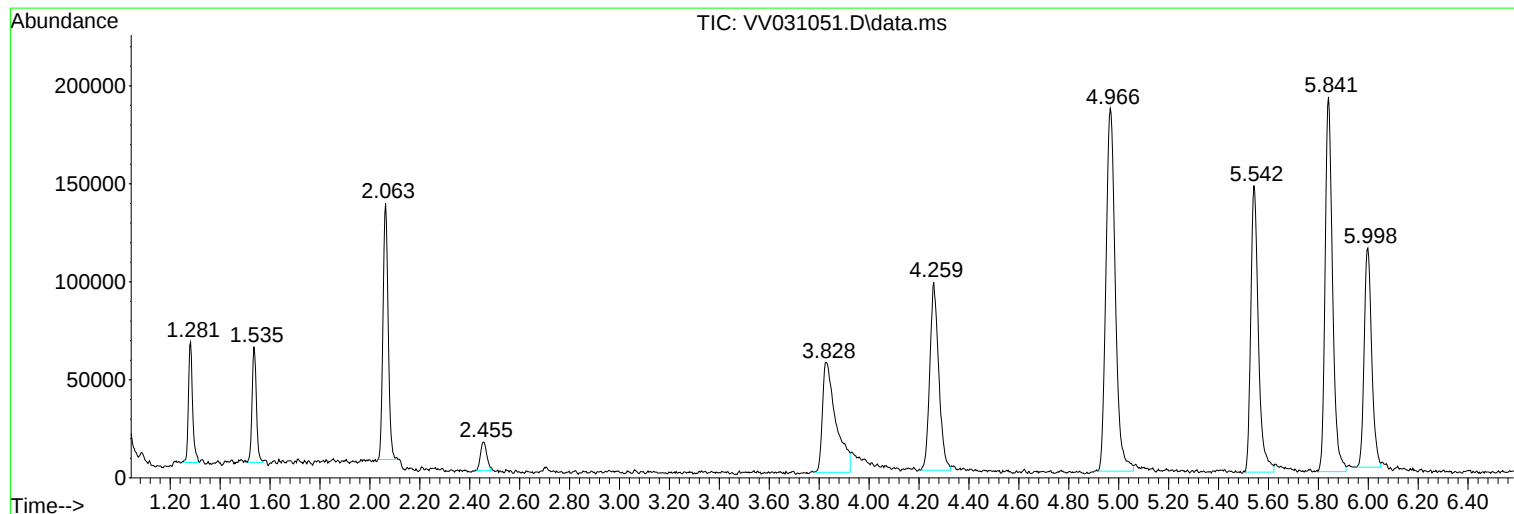

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
Data File : VV031051.D
Acq On : 16 May 2023 14:29
Operator : SY/MD
Sample : 02790-08DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0NY2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
Data File : VV031051.D
Acq On : 16 May 2023 14:29
Operator : SY/MD
Sample : 02790-08DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0NY2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc