

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
 Data File : VV031057.D
 Acq On : 16 May 2023 16:50
 Operator : SY/MD
 Sample : 02768-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CONP5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031057.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	85	rVB	55807	61620	12.95%	1.529%
2	1.539	147	155	165	rBV	60885	75142	15.79%	1.865%
3	2.063	306	318	329	rBV	123305	182238	38.30%	4.522%
4	3.822	853	865	887	rBV2	44129	156762	32.95%	3.890%
5	4.256	987	1000	1025	rVB2	90020	225851	47.47%	5.604%
6	4.966	1204	1221	1245	rBV3	180322	475795	100.00%	11.806%
7	5.542	1387	1400	1426	rBV	141870	301539	63.38%	7.482%
8	5.998	1527	1542	1565	rBV2	114944	242278	50.92%	6.012%
9	6.924	1818	1830	1845	rBV	42346	83659	17.58%	2.076%
10	7.252	1920	1932	1951	rBV	192322	350654	73.70%	8.701%
11	7.561	2020	2028	2044	rBV2	27025	48302	10.15%	1.199%
12	7.883	2118	2128	2138	rBV3	13712	24833	5.22%	0.616%
13	8.034	2163	2175	2211	rBV	213148	461876	97.07%	11.461%
14	8.793	2398	2411	2436	rBV	216751	378584	79.57%	9.394%
15	10.159	2823	2836	2853	rBV	92174	150320	31.59%	3.730%
16	10.333	2877	2890	2902	rVB	40665	71926	15.12%	1.785%
17	11.191	3145	3157	3177	rBV	225207	363221	76.34%	9.013%
18	11.503	3245	3254	3264	rBV7	8173	16130	3.39%	0.400%
19	11.567	3264	3274	3293	rVB	201215	333101	70.01%	8.265%
20	12.204	3462	3472	3483	rBV3	12087	20020	4.21%	0.497%
21	13.995	4022	4029	4036	rVB7	4047	6214	1.31%	0.154%


Sum of corrected areas: 4030065

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
Data File : VV031057.D
Acq On : 16 May 2023 16:50
Operator : SY/MD
Sample : 02768-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CONP5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

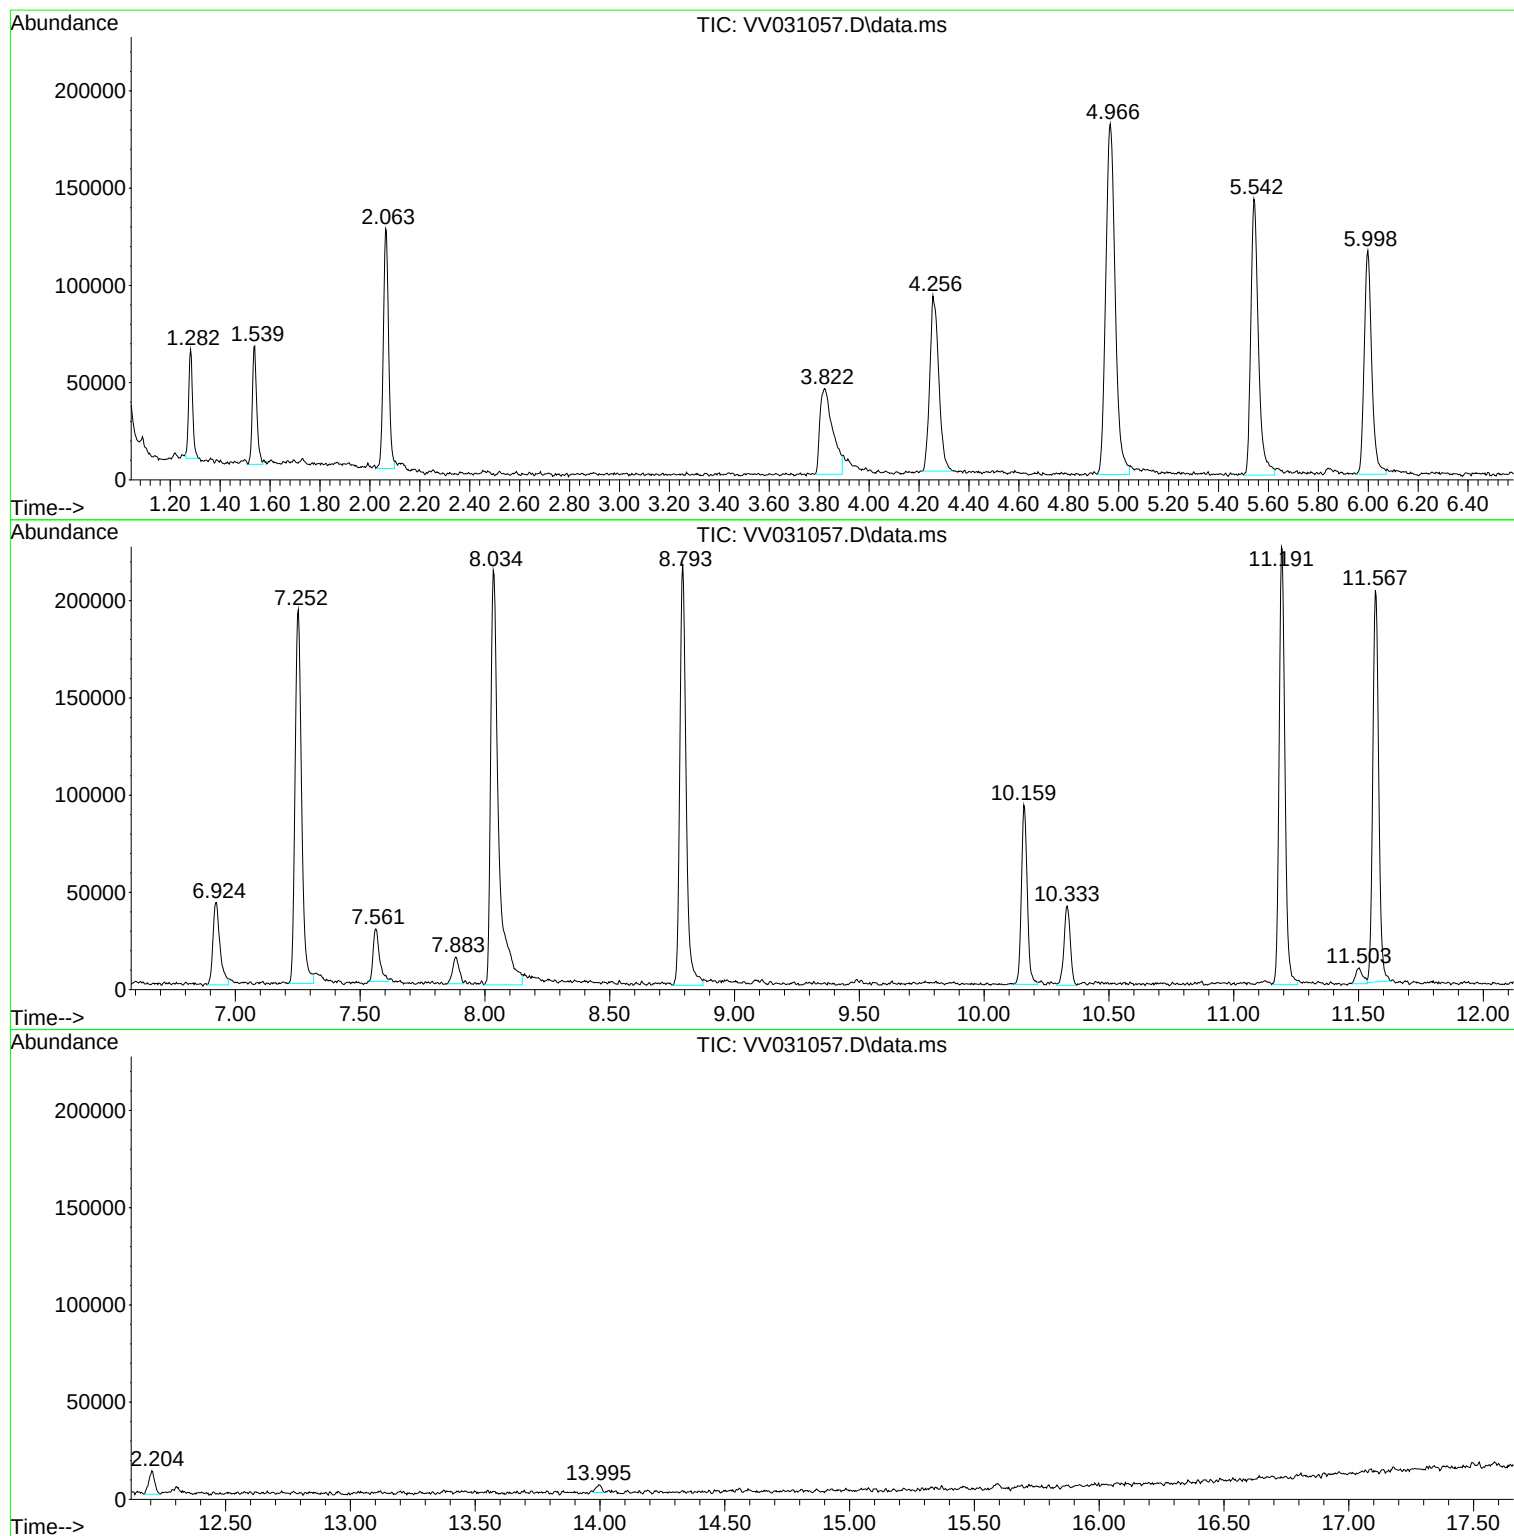

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
Data File : VV031057.D
Acq On : 16 May 2023 16:50
Operator : SY/MD
Sample : 02768-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CONP5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
Data File : VV031057.D
Acq On : 16 May 2023 16:50
Operator : SY/MD
Sample : 02768-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CONP5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------