


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
Data File : VV031040.D
Acq On : 16 May 2023 09:25
Operator : SY/MD
Sample : BFB262
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB262

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed May 17 01:41:23 2023

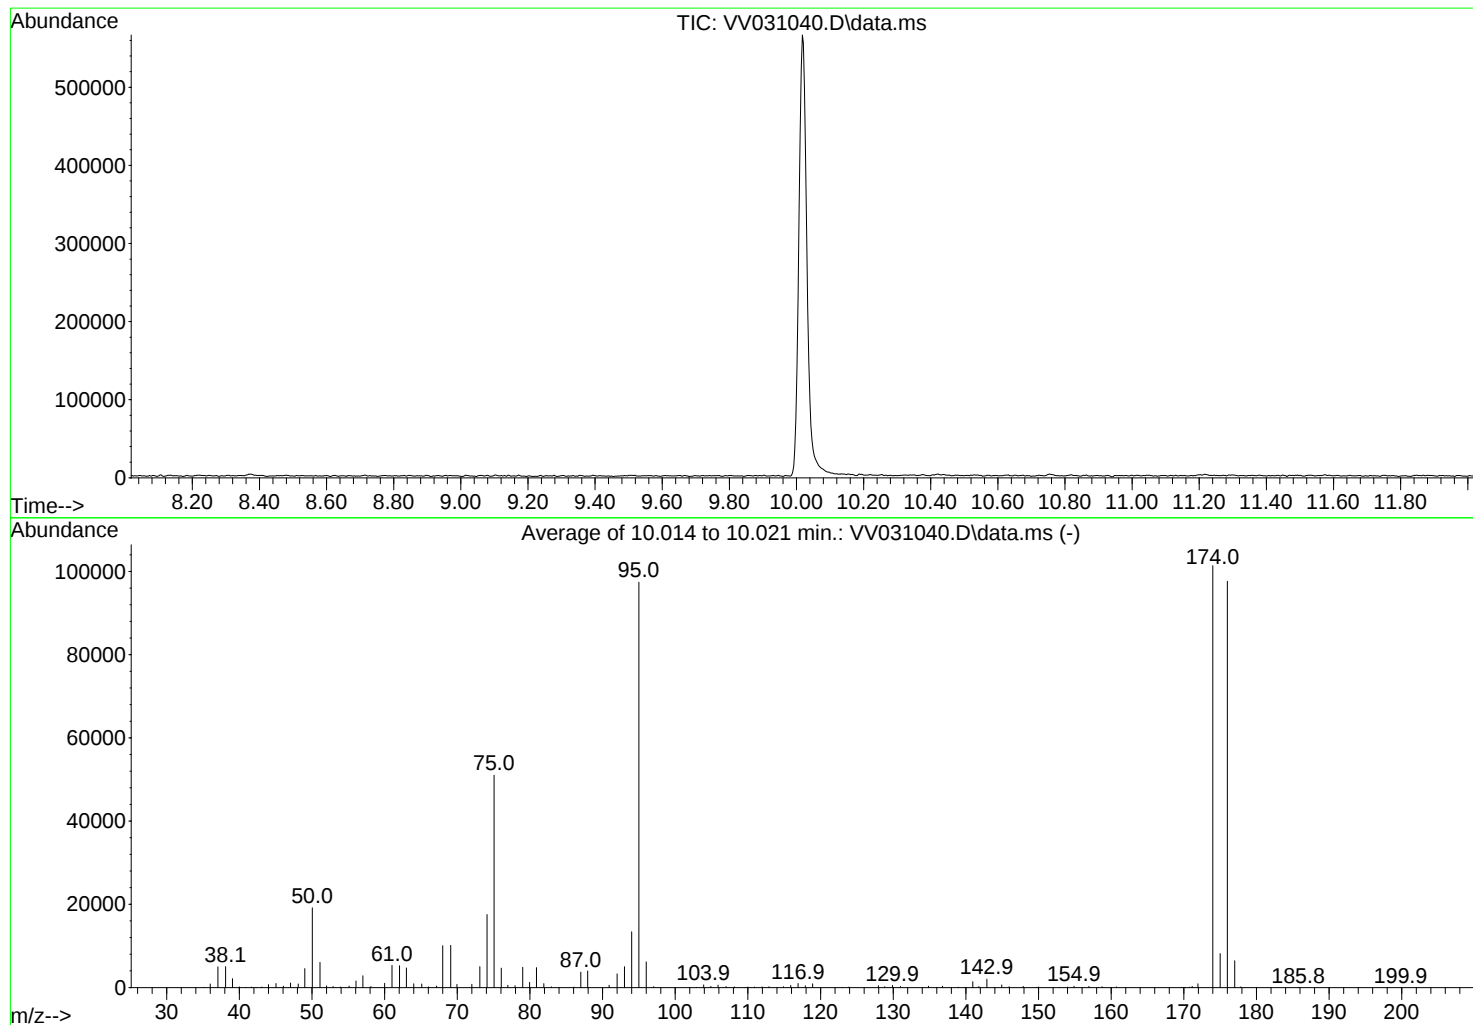

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	19173	PASS
75	95	30	80	52.4	51048	PASS
95	95	100	100	100.0	97421	PASS
96	95	5	9	6.3	6178	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	104.0	101360	PASS
175	174	5	9	8.1	8186	PASS
176	174	95	105	96.3	97629	PASS
177	176	5	10	6.6	6455	PASS

m/z	Abundance
35.60	155.0
36.20	119.0
36.60	121.0
37.70	127.0
39.30	170.0
40.00	190.0
40.90	126.0
42.60	113.0
43.90	225.0
44.50	149.0
45.40	131.0
45.80	150.0
46.50	106.0
47.40	114.0
51.50	105.0
59.30	143.0
69.90	107.0
74.10	101.0
159.20	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB262

m/z	Abundance
36.00	860.0
37.10	4781.0
38.10	4878.0
39.10	2013.0
40.00	360.0
41.00	188.0
41.60	169.0
42.30	113.0
43.10	143.0
44.00	922.0
45.10	904.0
46.10	269.0
47.10	1151.0
48.10	828.0
49.00	4340.0
50.10	18880.0
51.10	5966.0
52.00	391.0
52.90	206.0
54.00	151.0
55.10	339.0
56.00	1599.0
57.00	2612.0
58.10	211.0
60.00	1033.0
61.00	5331.0
62.10	5356.0
63.00	4348.0
64.00	900.0
65.10	753.0
66.00	194.0
67.10	319.0
68.00	9993.0
69.10	9614.0
70.00	819.0
72.00	649.0
73.10	4717.0
74.10	16984.0
75.00	48952.0
76.00	4672.0
76.90	519.0
78.10	489.0
79.00	4725.0
80.00	1261.0
80.90	4716.0
81.90	949.0
83.00	207.0
86.10	121.0
87.00	3622.0
87.90	3892.0
90.90	534.0
92.00	3323.0
93.00	4667.0
94.00	13130.0
95.00	93368.0
96.00	6151.0
97.10	204.0
102.90	127.0
103.90	615.0
104.90	240.0
105.90	542.0
107.00	250.0
108.10	180.0
109.60	103.0
110.00	137.0
110.90	164.0
111.90	129.0
112.90	197.0
114.90	247.0
116.00	503.0
116.90	904.0
117.90	430.0
118.90	831.0
123.90	168.0
128.00	409.0
128.90	207.0
129.90	491.0
130.90	271.0
134.80	285.0
136.70	321.0
139.00	122.0
140.90	1156.0
141.80	209.0
142.90	1974.0
144.90	614.0
145.90	231.0
147.90	206.0
149.70	129.0
150.00	136.0
154.00	129.0
154.90	316.0
157.00	302.0

Instrument :
MSVOA_V
ClientSampleId :
BFB262

158.80	223.0
160.70	168.0
171.30	265.0
171.90	848.0
174.00	95944.0
175.00	7922.0
176.00	90984.0
177.00	6419.0
177.90	204.0
185.80	129.0

Instrument :
MSVOA_V
ClientSampleId :
BFB262

m/z	Abundance
36.00	1001.0
37.00	5110.0
38.10	5174.0
39.10	2177.0
40.00	376.0
40.90	166.0
41.60	151.0
43.10	153.0
44.10	938.0
45.00	1014.0
46.00	377.0
47.10	1125.0
48.10	936.0
49.00	4790.0
50.00	19896.0
51.10	6179.0
52.00	393.0
52.90	247.0
54.00	150.0
55.10	356.0
56.10	1605.0
57.00	2904.0
58.10	277.0
60.00	1057.0
61.00	5501.0
62.00	5372.0
63.00	4931.0
64.00	951.0
65.10	882.0
66.00	189.0
67.20	389.0
68.00	10253.0
69.10	10546.0
70.00	922.0
72.00	832.0
73.10	5199.0
74.10	18224.0
75.10	52600.0
76.00	4724.0
76.90	599.0
77.90	418.0
79.00	4973.0
80.00	1283.0
80.90	4912.0
81.90	992.0
83.00	172.0
86.10	106.0
87.00	3855.0
88.00	4094.0
90.90	600.0
92.00	3424.0
93.00	5102.0
94.00	13920.0
95.00	100880.0
96.00	6230.0
97.10	219.0
102.90	108.0
103.90	671.0
104.90	299.0
105.90	655.0
107.00	268.0
108.20	187.0
110.00	158.0
110.90	138.0
112.00	168.0
112.90	217.0
114.90	207.0
115.90	509.0
116.90	979.0
117.90	433.0
118.90	973.0
123.00	101.0
123.90	148.0
128.00	449.0
128.80	199.0
129.90	565.0
131.00	278.0
134.90	347.0
136.80	321.0
138.90	121.0
141.00	1437.0
141.80	252.0
142.90	2087.0
143.90	108.0
144.90	666.0
145.90	211.0
147.90	315.0
150.00	148.0
152.90	106.0
154.00	133.0
154.90	372.0
156.90	310.0

Instrument :
MSVOA_V
ClientSampleId :
BFB262

158.20	106.0
158.70	231.0
160.70	153.0
169.70	100.0
170.20	103.0
171.10	304.0
172.00	936.0
174.00	104560.0
175.00	8429.0
176.00	100848.0
177.00	6601.0
177.80	146.0

Instrument :
MSVOA_V
ClientSampleId :
BFB262

m/z	Abundance
35.10	136.0
36.00	1086.0
37.10	5095.0
38.10	4972.0
39.00	2166.0
40.00	344.0
41.00	198.0
41.70	119.0
43.10	150.0
44.10	996.0
45.00	1036.0
46.00	363.0
47.00	1016.0
48.10	828.0
49.00	4573.0
50.10	18744.0
51.10	5979.0
52.00	391.0
52.90	274.0
53.80	134.0
55.10	374.0
56.10	1536.0
57.00	2944.0
58.10	248.0
60.00	1005.0
61.00	5129.0
62.00	5060.0
63.00	4833.0
64.00	915.0
65.10	952.0
66.10	139.0
67.20	437.0
68.00	9877.0
69.10	10268.0
70.00	867.0
72.00	917.0
73.10	5126.0
74.10	17712.0
75.10	51592.0
76.10	4582.0
77.00	540.0
77.90	395.0
79.00	4961.0
79.90	1169.0
80.90	4736.0
81.90	900.0
82.90	165.0
85.90	132.0
87.00	3662.0
88.00	3968.0
90.90	552.0
92.00	3156.0
93.00	5245.0
94.00	13174.0
95.00	98016.0
96.00	6154.0
97.00	242.0
103.90	652.0
104.90	283.0
105.90	657.0
107.00	223.0
108.20	168.0
110.00	141.0
110.90	101.0
112.00	187.0
112.90	190.0
114.90	160.0
115.80	592.0
116.90	1036.0
117.90	491.0
118.90	958.0
123.00	104.0
123.90	128.0
127.90	472.0
128.80	203.0
129.90	558.0
131.10	247.0
134.90	352.0
136.00	102.0
136.90	349.0
139.80	118.0
141.00	1587.0
141.80	260.0
142.90	2047.0
143.90	119.0
145.00	682.0
146.00	212.0
147.90	355.0
150.00	125.0
152.90	108.0
154.00	126.0
154.90	333.0

Instrument :
MSVOA_V
ClientSampleId :
BFB262

156.90	296.0
158.20	120.0
158.80	198.0
160.70	162.0
169.60	128.0
170.80	316.0
171.10	348.0
172.00	953.0
174.00	103576.0
175.00	8206.0
176.00	101056.0
177.00	6346.0
177.80	121.0
199.90	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB262