

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051624\
 Data File : VV035624.D
 Acq On : 16 May 2024 12:44
 Operator : SY/MD
 Sample : P2484-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: May 17 01:57:34 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 17 01:55:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	477775	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	485652	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.182	152	208985	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	140545	38.151	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	76.300%	
7) Chloroethane-d5	1.529	69	132186	48.691	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	97.380%	
11) 1,1-Dichloroethene-d2	2.057	65	64730	40.933	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	81.860%	
21) 2-Butanone-d5	3.790	46	204513	82.257	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	82.260%	
24) Chloroform-d	4.243	84	313586	46.407	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	92.820%	
26) 1,2-Dichloroethane-d4	4.934	65	197601	49.656	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	99.320%	
32) Benzene-d6	4.953	84	603021	44.113	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	88.220%	
36) 1,2-Dichloropropane-d6	5.982	67	207679	48.725	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	97.460%	
41) Toluene-d8	7.240	98	505386	40.616	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	81.240%	
43) trans-1,3-Dichloroprop...	7.551	79	85888	41.345	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	82.700%	
47) 2-Hexanone-d5	8.024	63	137045	69.969	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	69.970%	
56) 1,1,2,2-Tetrachloroeth...	10.149	84	221221	34.062	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	68.120%	
66) 1,2-Dichlorobenzene-d4	11.558	152	208068	50.112	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	100.220%	
Target Compounds						
					Qvalue	
13) Acetone	2.124	43	105537	45.851	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051624\
Data File : VV035624.D
Acq On : 16 May 2024 12:44
Operator : SY/MD
Sample : P2484-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: May 17 01:57:34 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 17 01:55:25 2024
Response via : Initial Calibration

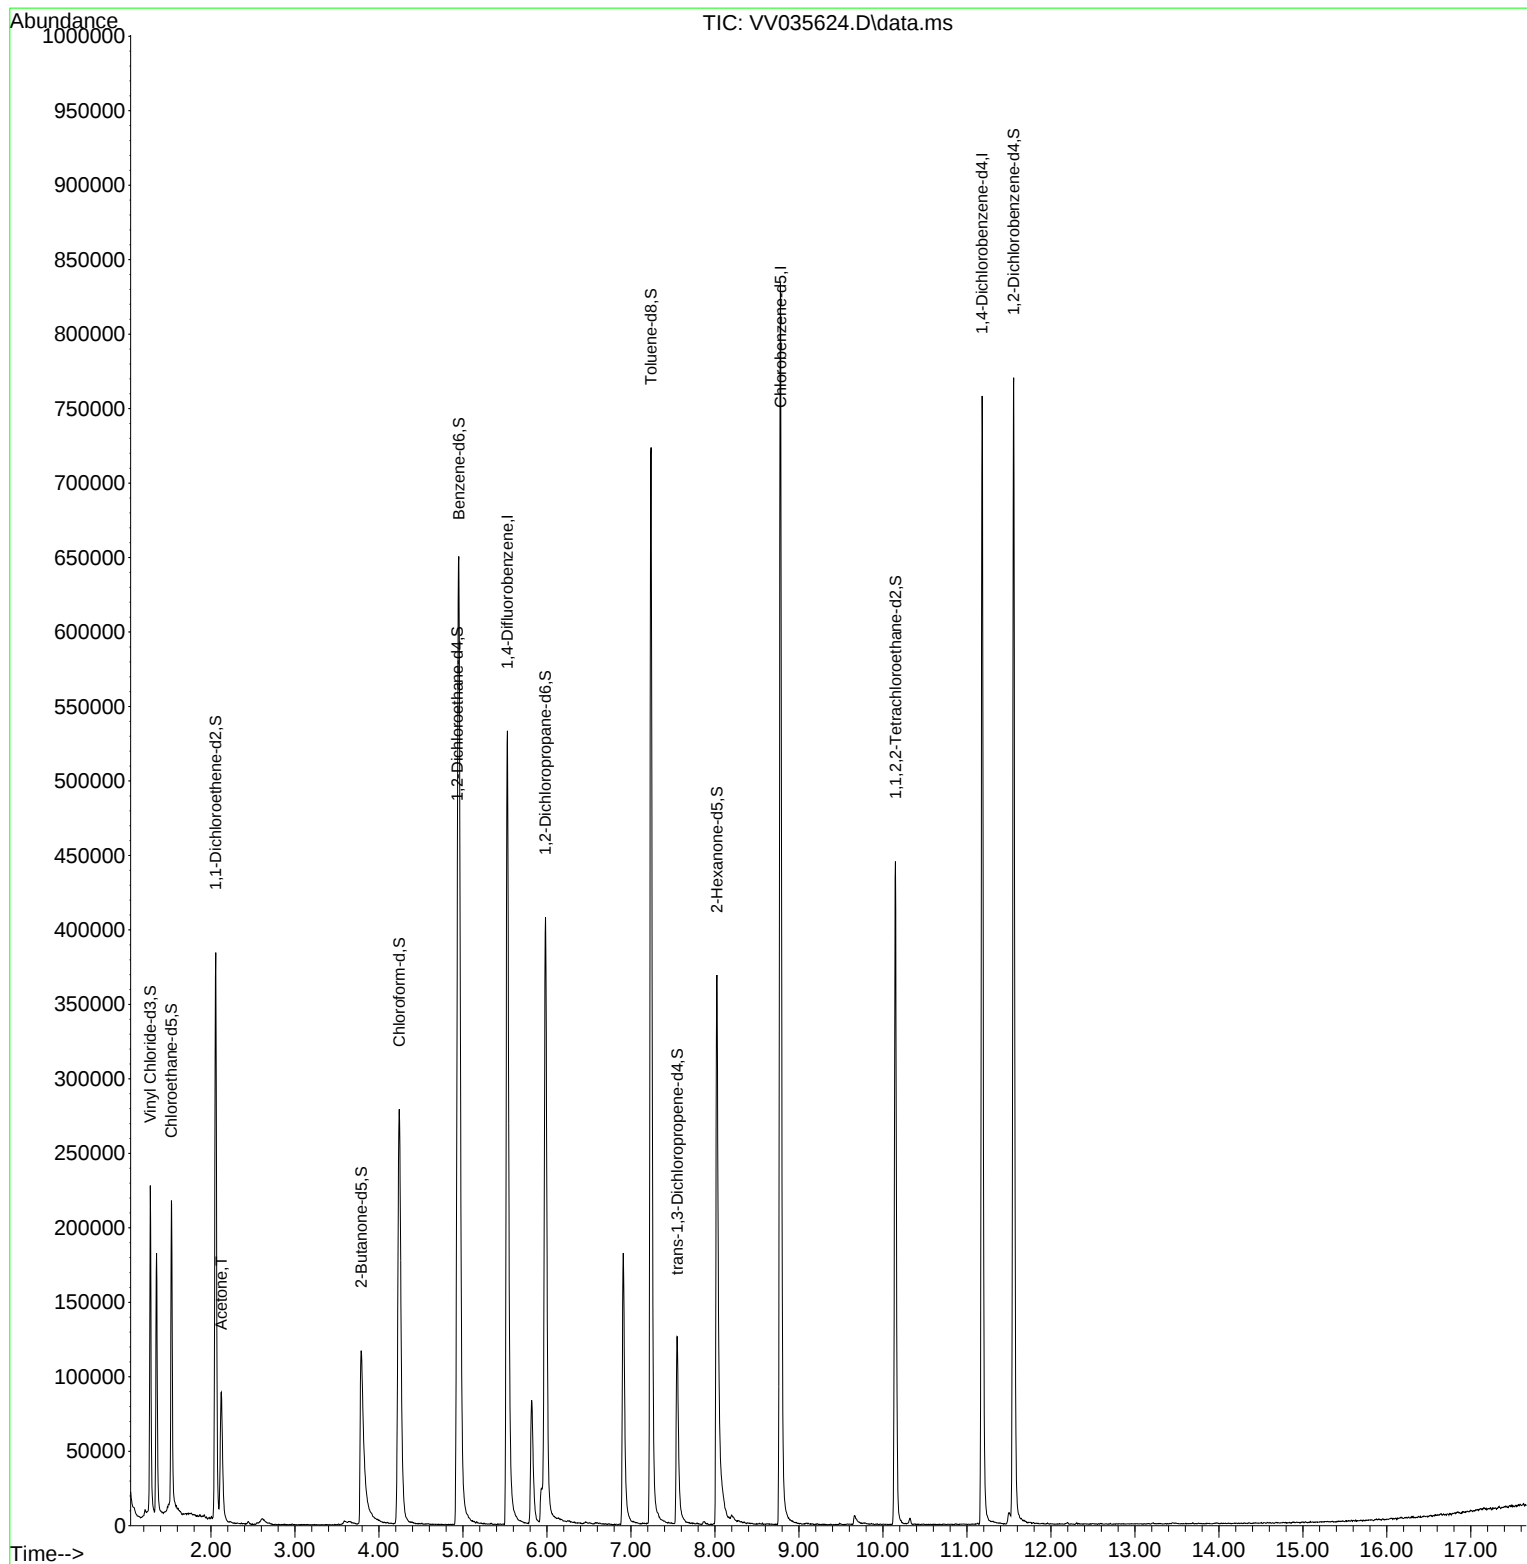

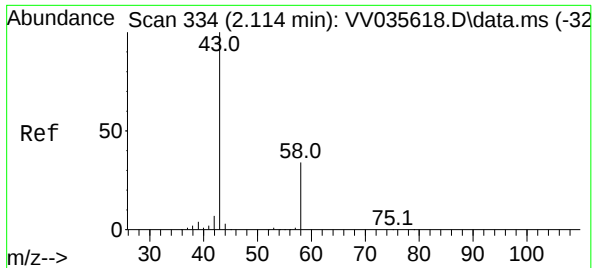

#13
 Acetone
 Concen: 45.851 ug/L
 RT: 2.124 min Scan# 34
 Delta R.T. 0.010 min
 Lab File: VV035624.D
 Acq: 16 May 2024 12:44

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 43 Resp: 105537
 Ion Ratio Lower Upper
 43 100
 58 35.0 0.0 68.8

