

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051624\
 Data File : VV035622.D
 Acq On : 16 May 2024 11:03
 Operator : SY/MD
 Sample : P2483-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHA12

Quant Time: May 17 01:57:04 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 17 01:55:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	439933	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	441247	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	181035	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	138760	40.907	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	81.820%	
7) Chloroethane-d5	1.529	69	127783	51.118	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	102.240%	
11) 1,1-Dichloroethene-d2	2.056	65	64131	44.042	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	88.080%	
21) 2-Butanone-d5	3.789	46	213678	93.336	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	93.340%	
24) Chloroform-d	4.246	84	311920	50.131	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	100.260%	
26) 1,2-Dichloroethane-d4	4.937	65	193398	52.781	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	105.560%	
32) Benzene-d6	4.957	84	597888	48.139	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	96.280%	
36) 1,2-Dichloropropane-d6	5.985	67	205227	52.996	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	106.000%	
41) Toluene-d8	7.239	98	502668	44.463	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	88.920%	
43) trans-1,3-Dichloroprop...	7.551	79	82712	43.823	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	87.640%	
47) 2-Hexanone-d5	8.024	63	142036	79.815	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	79.810%	
56) 1,1,2,2-Tetrachloroeth...	10.149	84	226018	38.302	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	76.600%	
66) 1,2-Dichlorobenzene-d4	11.558	152	200303	55.690	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	111.380%	
Target Compounds					Qvalue	
13) Acetone	2.121	43	12444	5.871	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051624\
Data File : VV035622.D
Acq On : 16 May 2024 11:03
Operator : SY/MD
Sample : P2483-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHA12

Quant Time: May 17 01:57:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 17 01:55:25 2024
Response via : Initial Calibration

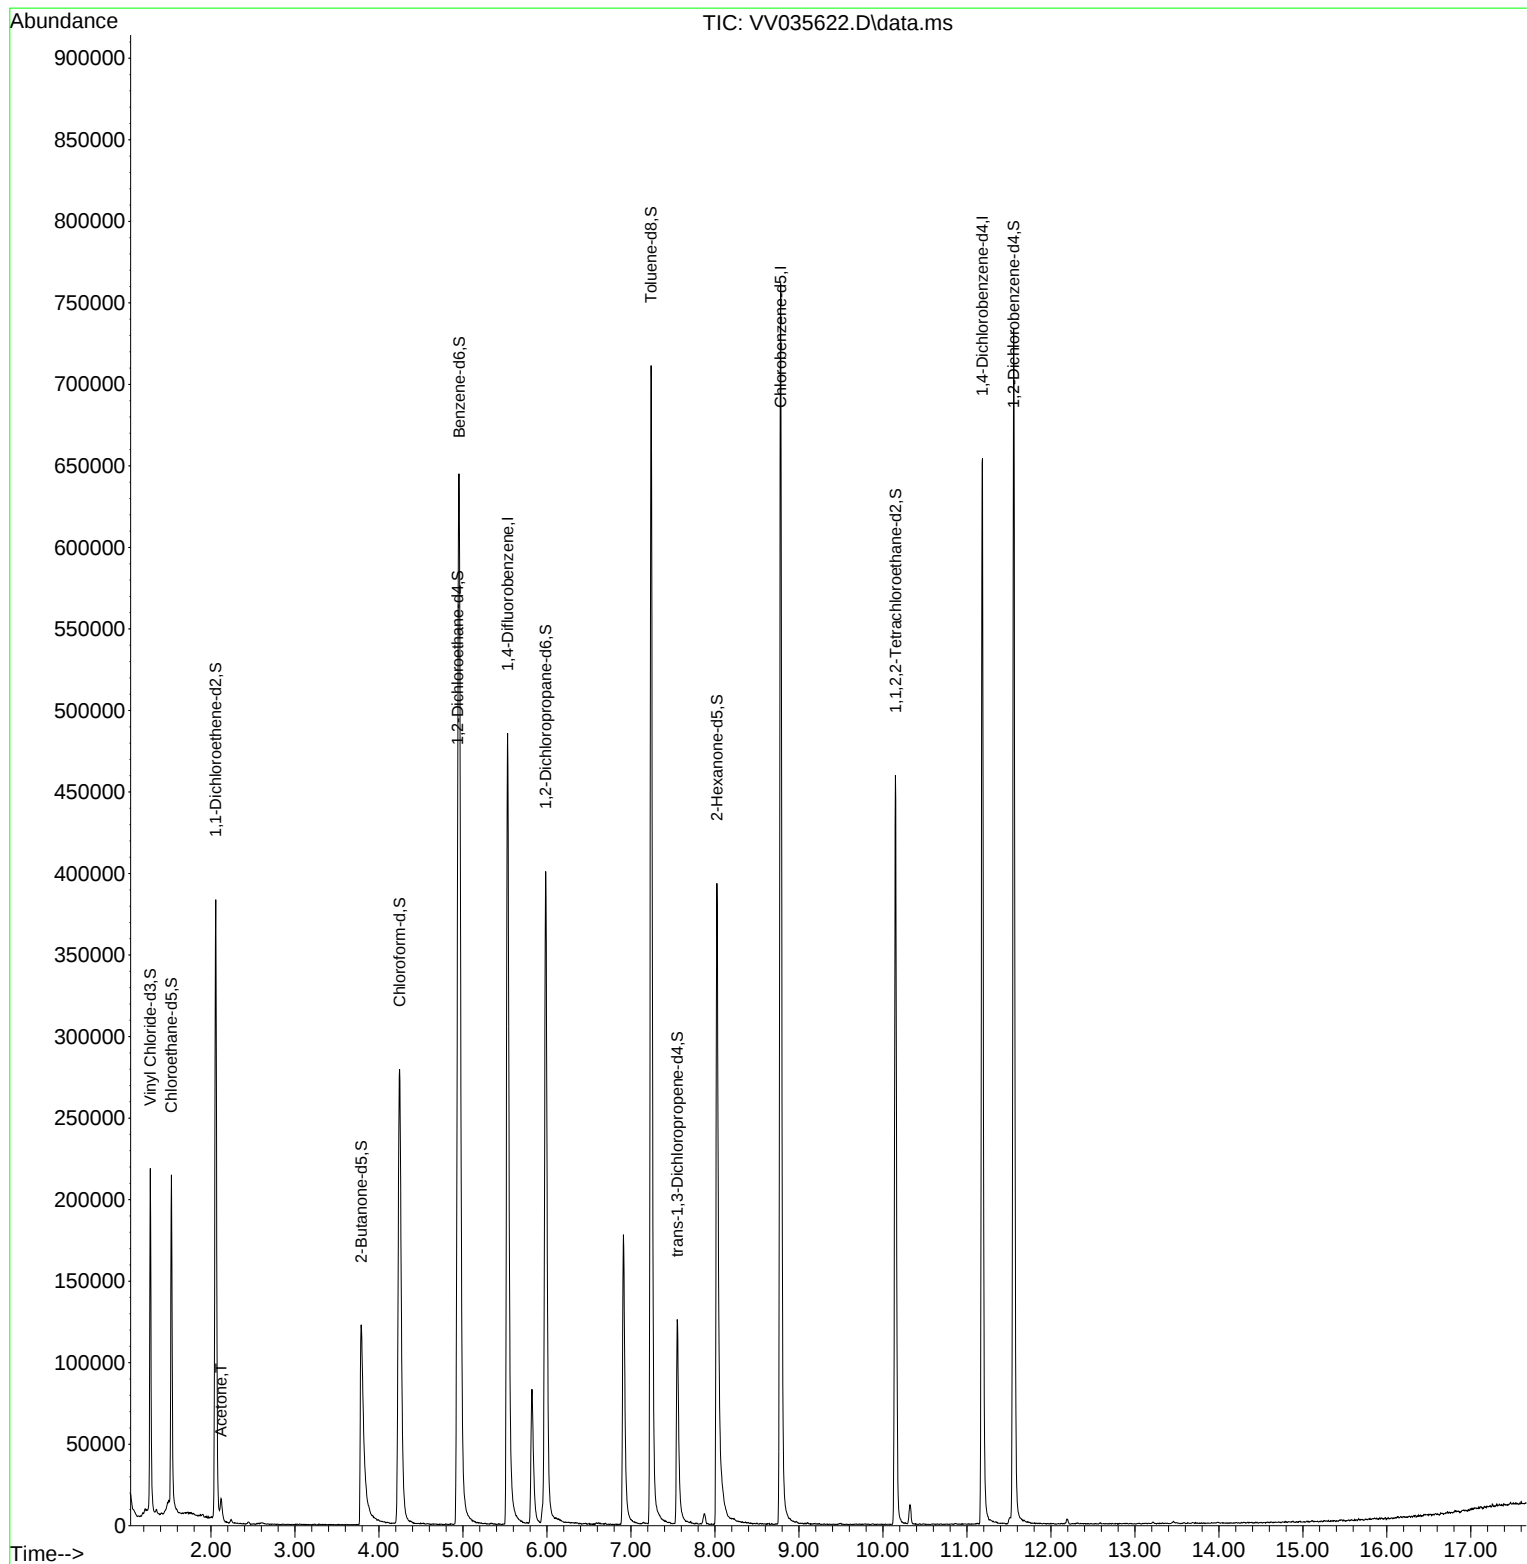

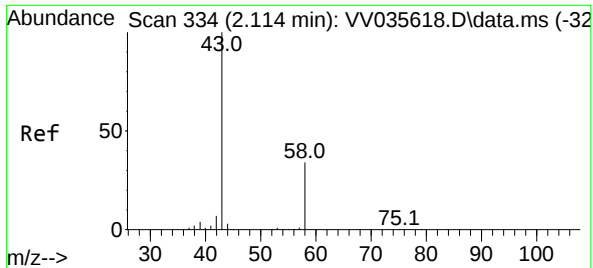

#13
 Acetone
 Concen: 5.871 ug/L
 RT: 2.121 min Scan# 31
 Delta R.T. 0.006 min
 Lab File: VV035622.D
 Acq: 16 May 2024 11:03

Instrument :
 MSVOA_V
 ClientSampleId :
 BHA12

Tgt Ion: 43 Resp: 12444
 Ion Ratio Lower Upper
 43 100
 58 35.6 0.0 68.8

