

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051624\
 Data File : VV035621.D
 Acq On : 16 May 2024 10:39
 Operator : SY/MD
 Sample : P2484-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHA20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

Signal : TIC: VV035621.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	66	74	89	rVB	218826	238317	13.41%	1.726%
2	1.349	90	96	110	rVB	169667	197398	11.11%	1.430%
3	1.529	145	152	180	rVB	207903	268405	15.10%	1.944%
4	2.053	306	315	327	rBV	378359	553530	31.15%	4.009%
5	2.121	328	336	359	rVB	90434	166727	9.38%	1.207%
6	2.439	429	435	446	rVB6	1589	2524	0.14%	0.018%
7	2.558	465	472	477	rBV3	1819	3301	0.19%	0.024%
8	2.719	521	522	527	rVB4	417	293	0.02%	0.002%
9	2.825	552	555	560	rVB2	445	311	0.02%	0.002%
10	2.876	568	571	574	rVB3	486	281	0.02%	0.002%
11	3.111	642	644	649	rVB4	377	298	0.02%	0.002%
12	3.294	697	701	705	rBV2	281	278	0.02%	0.002%
13	3.590	784	793	794	rBV3	1964	2207	0.12%	0.016%
14	3.738	836	839	843	rBV3	424	374	0.02%	0.003%
15	3.786	843	854	898	rBV	121948	383484	21.58%	2.777%
16	4.243	980	996	1027	rBV	286537	747502	42.06%	5.413%
17	4.503	1074	1077	1083	rVB4	408	364	0.02%	0.003%
18	4.545	1088	1090	1095	rVB3	631	487	0.03%	0.004%
19	4.584	1097	1102	1106	rBV3	438	435	0.02%	0.003%
20	4.825	1172	1177	1180	rBV3	445	439	0.02%	0.003%
21	4.950	1196	1216	1254	rBV2	670307	1777225	100.00%	12.870%
22	5.191	1288	1291	1294	rVV4	619	446	0.03%	0.003%
23	5.214	1294	1298	1302	rVB4	559	480	0.03%	0.003%
24	5.320	1326	1331	1333	rBV5	545	475	0.03%	0.003%
25	5.371	1344	1347	1352	rVB3	447	427	0.02%	0.003%
26	5.474	1375	1379	1382	rVB3	346	286	0.02%	0.002%
27	5.529	1382	1396	1434	rBV	514611	1084650	61.03%	7.855%
28	5.764	1466	1469	1476	rBV3	681	702	0.04%	0.005%
29	5.822	1476	1487	1515	rBV2	70956	156749	8.82%	1.135%
30	5.937	1515	1523	1525	rBV2	15454	21989	1.24%	0.159%
31	5.982	1526	1537	1567	rVB	418081	869395	48.92%	6.296%
32	6.346	1648	1650	1653	rBV3	453	320	0.02%	0.002%
33	6.468	1681	1688	1694	rBV4	993	1157	0.07%	0.008%
34	6.593	1722	1727	1729	rBV2	786	832	0.05%	0.006%
35	6.728	1766	1769	1774	rVB2	581	400	0.02%	0.003%
36	6.773	1781	1783	1789	rVB3	579	390	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051624\
 Data File : VV035621.D
 Acq On : 16 May 2024 10:39
 Operator : SY/MD
 Sample : P2484-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHA20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

37	6.838	1800	1803	1806	rVB	383	301	0.02%	0.002%
38	6.908	1815	1825	1864	rBV	187591	370412	20.84%	2.682%
39	7.143	1896	1898	1900	rBV3	821	360	0.02%	0.003%
40	7.185	1907	1911	1912	rBV3	566	442	0.02%	0.003%
41	7.240	1916	1928	1952	rBV	747350	1317466	74.13%	9.541%
42	7.551	2015	2025	2054	rBV	129620	248582	13.99%	1.800%
43	7.873	2113	2125	2134	rBV2	7239	12473	0.70%	0.090%
44	7.912	2134	2137	2142	rVB3	730	615	0.03%	0.004%
45	8.024	2160	2172	2215	rBV	394320	812014	45.69%	5.880%
46	8.397	2284	2288	2290	rBV3	555	439	0.02%	0.003%
47	8.439	2297	2301	2305	rBV3	354	361	0.02%	0.003%
48	8.461	2305	2308	2310	rBV3	556	300	0.02%	0.002%
49	8.600	2348	2351	2353	rBV2	469	287	0.02%	0.002%
50	8.674	2371	2374	2377	rBV3	500	308	0.02%	0.002%
51	8.690	2377	2379	2386	rVB4	536	490	0.03%	0.004%
52	8.738	2391	2394	2396	rBV3	486	317	0.02%	0.002%
53	8.780	2396	2407	2443	rBV	806710	1345401	75.70%	9.743%
54	8.969	2463	2466	2472	rVV5	1014	810	0.05%	0.006%
55	9.047	2487	2490	2495	rBV3	609	482	0.03%	0.003%
56	9.092	2499	2504	2506	rBV2	722	756	0.04%	0.005%
57	9.140	2517	2519	2523	rVB2	375	285	0.02%	0.002%
58	9.220	2538	2544	2546	rBV4	519	397	0.02%	0.003%
59	9.323	2574	2576	2583	rVB3	479	357	0.02%	0.003%
60	9.352	2583	2585	2593	rBV2	259	281	0.02%	0.002%
61	9.481	2622	2625	2628	rVV	460	421	0.02%	0.003%
62	9.500	2628	2631	2635	rVB5	695	461	0.03%	0.003%
63	9.600	2659	2662	2672	rVB4	523	579	0.03%	0.004%
64	9.667	2674	2683	2699	rBV3	5991	14092	0.79%	0.102%
65	9.764	2711	2713	2717	rVB3	585	407	0.02%	0.003%
66	9.821	2728	2731	2735	rBV3	498	305	0.02%	0.002%
67	10.149	2820	2833	2861	rBV	489345	782063	44.00%	5.664%
68	10.323	2876	2887	2898	rVB2	8631	14333	0.81%	0.104%
69	10.535	2950	2953	2956	rBV	509	295	0.02%	0.002%
70	10.625	2974	2981	2984	rBV3	336	349	0.02%	0.003%
71	10.690	2995	3001	3003	rBV3	265	291	0.02%	0.002%
72	10.850	3045	3051	3052	rBV2	317	297	0.02%	0.002%
73	10.863	3052	3055	3057	rBV3	457	368	0.02%	0.003%
74	11.063	3113	3117	3119	rBV2	399	339	0.02%	0.002%
75	11.130	3130	3138	3139	rBV3	1000	932	0.05%	0.007%
76	11.181	3143	3154	3188	rBV	718877	1141343	64.22%	8.265%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051624\
 Data File : VV035621.D
 Acq On : 16 May 2024 10:39
 Operator : SY/MD
 Sample : P2484-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHA20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

77	11.403	3219	3223	3225	rVB3	681	496	0.03%	0.004%
78	11.439	3231	3234	3238	rVB3	566	411	0.02%	0.003%
79	11.513	3245	3257	3258	rBV4	4495	6298	0.35%	0.046%
80	11.558	3260	3271	3300	rVB	776244	1229927	69.20%	8.907%
81	11.892	3373	3375	3380	rBV4	501	407	0.02%	0.003%
82	11.924	3381	3385	3389	rVV2	386	358	0.02%	0.003%
83	12.194	3463	3469	3478	rVB3	1508	2187	0.12%	0.016%
84	12.349	3513	3517	3519	rBV2	447	340	0.02%	0.002%
85	12.461	3548	3552	3557	rVV3	394	443	0.02%	0.003%
86	12.490	3558	3561	3564	rVB2	369	285	0.02%	0.002%
87	12.525	3569	3572	3576	rVB2	470	328	0.02%	0.002%
88	12.596	3587	3594	3597	rBV2	1140	1281	0.07%	0.009%
89	12.763	3642	3646	3652	rVB2	323	308	0.02%	0.002%
90	12.812	3659	3661	3665	rVB2	461	331	0.02%	0.002%
91	13.210	3777	3785	3795	rVB4	1889	3195	0.18%	0.023%
92	13.336	3821	3824	3828	rBV2	441	310	0.02%	0.002%
93	13.397	3837	3843	3846	rBV3	461	482	0.03%	0.003%
94	13.455	3855	3861	3874	rVB3	2955	4359	0.25%	0.032%
95	13.683	3927	3932	3934	rBV3	1507	1421	0.08%	0.010%
96	14.030	4038	4040	4044	rVB	610	304	0.02%	0.002%
97	14.374	4145	4147	4151	rVB3	482	343	0.02%	0.002%
98	14.468	4172	4176	4179	rBV	669	548	0.03%	0.004%
99	14.490	4179	4183	4184	rBV	494	296	0.02%	0.002%
100	14.757	4264	4266	4268	rBV3	628	380	0.02%	0.003%




Sum of corrected areas: 13808727

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051624\
Data File : VV035621.D
Acq On : 16 May 2024 10:39
Operator : SY/MD
Sample : P2484-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHA20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

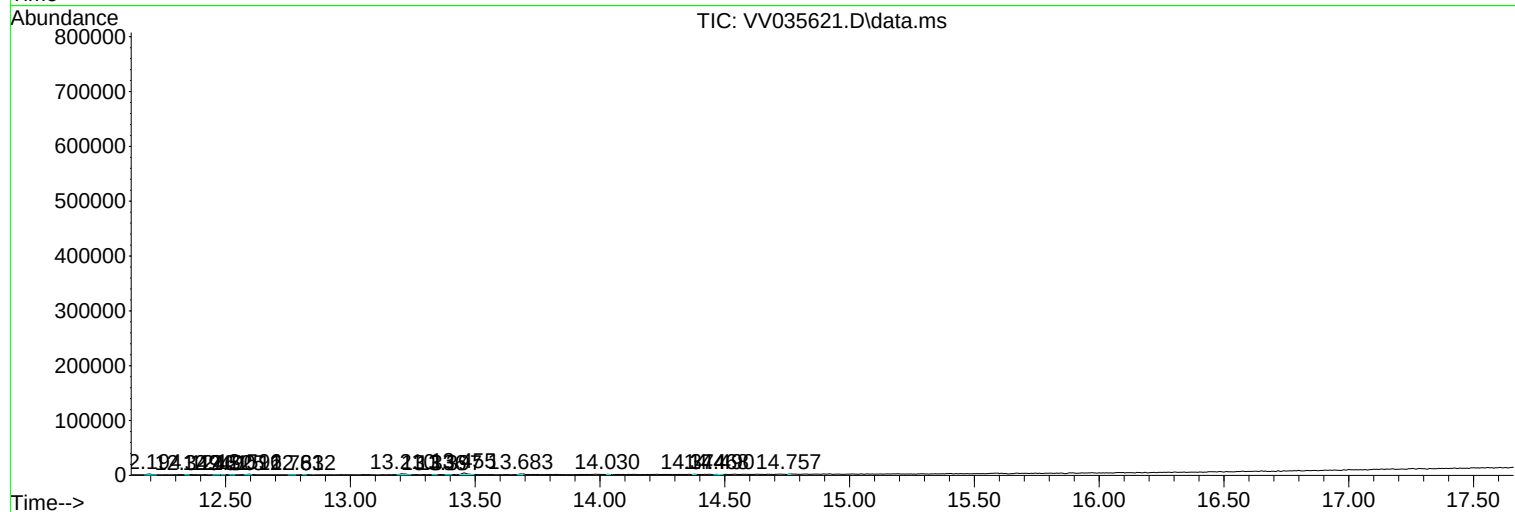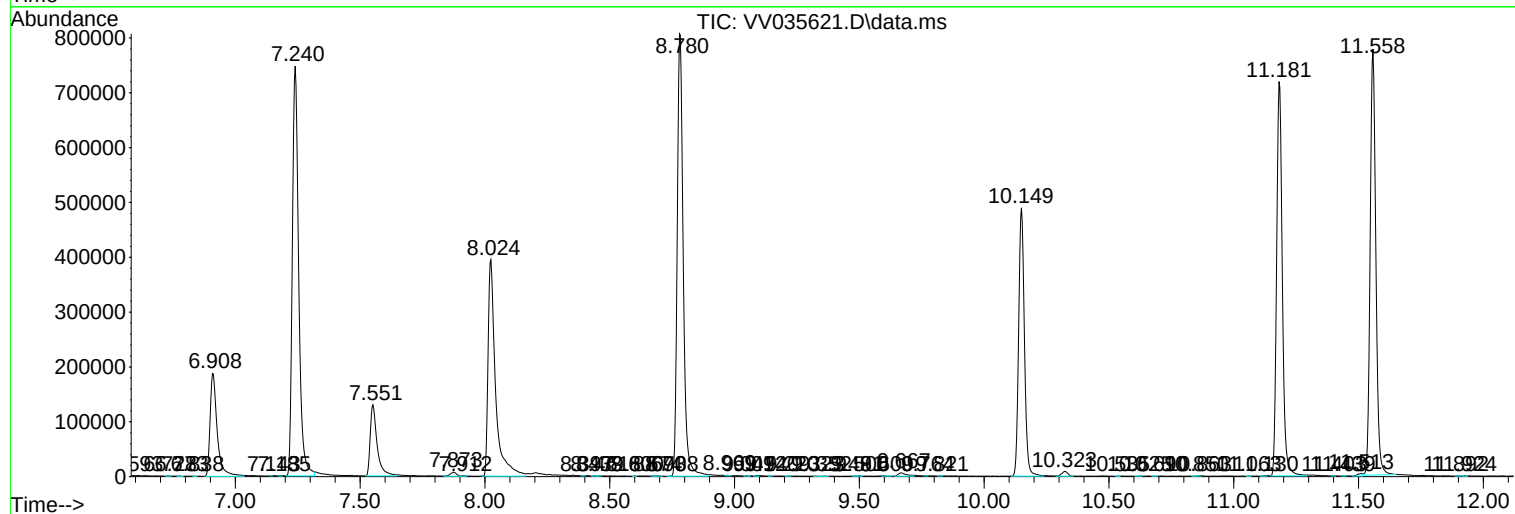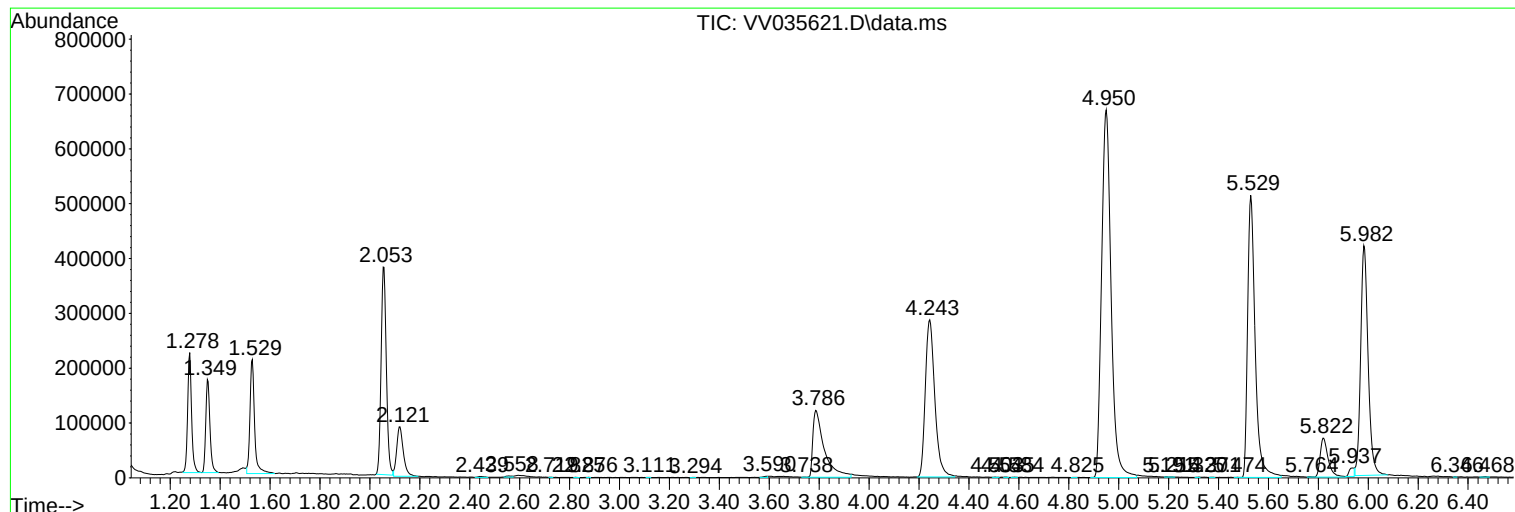

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051624\
Data File : VV035621.D
Acq On : 16 May 2024 10:39
Operator : SY/MD
Sample : P2484-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHA20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051624\
Data File : VV035621.D
Acq On : 16 May 2024 10:39
Operator : SY/MD
Sample : P2484-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHA20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------