

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051624\
 Data File : VV035622.D
 Acq On : 16 May 2024 11:03
 Operator : SY/MD
 Sample : P2483-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHA12

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

Signal : TIC: VV035622.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	91	rVB	210810	227143	13.08%	1.765%
2	1.529	145	152	171	rVB	205255	243297	14.01%	1.890%
3	2.056	306	316	330	rBV	378176	544856	31.38%	4.233%
4	2.240	365	373	382	rBV2	2300	3433	0.20%	0.027%
5	2.426	427	431	432	rBV3	474	296	0.02%	0.002%
6	2.449	433	438	445	rVB5	1467	2152	0.12%	0.017%
7	2.478	445	447	450	rBV2	258	182	0.01%	0.001%
8	2.548	466	469	471	rBV3	476	323	0.02%	0.003%
9	2.709	515	519	521	rBV2	292	261	0.02%	0.002%
10	2.786	540	543	547	rBV2	305	205	0.01%	0.002%
11	2.847	560	562	566	rBV2	231	178	0.01%	0.001%
12	2.921	583	585	592	rVB	243	207	0.01%	0.002%
13	3.027	615	618	622	rVB2	413	314	0.02%	0.002%
14	3.056	622	627	632	rBV2	397	444	0.03%	0.003%
15	3.117	644	646	649	rVB3	301	164	0.01%	0.001%
16	3.214	672	676	679	rBV	281	225	0.01%	0.002%
17	3.285	695	698	702	rBV3	447	336	0.02%	0.003%
18	3.596	792	795	798	rBV2	357	283	0.02%	0.002%
19	3.613	798	800	806	rVB	175	165	0.01%	0.001%
20	3.670	813	818	821	rBV2	225	243	0.01%	0.002%
21	3.789	846	855	895	rBV	122578	369056	21.26%	2.867%
22	4.246	981	997	1032	rBV	278198	729569	42.02%	5.668%
23	4.497	1073	1075	1079	rBV4	496	223	0.01%	0.002%
24	4.748	1150	1153	1156	rVB	280	188	0.01%	0.001%
25	4.799	1164	1169	1170	rBV	344	258	0.01%	0.002%
26	4.838	1178	1181	1184	rBV2	290	217	0.01%	0.002%
27	4.850	1184	1185	1188	rBV	345	191	0.01%	0.001%
28	4.953	1201	1217	1266	rBV2	644193	1736267	100.00%	13.489%
29	5.326	1330	1333	1335	rBV2	497	336	0.02%	0.003%
30	5.429	1363	1365	1367	rVB2	422	177	0.01%	0.001%
31	5.477	1376	1380	1381	rBV2	262	178	0.01%	0.001%
32	5.532	1386	1397	1428	rBV	485071	1013523	58.37%	7.874%
33	5.821	1476	1487	1511	rBV2	82026	175781	10.12%	1.366%
34	5.985	1519	1538	1571	rBV	399370	859634	49.51%	6.679%
35	6.391	1661	1664	1667	rBV4	601	448	0.03%	0.003%
36	6.429	1673	1676	1678	rBV3	391	243	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051624\
 Data File : VV035622.D
 Acq On : 16 May 2024 11:03
 Operator : SY/MD
 Sample : P2483-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHA12

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

37	6.493	1693	1696	1700	rBV2	300	260	0.01%	0.002%
38	6.564	1716	1718	1720	rVB2	416	195	0.01%	0.002%
39	6.590	1720	1726	1728	rBV4	897	876	0.05%	0.007%
40	6.632	1737	1739	1743	rVB3	659	425	0.02%	0.003%
41	6.696	1755	1759	1764	rVB3	725	612	0.04%	0.005%
42	6.757	1775	1778	1783	rVB3	336	266	0.02%	0.002%
43	6.786	1783	1787	1793	rVB3	308	305	0.02%	0.002%
44	6.815	1793	1796	1799	rBV3	407	353	0.02%	0.003%
45	6.911	1815	1826	1853	rBV	177674	347598	20.02%	2.701%
46	7.239	1917	1928	1967	rBV	710471	1290207	74.31%	10.024%
47	7.551	2016	2025	2057	rBV	125078	239090	13.77%	1.858%
48	7.773	2090	2094	2096	rBV3	537	356	0.02%	0.003%
49	7.873	2114	2125	2134	rBV	6442	11910	0.69%	0.093%
50	8.024	2163	2172	2223	rBV	392984	821678	47.32%	6.384%
51	8.538	2330	2332	2337	rVB3	510	418	0.02%	0.003%
52	8.564	2338	2340	2345	rVB3	390	248	0.01%	0.002%
53	8.632	2358	2361	2365	rBV4	404	404	0.02%	0.003%
54	8.680	2372	2376	2380	rVB2	493	393	0.02%	0.003%
55	8.725	2388	2390	2395	rVB4	390	263	0.02%	0.002%
56	8.783	2396	2408	2438	rBV	760837	1264683	72.84%	9.826%
57	9.072	2496	2498	2503	rVB2	454	202	0.01%	0.002%
58	9.101	2503	2507	2509	rBV3	751	618	0.04%	0.005%
59	9.152	2520	2523	2526	rBV4	222	188	0.01%	0.001%
60	9.191	2532	2535	2537	rBV3	410	194	0.01%	0.002%
61	9.243	2549	2551	2555	rVB3	512	308	0.02%	0.002%
62	9.297	2566	2568	2574	rVB2	434	351	0.02%	0.003%
63	9.333	2574	2579	2580	rBV3	229	190	0.01%	0.001%
64	9.361	2583	2588	2593	rBV3	376	382	0.02%	0.003%
65	9.407	2599	2602	2605	rBV2	320	200	0.01%	0.002%
66	9.480	2620	2625	2626	rBV2	480	352	0.02%	0.003%
67	9.490	2626	2628	2629	rVV2	581	289	0.02%	0.002%
68	9.554	2644	2648	2650	rBV2	205	177	0.01%	0.001%
69	9.570	2650	2653	2657	rVB2	243	189	0.01%	0.001%
70	9.715	2694	2698	2700	rBV2	233	177	0.01%	0.001%
71	9.757	2709	2711	2716	rBV	209	185	0.01%	0.001%
72	10.030	2794	2796	2799	rVB	333	166	0.01%	0.001%
73	10.149	2821	2833	2857	rBV	459578	731275	42.12%	5.681%
74	10.323	2877	2887	2898	rVB3	11898	20098	1.16%	0.156%
75	10.365	2898	2900	2906	rVV3	374	351	0.02%	0.003%
76	10.390	2906	2908	2912	rVB3	472	282	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051624\
 Data File : VV035622.D
 Acq On : 16 May 2024 11:03
 Operator : SY/MD
 Sample : P2483-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHA12

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

77	10.435	2920	2922	2926	rVB	345	177	0.01%	0.001%
78	10.484	2933	2937	2942	rBV2	331	350	0.02%	0.003%
79	10.863	3048	3055	3056	rBV3	581	583	0.03%	0.005%
80	10.940	3076	3079	3083	rBV	447	300	0.02%	0.002%
81	11.014	3098	3102	3103	rBV2	331	201	0.01%	0.002%
82	11.185	3143	3155	3180	rBV	653520	1040186	59.91%	8.081%
83	11.513	3248	3257	3260	rBV7	3658	5950	0.34%	0.046%
84	11.558	3260	3271	3300	rVB	731489	1165058	67.10%	9.052%
85	11.869	3367	3368	3377	rVB2	520	477	0.03%	0.004%
86	12.123	3443	3447	3451	rBV2	514	530	0.03%	0.004%
87	12.146	3452	3454	3458	rVV2	466	335	0.02%	0.003%
88	12.168	3458	3461	3463	rVV3	742	540	0.03%	0.004%
89	12.191	3463	3468	3481	rVB4	3182	4940	0.28%	0.038%
90	12.448	3546	3548	3551	rVB	363	195	0.01%	0.002%
91	12.577	3584	3588	3590	rBV2	537	375	0.02%	0.003%
92	12.590	3590	3592	3597	rVB2	806	580	0.03%	0.005%
93	12.702	3624	3627	3633	rBV	399	444	0.03%	0.003%
94	12.734	3633	3637	3639	rBV3	444	299	0.02%	0.002%
95	12.815	3659	3662	3663	rBV3	447	218	0.01%	0.002%
96	13.275	3799	3805	3807	rBV2	414	450	0.03%	0.003%
97	13.628	3913	3915	3919	rBV4	445	314	0.02%	0.002%
98	13.725	3942	3945	3949	rVB2	668	412	0.02%	0.003%
99	13.747	3950	3952	3957	rBV2	430	276	0.02%	0.002%
100	14.268	4112	4114	4119	rBV3	559	420	0.02%	0.003%


Sum of corrected areas: 12871320

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051624\
Data File : VV035622.D
Acq On : 16 May 2024 11:03
Operator : SY/MD
Sample : P2483-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHA12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

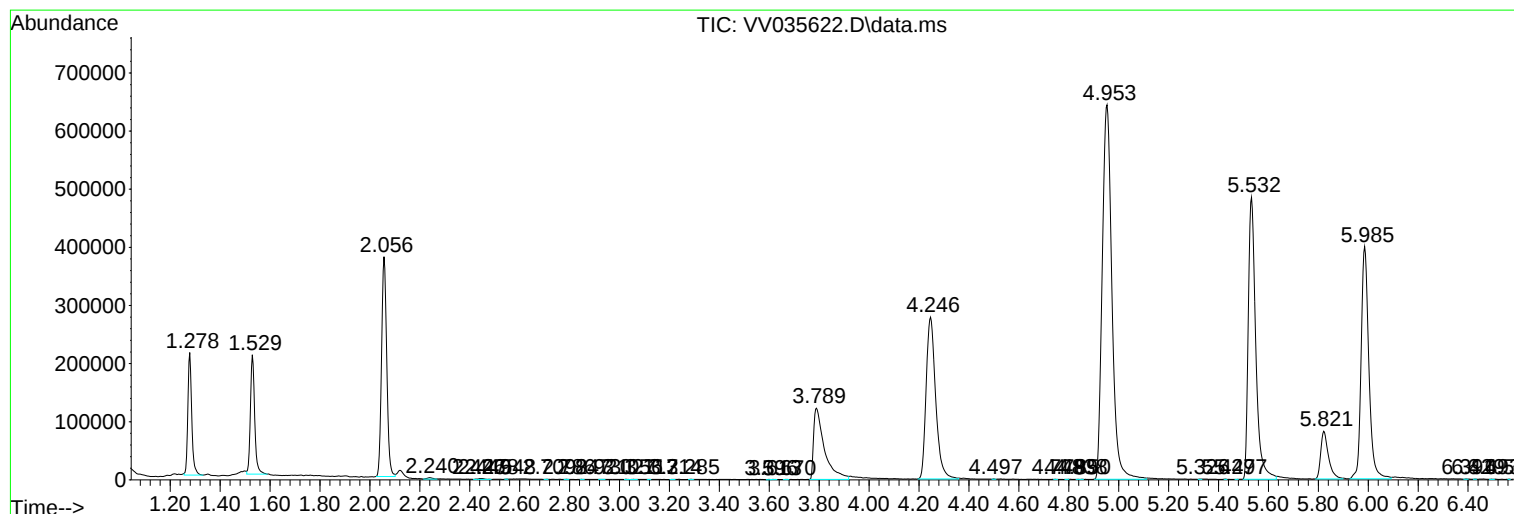

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051624\
Data File : VV035622.D
Acq On : 16 May 2024 11:03
Operator : SY/MD
Sample : P2483-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHA12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051624\
Data File : VV035622.D
Acq On : 16 May 2024 11:03
Operator : SY/MD
Sample : P2483-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHA12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------