

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051624\
 Data File : VV035626.D
 Acq On : 16 May 2024 14:50
 Operator : SY/MD
 Sample : P2483-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

Signal : TIC: VV035626.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	92	rVB	176039	193266	11.85%	1.564%
2	1.529	145	152	168	rVB	183083	211798	12.98%	1.714%
3	2.056	306	316	330	rBV	316583	457814	28.06%	3.704%
4	2.243	365	374	381	rBV3	1712	2887	0.18%	0.023%
5	2.317	393	397	404	rVB6	719	987	0.06%	0.008%
6	2.445	430	437	447	rVB4	2974	5061	0.31%	0.041%
7	2.558	468	472	473	rBV2	396	243	0.01%	0.002%
8	2.606	484	487	489	rBV3	508	365	0.02%	0.003%
9	2.699	511	516	523	rBV5	1188	1310	0.08%	0.011%
10	3.072	629	632	635	rBV	280	249	0.02%	0.002%
11	3.127	645	649	653	rVB3	275	273	0.02%	0.002%
12	3.153	653	657	669	rVB4	453	736	0.05%	0.006%
13	3.507	762	767	771	rVB3	414	409	0.03%	0.003%
14	3.789	846	855	902	rBV	126988	396208	24.28%	3.205%
15	4.243	980	996	1023	rBV	263160	688909	42.23%	5.573%
16	4.503	1074	1077	1083	rVB4	595	577	0.04%	0.005%
17	4.609	1108	1110	1116	rVB3	537	405	0.02%	0.003%
18	4.638	1116	1119	1123	rBV4	468	369	0.02%	0.003%
19	4.828	1174	1178	1181	rVB3	343	305	0.02%	0.002%
20	4.847	1181	1184	1190	rBV4	424	457	0.03%	0.004%
21	4.950	1201	1216	1261	rBV2	606161	1631513	100.00%	13.199%
22	5.243	1305	1307	1313	rVB4	536	328	0.02%	0.003%
23	5.272	1313	1316	1321	rBV5	625	527	0.03%	0.004%
24	5.314	1326	1329	1331	rVB4	766	463	0.03%	0.004%
25	5.375	1345	1348	1352	rVB3	505	301	0.02%	0.002%
26	5.397	1352	1355	1358	rVB2	438	269	0.02%	0.002%
27	5.529	1386	1396	1434	rBV	461763	982561	60.22%	7.949%
28	5.822	1475	1487	1519	rBV3	72949	162321	9.95%	1.313%
29	5.986	1520	1538	1569	rBV	375045	822823	50.43%	6.657%
30	6.365	1654	1656	1660	rVB3	619	329	0.02%	0.003%
31	6.387	1660	1663	1665	rVB4	665	396	0.02%	0.003%
32	6.407	1665	1669	1673	rBV3	507	429	0.03%	0.003%
33	6.452	1680	1683	1687	rVB3	610	406	0.02%	0.003%
34	6.580	1718	1723	1725	rBV3	894	829	0.05%	0.007%
35	6.754	1775	1777	1780	rVB3	425	272	0.02%	0.002%
36	6.912	1814	1826	1856	rBV	170442	336789	20.64%	2.725%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051624\
 Data File : VV035626.D
 Acq On : 16 May 2024 14:50
 Operator : SY/MD
 Sample : P2483-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

37	7.143	1894	1898	1899	rBV3	824	663	0.04%	0.005%
38	7.239	1917	1928	1954	rBV	642849	1147123	70.31%	9.281%
39	7.484	2002	2004	2009	rVB4	797	570	0.03%	0.005%
40	7.551	2015	2025	2056	rBV	117423	234265	14.36%	1.895%
41	7.783	2094	2097	2101	rVB4	451	300	0.02%	0.002%
42	7.834	2109	2113	2116	rBV2	495	471	0.03%	0.004%
43	7.879	2125	2127	2131	rVB2	701	326	0.02%	0.003%
44	7.911	2134	2137	2144	rVB6	1145	1230	0.08%	0.010%
45	8.024	2163	2172	2221	rBV	416854	863219	52.91%	6.984%
46	8.445	2301	2303	2306	rBV3	446	274	0.02%	0.002%
47	8.497	2315	2319	2323	rBV4	536	566	0.03%	0.005%
48	8.645	2363	2365	2368	rVB3	432	280	0.02%	0.002%
49	8.783	2396	2408	2444	rBV	727744	1222953	74.96%	9.894%
50	9.053	2490	2492	2498	rBV2	577	518	0.03%	0.004%
51	9.095	2498	2505	2513	rVV7	1534	2597	0.16%	0.021%
52	9.156	2522	2524	2530	rVB4	383	323	0.02%	0.003%
53	9.182	2530	2532	2534	rVB2	632	293	0.02%	0.002%
54	9.320	2571	2575	2578	rVB3	367	268	0.02%	0.002%
55	9.394	2594	2598	2603	rVB4	332	323	0.02%	0.003%
56	9.493	2620	2629	2634	rBV3	1911	2571	0.16%	0.021%
57	9.532	2634	2641	2645	rBV5	475	754	0.05%	0.006%
58	9.686	2684	2689	2695	rVV3	371	440	0.03%	0.004%
59	9.802	2721	2725	2729	rVB	340	242	0.01%	0.002%
60	9.876	2741	2748	2756	rVB4	1122	1617	0.10%	0.013%
61	9.931	2763	2765	2770	rVB	449	247	0.02%	0.002%
62	9.969	2770	2777	2782	rBV2	327	468	0.03%	0.004%
63	10.005	2783	2788	2792	rBV2	223	245	0.02%	0.002%
64	10.149	2821	2833	2864	rBV	478579	759361	46.54%	6.143%
65	10.326	2883	2888	2895	rVB4	1262	1594	0.10%	0.013%
66	10.445	2923	2925	2929	rBV	410	341	0.02%	0.003%
67	10.481	2929	2936	2937	rBV4	922	758	0.05%	0.006%
68	10.718	3007	3010	3015	rVB2	305	287	0.02%	0.002%
69	10.825	3039	3043	3045	rBV	343	244	0.01%	0.002%
70	10.860	3049	3054	3067	rVB4	1826	2847	0.17%	0.023%
71	10.924	3067	3074	3077	rBV2	217	276	0.02%	0.002%
72	10.963	3083	3086	3091	rVB2	392	291	0.02%	0.002%
73	11.027	3101	3106	3111	rBV3	387	456	0.03%	0.004%
74	11.127	3129	3137	3144	rBV4	3750	5949	0.36%	0.048%
75	11.181	3144	3154	3185	rVV	637205	1006942	61.72%	8.146%
76	11.461	3238	3241	3245	rBV2	413	371	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051624\
 Data File : VV035626.D
 Acq On : 16 May 2024 14:50
 Operator : SY/MD
 Sample : P2483-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

77	11.513	3250	3257	3259	rBV2	3028	3558	0.22%	0.029%
78	11.558	3260	3271	3297	rVB	672268	1079489	66.16%	8.733%
79	11.860	3363	3365	3368	rVB3	498	251	0.02%	0.002%
80	12.050	3421	3424	3427	rBV4	398	244	0.01%	0.002%
81	12.191	3464	3468	3471	rBV2	456	333	0.02%	0.003%
82	12.252	3483	3487	3488	rBV	397	319	0.02%	0.003%
83	12.281	3493	3496	3498	rBV	449	250	0.02%	0.002%
84	12.300	3500	3502	3508	rVB3	409	304	0.02%	0.002%
85	12.368	3515	3523	3532	rVB6	1803	3034	0.19%	0.025%
86	12.416	3532	3538	3541	rBV	493	515	0.03%	0.004%
87	12.480	3555	3558	3563	rVB2	606	499	0.03%	0.004%
88	12.587	3584	3591	3605	rVB3	5757	8668	0.53%	0.070%
89	12.744	3637	3640	3644	rVB2	537	356	0.02%	0.003%
90	13.027	3725	3728	3732	rBV3	353	327	0.02%	0.003%
91	13.069	3737	3741	3744	rBV2	492	334	0.02%	0.003%
92	13.091	3744	3748	3749	rBV2	344	246	0.02%	0.002%
93	13.207	3775	3784	3801	rVB2	10359	17519	1.07%	0.142%
94	13.281	3804	3807	3810	rBV2	443	284	0.02%	0.002%
95	13.442	3847	3857	3877	rBV2	30996	53712	3.29%	0.435%
96	13.683	3923	3932	3947	rBV4	13278	22487	1.38%	0.182%
97	13.754	3951	3954	3958	rBV	456	334	0.02%	0.003%
98	14.043	4041	4044	4047	rBV3	834	585	0.04%	0.005%
99	14.210	4093	4096	4099	rBV3	575	386	0.02%	0.003%
100	14.304	4121	4125	4126	rBV	547	381	0.02%	0.003%




Sum of corrected areas: 12360462

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051624\
Data File : VV035626.D
Acq On : 16 May 2024 14:50
Operator : SY/MD
Sample : P2483-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

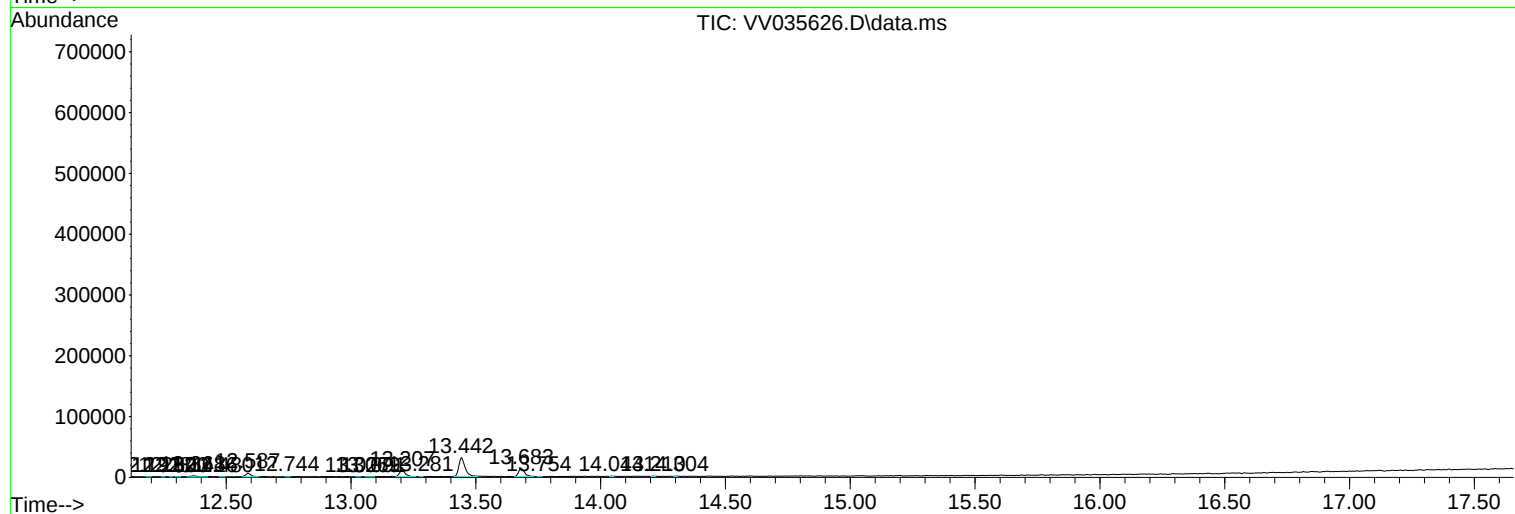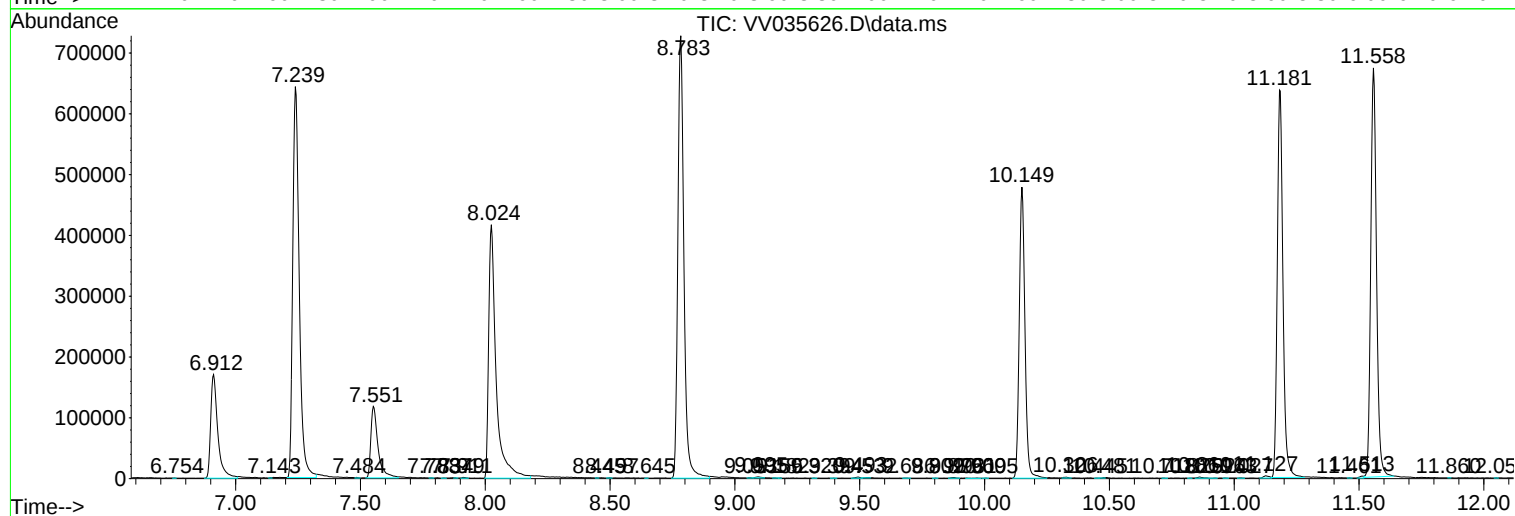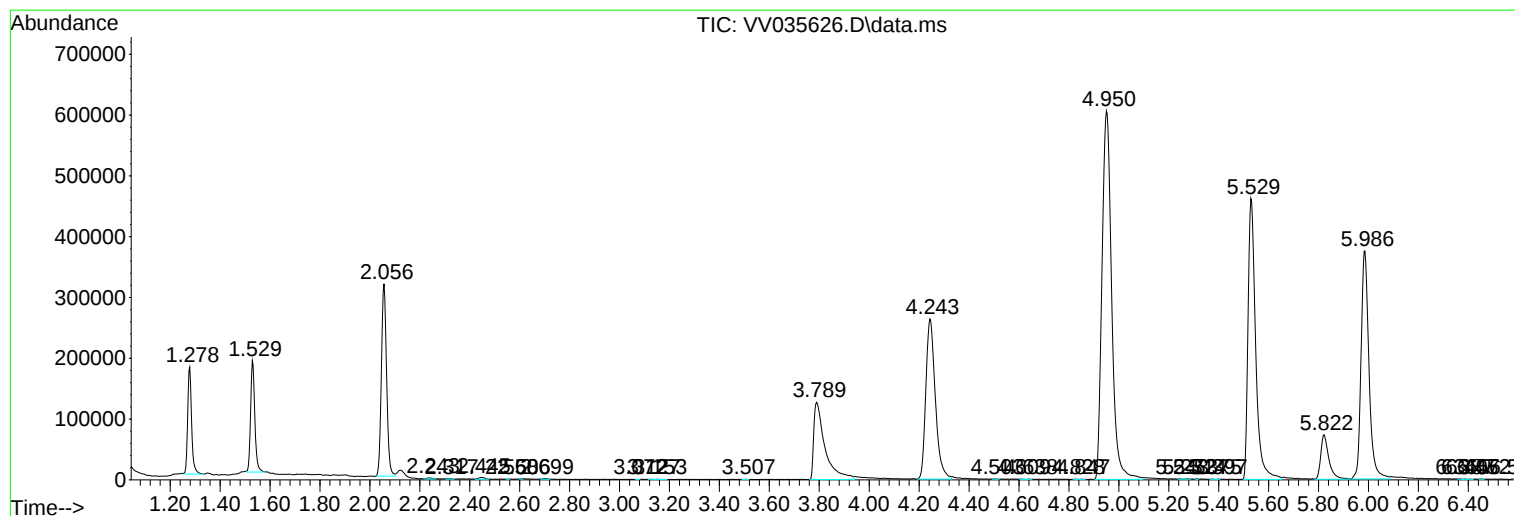

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051624\
Data File : VV035626.D
Acq On : 16 May 2024 14:50
Operator : SY/MD
Sample : P2483-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051624\
Data File : VV035626.D
Acq On : 16 May 2024 14:50
Operator : SY/MD
Sample : P2483-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
