
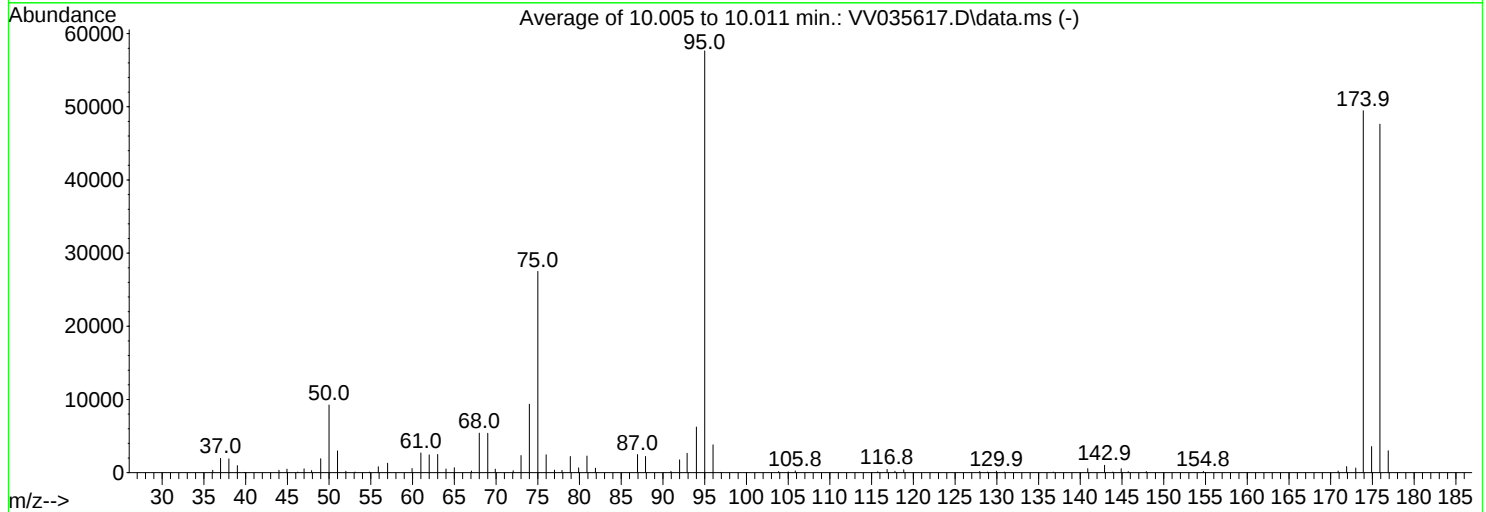


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051624\
Data File : VV035617.D
Acq On : 16 May 2024 08:24
Operator : SY/MD
Sample : BFB303
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB303

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Title : VOC Analysis
Last Update : Fri May 17 01:55:25 2024

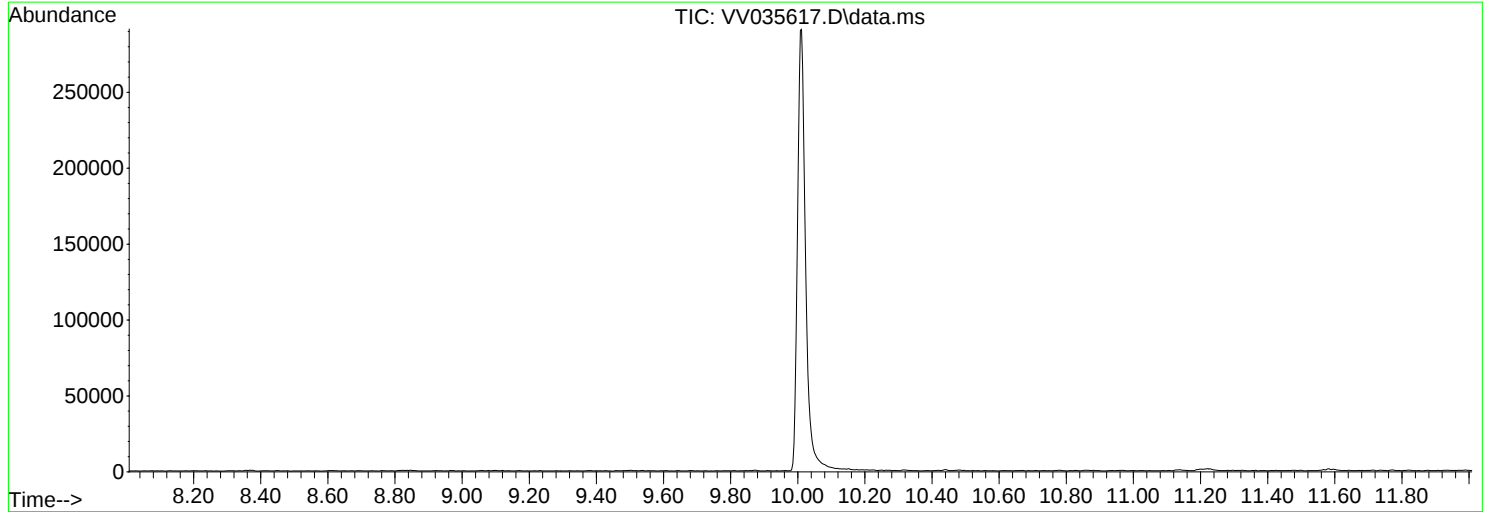

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	9255	PASS
75	95	30	80	47.7	27501	PASS
95	95	100	100	100.0	57645	PASS
96	95	5	9	6.6	3806	PASS
173	174	0.00	2	1.3	629	PASS
174	95	50	120	85.8	49467	PASS
175	174	5	9	7.2	3570	PASS
176	174	95	105	96.3	47621	PASS
177	176	5	10	6.3	2991	PASS

m/z	Abundance
40.00	235.0
44.00	480.0

Instrument :
MSVOA_V
ClientSampleId :
BFB303

m/z	Abundance
36.10	327.0
37.00	1826.0
38.00	1849.0
39.00	923.0
39.80	259.0
44.00	765.0
44.90	414.0
46.20	120.0
47.00	464.0
47.90	269.0
49.00	1758.0
50.00	8880.0
51.00	2866.0
52.00	181.0
53.10	125.0
54.90	136.0
55.90	762.0
57.00	1314.0
60.00	569.0
61.00	2506.0
62.00	2360.0
63.00	2424.0
64.00	435.0
65.00	622.0
67.10	211.0
68.00	5296.0
69.00	4840.0
69.90	444.0
72.10	253.0
73.00	2202.0
74.00	8763.0
75.00	25816.0
76.00	2371.0
77.00	283.0
77.90	289.0
78.90	1913.0
79.90	568.0
80.90	2088.0
81.90	600.0
87.00	2484.0
87.90	2075.0
90.90	172.0
92.00	1576.0
92.90	2617.0
94.00	5679.0
95.00	53616.0
96.00	3580.0
103.90	166.0
105.00	109.0
105.90	236.0
115.80	109.0
116.80	450.0
117.80	151.0
118.90	344.0
128.00	152.0
128.90	139.0
130.00	186.0
140.90	480.0
142.90	927.0
144.90	590.0
145.80	162.0
147.90	110.0
154.70	165.0
170.90	206.0
171.90	739.0
173.00	585.0
173.90	44864.0
174.90	3232.0
175.90	42608.0
176.90	2847.0

Instrument :
MSVOA_V
ClientSampleId :
BFB303

m/z	Abundance
36.10	321.0
37.00	2021.0
38.00	1861.0
39.00	985.0
39.80	299.0
44.00	825.0
44.90	475.0
46.30	121.0
47.00	539.0
47.90	288.0
49.00	1948.0
50.00	9576.0
51.00	3059.0
52.00	214.0
53.10	111.0
54.80	132.0
55.90	850.0
57.00	1311.0
60.00	611.0
61.00	2796.0
62.00	2472.0
63.00	2566.0
64.00	513.0
65.00	723.0
67.10	223.0
68.00	5591.0
69.00	5524.0
69.90	497.0
72.10	279.0
73.00	2423.0
74.00	9769.0
75.00	28504.0
76.00	2519.0
77.00	358.0
77.90	334.0
78.90	2258.0
79.90	681.0
80.90	2333.0
81.90	627.0
87.00	2598.0
87.90	2289.0
90.90	176.0
92.00	1842.0
92.90	2755.0
94.00	6428.0
95.00	59792.0
96.00	3898.0
103.90	145.0
105.00	134.0
105.90	242.0
115.80	145.0
116.90	454.0
117.80	209.0
118.80	403.0
128.00	184.0
128.90	132.0
130.00	194.0
130.90	127.0
136.70	110.0
140.90	599.0
142.90	1041.0
143.90	115.0
144.90	578.0
145.80	173.0
147.90	154.0
154.80	184.0
170.90	245.0
171.90	876.0
173.00	648.0
173.90	51296.0
174.90	3700.0
175.90	49248.0
176.90	3094.0

Instrument :
MSVOA_V
ClientSampleId :
BFB303

m/z	Abundance
36.00	322.0
37.00	2002.0
38.00	1909.0
39.00	994.0
39.80	309.0
44.00	868.0
45.00	536.0
47.00	549.0
47.90	297.0
49.00	1976.0
50.00	9308.0
51.00	3002.0
52.00	212.0
55.90	819.0
57.00	1230.0
59.90	523.0
61.00	2755.0
62.00	2425.0
63.00	2467.0
64.00	565.0
65.00	701.0
67.00	205.0
68.00	5341.0
69.00	5795.0
69.90	489.0
71.90	285.0
73.00	2387.0
74.00	9544.0
75.00	28184.0
76.00	2438.0
77.00	416.0
77.90	328.0
78.90	2445.0
79.90	747.0
80.90	2373.0
81.90	584.0
86.90	2336.0
87.90	2279.0
91.00	185.0
92.00	1831.0
92.90	2557.0
94.00	6564.0
95.00	59528.0
96.00	3940.0
96.90	128.0
103.80	126.0
105.00	112.0
105.80	252.0
115.70	162.0
116.90	441.0
117.80	249.0
118.80	414.0
127.90	214.0
129.90	195.0
130.90	131.0
136.80	128.0
140.90	588.0
142.90	1033.0
143.90	150.0
144.90	473.0
145.70	157.0
147.90	187.0
154.80	192.0
170.90	234.0
171.90	859.0
173.00	653.0
173.90	52240.0
174.90	3779.0
175.90	51008.0
176.90	3033.0

Instrument :
MSVOA_V
ClientSampleId :
BFB303