

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051722\
 Data File : VV025920.D
 Acq On : 17 May 2022 11:06
 Operator : SY/MD
 Sample : VV0517WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK360

Quant Time: May 18 05:57:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 18 05:55:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	208845	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	208774	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	93165	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	75690	4.388	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.800%
7) Chloroethane-d5	1.568	69	70922	4.802	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.000%
11) 1,1-Dichloroethene-d2	2.108	63	128978	3.378	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.600%
20) 2-Butanone-d5	3.902	46	63337	31.708	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	63.420%
24) Chloroform-d	4.346	84	134902	4.788	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.800%
26) 1,2-Dichloroethane-d4	5.031	65	57909	4.847	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.000%
32) Benzene-d6	5.047	84	270309	4.986	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.800%
36) 1,2-Dichloropropane-d6	6.066	67	81275	5.157	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.200%
41) Toluene-d8	7.313	98	225672	4.478	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.600%
43) trans-1,3-Dichloroprop...	7.622	79	19103	3.706	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	74.200%
46) 2-Hexanone-d5	8.088	63	83812	43.793	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.580%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	48244	4.752	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.000%
66) 1,2-Dichlorobenzene-d4	11.622	152	69083	5.208	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.200%
Target Compounds						
16) Methylene chloride	2.510	84	6757	0.332	ug/L	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051722\
Data File : VV025920.D
Acq On : 17 May 2022 11:06
Operator : SY/MD
Sample : VV0517WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK360


Quant Time: May 18 05:57:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 18 05:55:49 2022
Response via : Initial Calibration

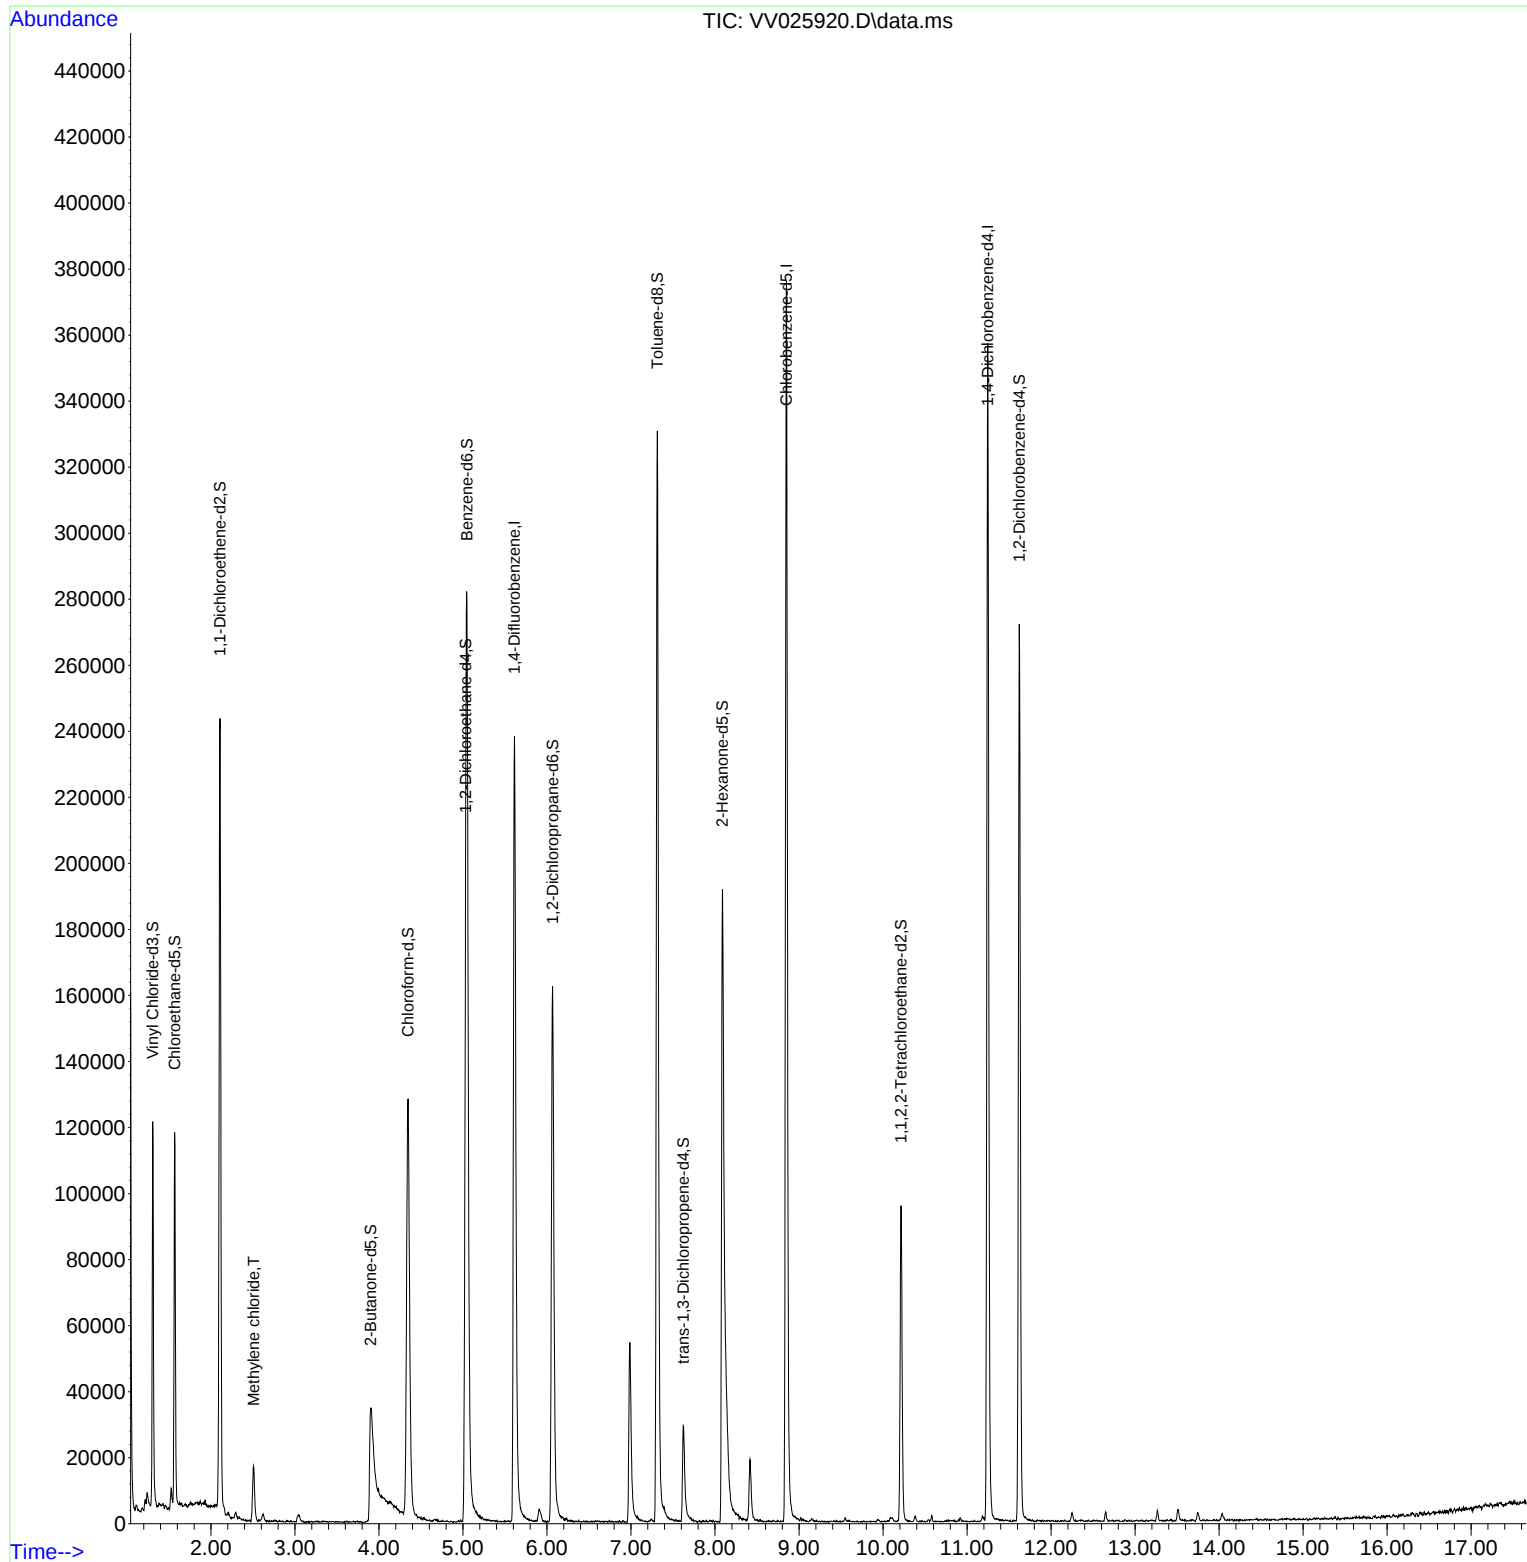

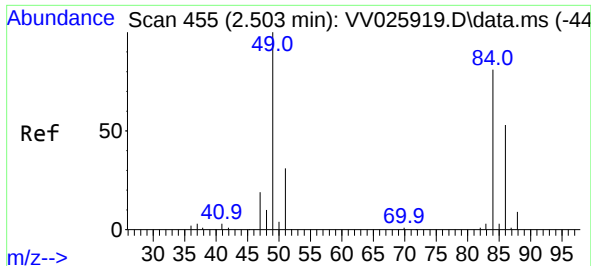

#16
Methylene chloride
Concen: 0.332 ug/L
RT: 2.510 min Scan# 4
Delta R.T. 0.006 min
Lab File: VV025920.D
Acq: 17 May 2022 11:06

Instrument :
MSVOA_V
ClientSampleId :
VBLK360

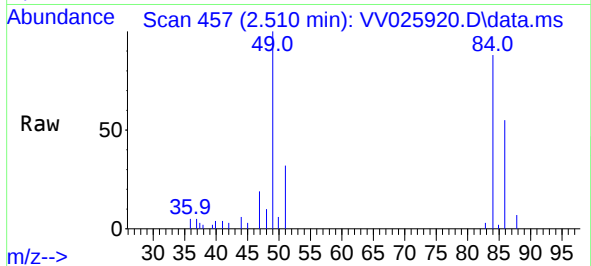

Tgt Ion: 84 Resp: 6757

Ion	Ratio	Lower	Upper
84	100		
86	62.9	45.4	84.2
49	113.7	85.6	159.0

