

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051722\
 Data File : VV025920.D
 Acq On : 17 May 2022 11:06
 Operator : SY/MD
 Sample : VV0517WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK360

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025920.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	59	62	74	rVV2	5139	7985	1.14%	0.141%
2	1.307	75	83	98	rVB	116765	124602	17.75%	2.200%
3	1.526	145	151	157	rBV2	6318	8146	1.16%	0.144%
4	1.568	157	164	178	rVB	113057	126591	18.03%	2.235%
5	2.108	321	332	346	rVB	238724	340394	48.48%	6.009%
6	2.507	446	456	472	rBV2	16894	29062	4.14%	0.513%
7	3.905	880	891	916	rBV3	34087	130208	18.54%	2.298%
8	4.346	1011	1028	1057	rVB2	126166	316449	45.07%	5.586%
9	5.043	1229	1245	1271	rBV2	281732	702180	100.00%	12.395%
10	5.612	1411	1422	1453	rBV	237485	487377	69.41%	8.603%
11	5.905	1505	1513	1528	rBV6	3715	8084	1.15%	0.143%
12	6.066	1546	1563	1591	rBV	162416	341415	48.62%	6.027%
13	6.985	1839	1849	1872	rBV	54497	108823	15.50%	1.921%
14	7.313	1939	1951	1972	rBV	330401	581797	82.86%	10.270%
15	7.622	2039	2047	2073	rBV	28993	58963	8.40%	1.041%
16	8.088	2182	2192	2231	rBV	191516	483471	68.85%	8.534%
17	8.416	2283	2294	2311	rBV2	18423	33284	4.74%	0.588%
18	8.850	2417	2429	2452	rBV	375648	627780	89.40%	11.082%
19	10.214	2842	2853	2871	rBV	95436	155153	22.10%	2.739%
20	11.246	3163	3174	3193	rBV	356499	557368	79.38%	9.839%
21	11.622	3279	3291	3312	rBV	271610	435844	62.07%	7.694%




Sum of corrected areas: 5664976

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051722\
Data File : VV025920.D
Acq On : 17 May 2022 11:06
Operator : SY/MD
Sample : VV0517WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK360

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

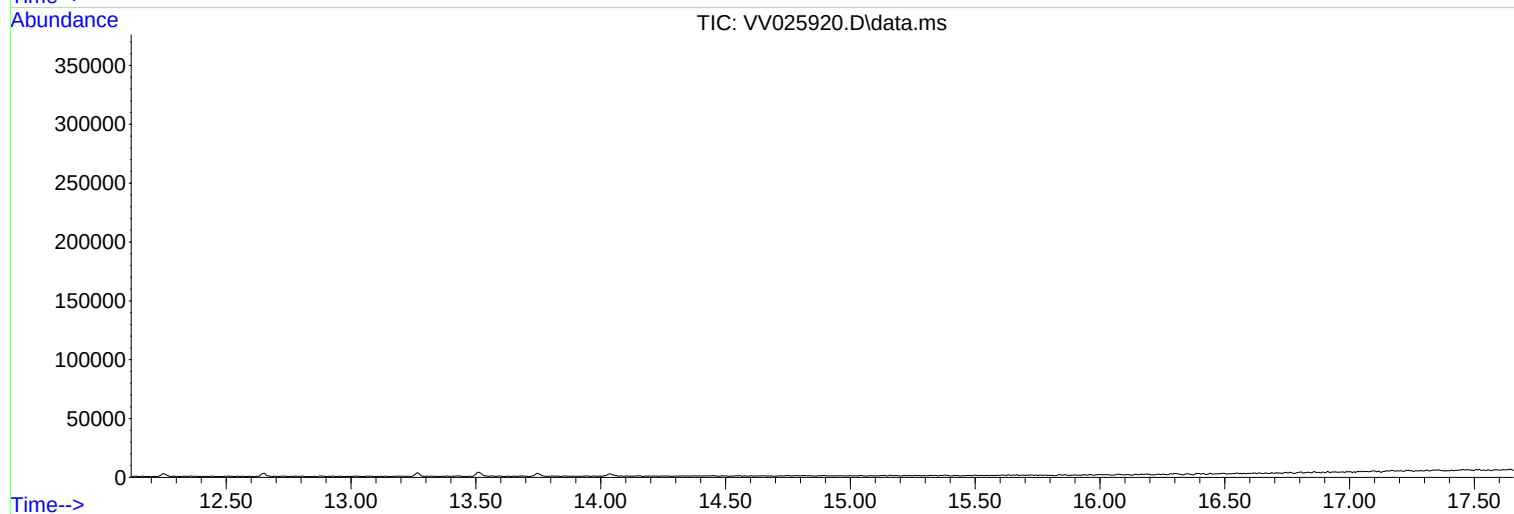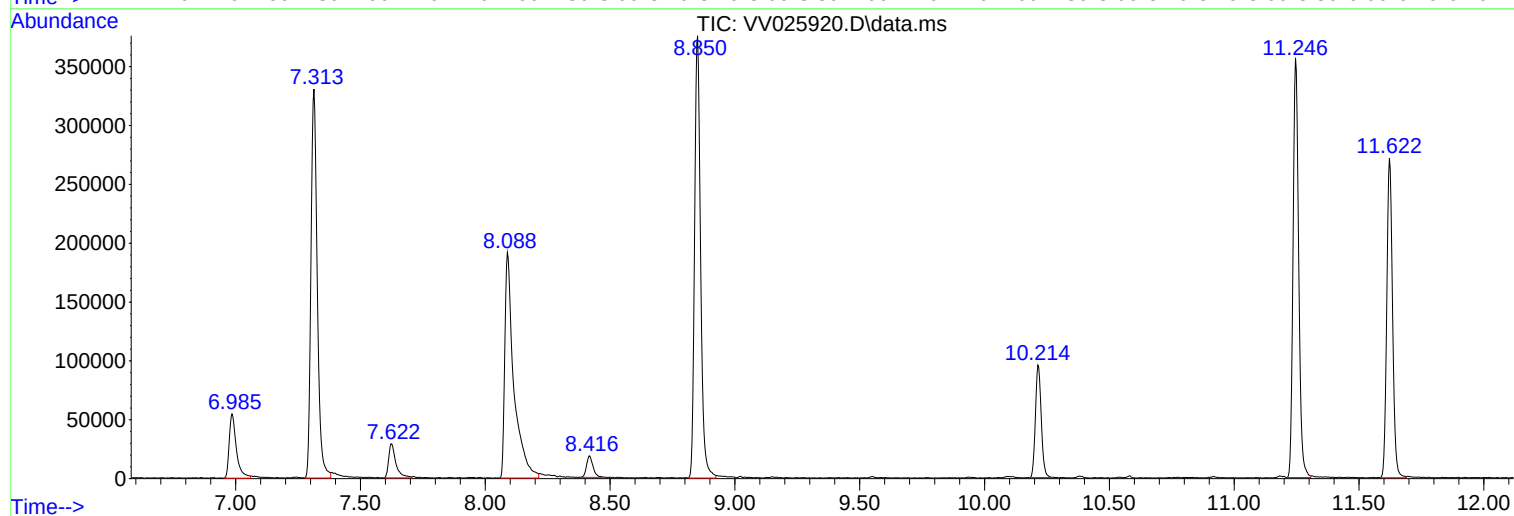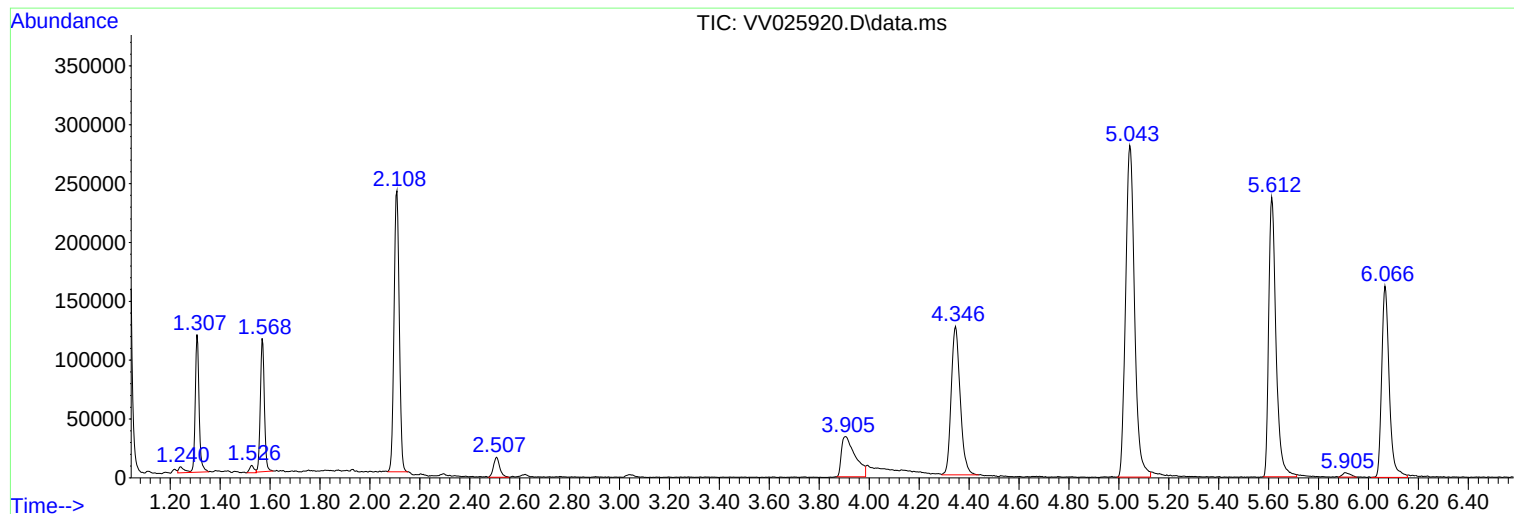

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051722\
Data File : VV025920.D
Acq On : 17 May 2022 11:06
Operator : SY/MD
Sample : VV0517WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK360

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051722\
Data File : VV025920.D
Acq On : 17 May 2022 11:06
Operator : SY/MD
Sample : VV0517WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK360

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc