

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051722\
 Data File : VV025924.D
 Acq On : 17 May 2022 13:05
 Operator : SY/MD
 Sample : N2831-10
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025924.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rBV	114495	119476	18.08%	2.182%
2	1.523	127	150	151	rBV2	14101	38837	5.88%	0.709%
3	1.568	157	164	176	rVB	104752	118985	18.00%	2.173%
4	2.108	323	332	354	rVB	236418	352520	53.34%	6.439%
5	2.510	444	457	472	rBV2	11353	20423	3.09%	0.373%
6	3.908	878	892	939	rBV2	41665	199600	30.20%	3.646%
7	4.346	1011	1028	1050	rBV2	118463	298511	45.16%	5.453%
8	5.043	1227	1245	1273	rBV3	265598	660952	100.00%	12.073%
9	5.613	1408	1422	1454	rBV	214279	446521	67.56%	8.156%
10	6.066	1548	1563	1588	rBV	152101	317910	48.10%	5.807%
11	6.986	1838	1849	1864	rBV	50115	97528	14.76%	1.781%
12	7.314	1939	1951	1974	rBV	311866	545831	82.58%	9.970%
13	7.622	2037	2047	2070	rBV	29025	54911	8.31%	1.003%
14	8.088	2182	2192	2226	rBV	216161	458507	69.37%	8.375%
15	8.416	2284	2294	2305	rBV3	14882	25608	3.87%	0.468%
16	8.850	2418	2429	2450	rBV	346300	579692	87.71%	10.589%
17	10.214	2841	2853	2869	rBV	95063	152927	23.14%	2.793%
18	10.378	2895	2904	2916	rBV4	8246	12623	1.91%	0.231%
19	11.246	3162	3174	3197	rBV	346526	542191	82.03%	9.904%
20	11.622	3280	3291	3310	rBV	269761	423547	64.08%	7.736%
21	12.246	3476	3485	3497	rBV3	4767	7588	1.15%	0.139%


Sum of corrected areas: 5474688

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051722\
Data File : VV025924.D
Acq On : 17 May 2022 13:05
Operator : SY/MD
Sample : N2831-10
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

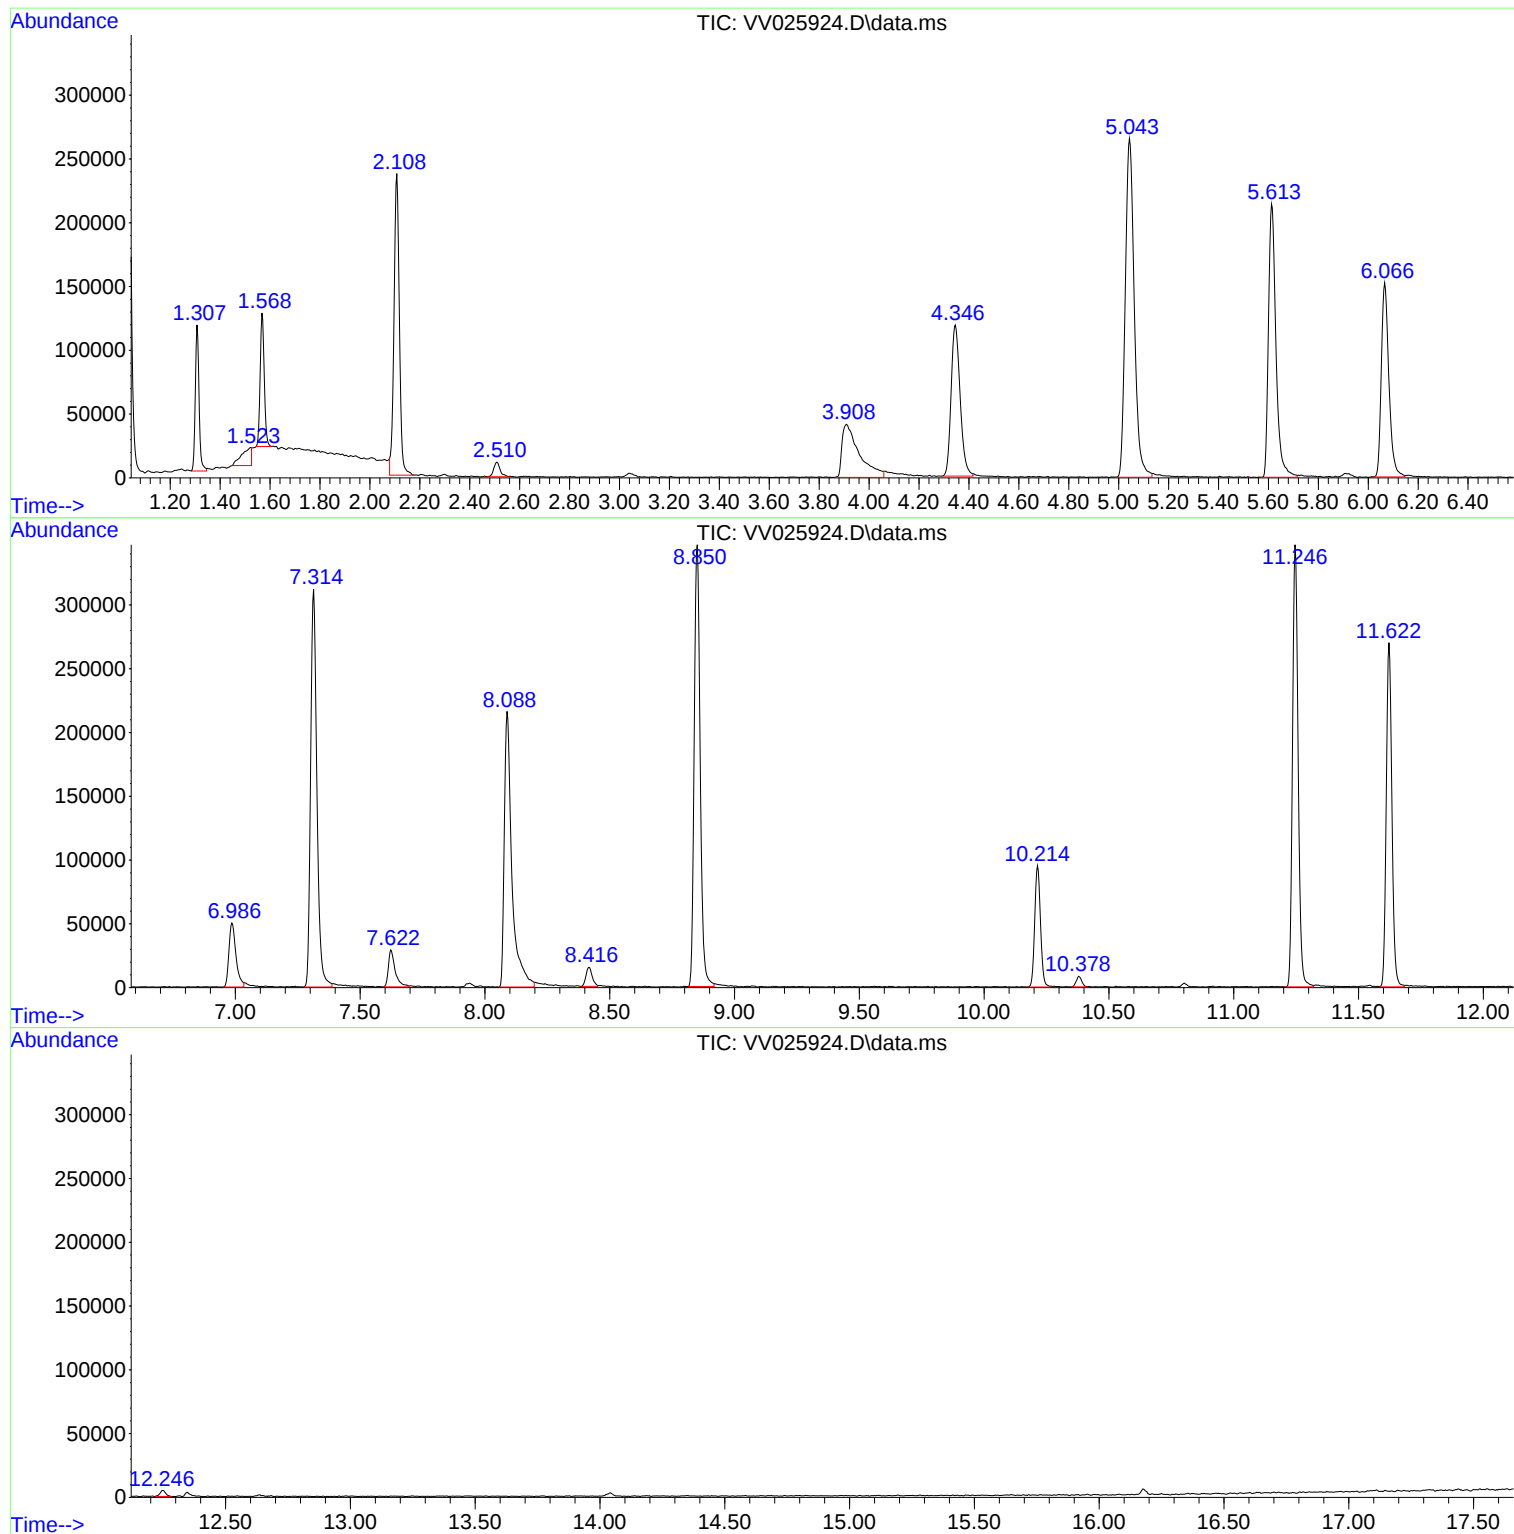

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051722\
Data File : VV025924.D
Acq On : 17 May 2022 13:05
Operator : SY/MD
Sample : N2831-10
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051722\
Data File : VV025924.D
Acq On : 17 May 2022 13:05
Operator : SY/MD
Sample : N2831-10
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc