
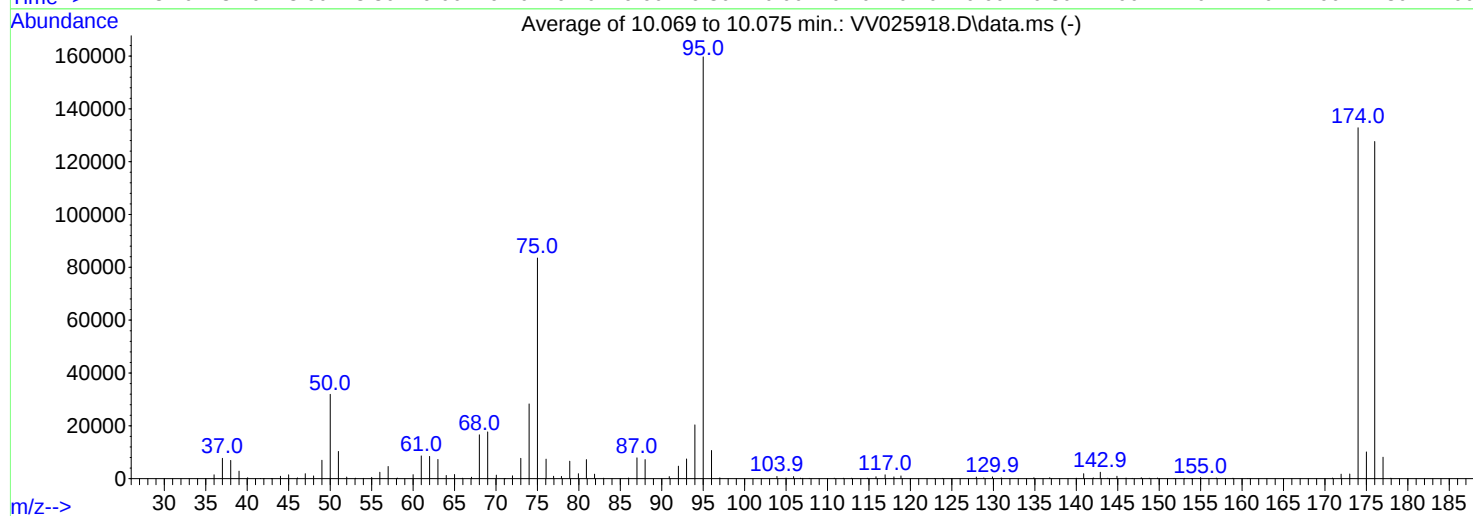


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051722\
 Data File : VV025918.D
 Acq On : 17 May 2022 09:54
 Operator : SY/MD
 Sample : BFB318
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB318

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed May 18 05:55:49 2022

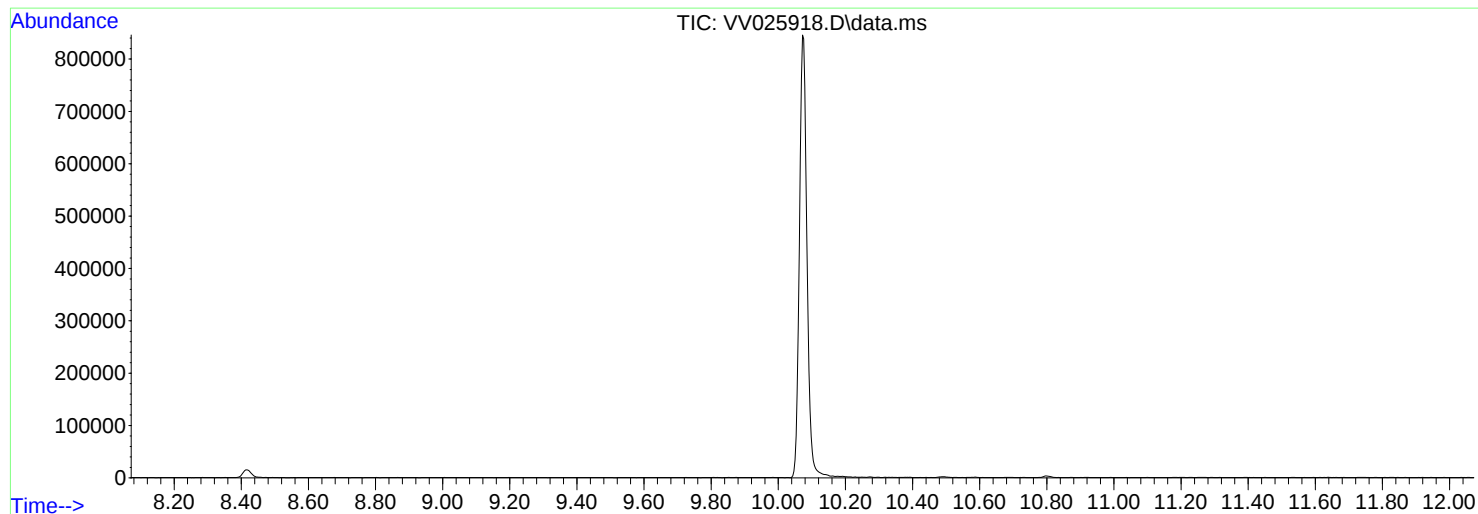

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	31917	PASS
75	95	30	80	52.3	83509	PASS
95	95	100	100	100.0	159680	PASS
96	95	5	9	6.7	10651	PASS
173	174	0.00	2	1.3	1787	PASS
174	95	50	120	83.2	132843	PASS
175	174	5	9	7.6	10090	PASS
176	174	95	105	96.1	127627	PASS
177	176	5	10	6.4	8117	PASS

Scan 2796 (10.030 min): VV025918.D\data.ms
BFB318

m/z	Abundance
39.80	198.0
44.00	358.0

Instrument :
MSVOA_V
ClientSampleId :
BFB318

m/z	Abundance
36.00	1348.0
37.00	7268.0
38.00	6610.0
39.00	2632.0
40.10	402.0
41.60	103.0
44.00	1287.0
45.00	1352.0
46.10	303.0
47.00	1866.0
48.00	1044.0
49.00	6867.0
50.00	30088.0
51.00	9747.0
52.00	573.0
53.10	171.0
54.00	115.0
55.00	525.0
56.00	2368.0
57.00	4356.0
58.10	255.0
60.00	1454.0
61.00	8338.0
62.00	8115.0
63.00	6921.0
64.00	1163.0
65.00	1385.0
65.90	198.0
67.00	529.0
68.00	15525.0
69.00	16744.0
70.00	1226.0
72.00	1032.0
73.00	6864.0
74.00	26680.0
75.00	79456.0
76.10	7178.0
77.00	931.0
77.90	881.0
78.90	6289.0
79.90	1765.0
80.90	6932.0
81.90	1563.0
83.00	161.0
86.00	237.0
87.00	7362.0
88.00	7067.0
90.90	701.0
92.00	4423.0
93.00	7032.0
94.00	19680.0
95.00	149952.0
96.00	10130.0
97.10	303.0
103.90	754.0
105.00	262.0
105.90	747.0
106.70	197.0
107.00	196.0
107.80	113.0
110.80	170.0
111.90	166.0
112.90	209.0
114.80	203.0
115.80	677.0
117.00	1398.0
118.00	605.0
118.90	1029.0
123.90	148.0
128.00	529.0
128.90	254.0
129.90	612.0
131.00	288.0
134.90	325.0
136.80	340.0
140.00	165.0
140.90	1686.0
142.10	228.0
142.90	2420.0
143.80	167.0
144.90	964.0
146.00	243.0
146.70	101.0
147.80	339.0
148.80	146.0
149.80	178.0
151.80	115.0
153.00	115.0
155.00	403.0
156.90	181.0
158.90	168.0
161.00	147.0

Instrument :
MSVOA_V
ClientSampleId :
BFB318

170.90	278.0
172.00	1627.0
173.00	1752.0
174.00	121472.0
175.00	9320.0
176.00	115680.0
177.00	7638.0
177.90	208.0

Instrument :
MSVOA_V
ClientSampleId :
BFB318

m/z	Abundance
36.00	1529.0
37.00	7994.0
38.00	7181.0
39.00	2938.0
40.10	388.0
41.60	108.0
44.00	1310.0
45.00	1482.0
46.10	301.0
47.00	1911.0
48.00	1093.0
49.00	7215.0
50.00	33136.0
51.00	10788.0
52.00	616.0
53.00	175.0
54.00	115.0
55.00	530.0
56.00	2456.0
57.00	4675.0
58.10	266.0
60.00	1623.0
61.00	8904.0
62.00	8727.0
63.00	7491.0
64.00	1205.0
65.00	1651.0
65.90	189.0
67.10	590.0
68.00	17232.0
69.00	18424.0
70.00	1381.0
72.00	1177.0
73.00	7948.0
74.00	29432.0
75.00	86416.0
76.00	7639.0
76.90	968.0
77.90	917.0
78.90	6866.0
80.00	1938.0
80.90	7469.0
81.90	1707.0
83.00	171.0
86.00	307.0
87.00	8221.0
88.00	7467.0
90.90	803.0
92.00	4840.0
93.00	7737.0
94.00	21136.0
95.00	165888.0
96.00	11087.0
97.00	306.0
103.90	936.0
105.00	241.0
105.90	815.0
106.80	199.0
107.00	194.0
107.80	139.0
110.80	190.0
111.90	183.0
112.90	196.0
114.80	221.0
115.80	744.0
116.90	1510.0
118.00	693.0
118.90	1076.0
122.90	110.0
123.90	164.0
128.00	621.0
128.90	310.0
129.90	697.0
131.00	314.0
134.90	359.0
136.80	369.0
140.00	215.0
140.90	1924.0
142.10	307.0
142.90	2493.0
143.80	200.0
144.90	944.0
146.00	281.0
146.70	122.0
147.90	340.0
148.80	185.0
149.80	227.0
151.80	150.0
153.00	125.0
153.90	101.0
155.00	426.0
156.90	217.0

Instrument :
MSVOA_V
ClientSampleId :
BFB318

158.90	193.0
160.90	136.0
170.90	256.0
171.90	1756.0
173.00	1826.0
174.00	137664.0
175.00	10452.0
176.00	132352.0
177.00	8372.0
177.90	214.0

Instrument :
MSVOA_V
ClientSampleId :
BFB318

m/z	Abundance
36.00	1449.0
37.00	7844.0
38.00	7005.0
39.00	2933.0
40.00	318.0
42.00	122.0
42.90	116.0
44.00	1226.0
45.00	1471.0
46.00	313.0
47.00	1810.0
48.00	1023.0
49.00	6879.0
50.00	32528.0
51.00	10291.0
52.00	581.0
53.00	184.0
54.00	119.0
55.00	457.0
56.00	2485.0
57.00	4716.0
58.10	242.0
60.00	1547.0
61.00	8548.0
62.00	8337.0
63.00	7332.0
64.00	1190.0
65.00	1718.0
66.00	173.0
67.10	559.0
68.00	17120.0
69.00	17896.0
70.10	1427.0
71.00	102.0
72.00	1100.0
73.00	8334.0
74.00	28744.0
75.00	84656.0
76.00	7383.0
76.90	906.0
77.90	811.0
78.90	6735.0
80.00	1927.0
80.90	7222.0
81.90	1765.0
83.00	149.0
86.00	292.0
87.00	7998.0
88.00	7020.0
90.90	819.0
92.00	4881.0
93.00	7633.0
94.00	20328.0
95.00	163200.0
96.00	10736.0
96.90	292.0
103.90	924.0
105.00	229.0
105.90	799.0
106.80	192.0
107.80	144.0
110.80	215.0
111.90	174.0
112.90	166.0
114.80	212.0
115.90	715.0
116.90	1452.0
118.00	752.0
118.80	1081.0
122.90	100.0
123.80	164.0
127.90	666.0
128.80	308.0
129.90	723.0
130.90	293.0
134.90	365.0
136.80	318.0
140.00	240.0
140.90	1993.0
142.00	335.0
142.90	2410.0
143.80	197.0
144.90	837.0
146.00	276.0
146.80	113.0
147.90	343.0
148.80	168.0
149.80	251.0
151.80	162.0
153.10	135.0
155.00	431.0
156.90	251.0

Instrument :
MSVOA_V
ClientSampleId :
BFB318

158.90	231.0
160.70	147.0
170.90	267.0
171.90	1725.0
173.00	1783.0
174.00	139392.0
175.00	10497.0
176.00	134848.0
177.00	8342.0
178.00	217.0

Instrument :
MSVOA_V
ClientSampleId :
BFB318