
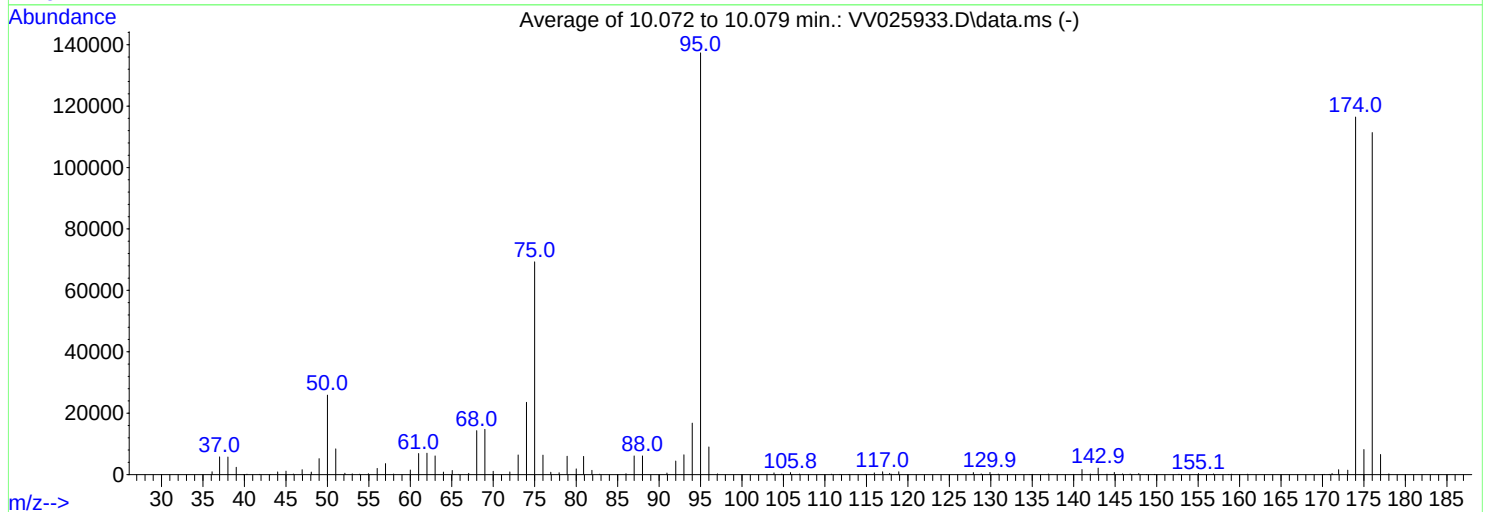


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051922\
 Data File : VV025933.D
 Acq On : 19 May 2022 09:46
 Operator : SY/MD
 Sample : BFB202
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB202

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM051822.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu May 19 07:42:58 2022

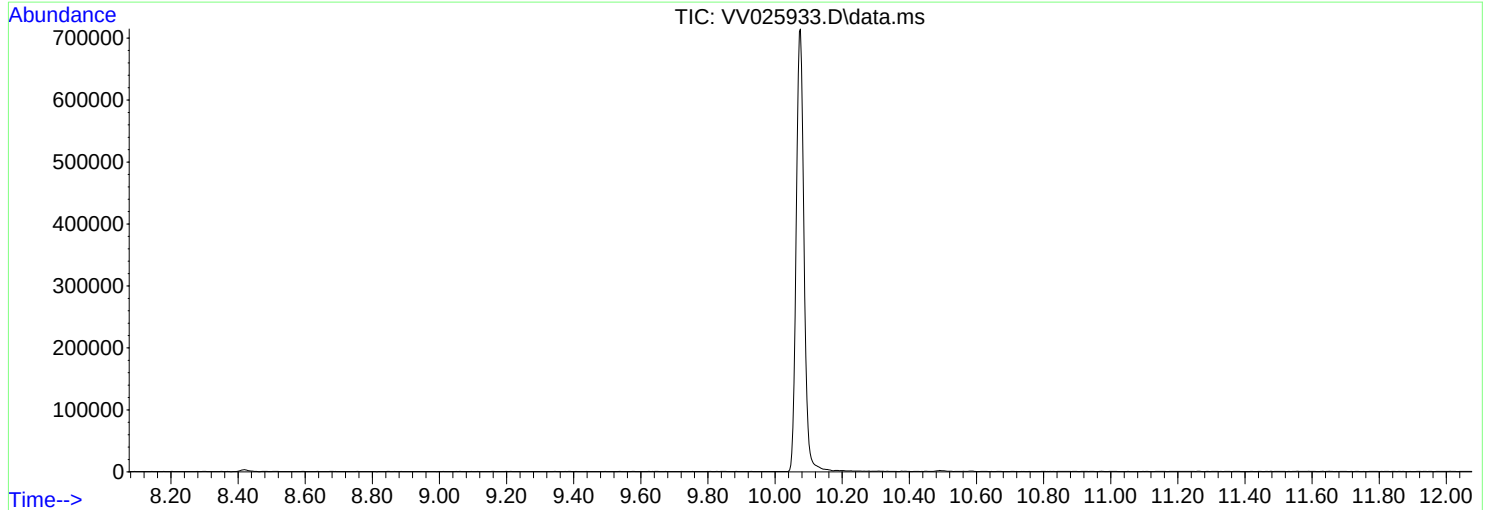

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	25925	PASS
75	95	30	80	50.4	69277	PASS
95	95	100	100	100.0	137347	PASS
96	95	5	9	6.6	9031	PASS
173	174	0.00	2	1.3	1463	PASS
174	95	50	120	84.8	116459	PASS
175	174	5	9	7.0	8192	PASS
176	174	95	101	95.6	111381	PASS
177	176	5	9	5.9	6558	PASS

m/z	Abundance
39.90	218.0
44.00	319.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202

m/z	Abundance
36.10	992.0
37.00	5865.0
38.00	6294.0
39.00	2559.0
40.00	241.0
43.10	119.0
44.00	1242.0
45.00	1293.0
45.90	185.0
46.90	1809.0
48.00	818.0
49.00	5632.0
50.00	26896.0
51.00	9027.0
52.10	517.0
53.00	258.0
53.90	138.0
55.00	325.0
56.00	2148.0
57.00	3613.0
58.00	200.0
60.00	1511.0
61.00	7216.0
62.00	7371.0
63.00	6262.0
64.00	946.0
65.00	1321.0
65.90	127.0
67.10	399.0
68.00	14536.0
69.00	15764.0
70.00	1140.0
72.00	915.0
73.00	6587.0
74.00	24448.0
75.00	70808.0
76.00	6512.0
77.00	807.0
77.90	619.0
78.90	6188.0
80.00	1986.0
80.90	6134.0
81.90	1445.0
83.00	163.0
86.00	361.0
87.00	6339.0
88.00	6176.0
90.90	582.0
92.00	4825.0
93.00	6919.0
94.00	17312.0
95.00	141312.0
96.00	9254.0
97.00	267.0
103.90	635.0
104.80	235.0
105.90	699.0
107.00	222.0
110.80	155.0
112.90	137.0
114.90	182.0
115.90	583.0
116.90	997.0
117.80	631.0
118.90	915.0
127.90	740.0
128.80	297.0
129.90	779.0
131.00	212.0
134.70	191.0
137.00	276.0
140.10	151.0
141.00	1740.0
142.00	196.0
142.90	2068.0
144.00	181.0
144.90	800.0
145.90	227.0
146.80	229.0
147.90	380.0
148.80	104.0
149.70	127.0
152.70	185.0
155.10	381.0
156.80	256.0
158.70	107.0
159.10	152.0
160.90	196.0
170.20	117.0
171.10	349.0
172.00	1666.0
173.10	1511.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202

174.00	117120.0
175.00	8359.0
176.00	112280.0
177.00	6791.0
178.00	265.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202

m/z	Abundance
36.10	965.0
37.00	5946.0
38.00	5900.0
39.00	2497.0
40.00	248.0
40.30	244.0
41.90	138.0
44.00	1232.0
45.00	1154.0
45.90	181.0
47.00	1666.0
48.00	854.0
49.00	5269.0
50.00	26888.0
51.00	8556.0
52.10	522.0
53.00	281.0
53.90	156.0
55.00	334.0
56.00	2110.0
57.00	3735.0
58.00	212.0
60.00	1555.0
61.00	7106.0
62.00	7231.0
63.00	6285.0
64.00	863.0
65.10	1380.0
65.90	129.0
67.10	445.0
68.00	14791.0
69.00	15174.0
70.00	1144.0
72.00	930.0
73.00	6673.0
74.00	24352.0
75.00	71608.0
76.00	6451.0
76.90	806.0
78.00	671.0
78.90	6140.0
80.00	1988.0
80.90	6182.0
81.90	1417.0
82.80	144.0
86.00	349.0
87.00	6203.0
88.00	6268.0
91.00	547.0
92.00	4569.0
93.00	6647.0
94.00	17328.0
95.00	141440.0
96.00	9343.0
97.10	246.0
103.00	121.0
103.80	604.0
104.80	212.0
105.80	721.0
106.90	216.0
110.80	141.0
111.80	115.0
112.90	119.0
114.80	131.0
115.90	592.0
116.90	959.0
117.80	589.0
118.90	971.0
127.90	741.0
128.90	266.0
129.90	784.0
130.90	232.0
135.00	199.0
137.00	241.0
141.00	1724.0
142.00	196.0
142.90	2208.0
144.00	179.0
144.90	737.0
145.90	244.0
146.80	225.0
147.80	393.0
149.80	136.0
152.70	193.0
155.00	424.0
156.90	283.0
159.10	166.0
160.90	194.0
170.20	137.0
171.20	386.0
172.00	1655.0
173.00	1508.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202

174.00	120136.0
175.00	8417.0
176.00	114816.0
177.00	6641.0
178.00	260.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202

m/z	Abundance
36.10	839.0
37.00	5520.0
38.00	4960.0
39.00	2161.0
39.90	247.0
40.30	234.0
41.80	153.0
44.00	1139.0
45.00	964.0
45.90	188.0
47.00	1448.0
48.10	814.0
49.00	4705.0
50.00	23992.0
51.00	7590.0
52.10	455.0
53.00	275.0
53.90	145.0
54.90	296.0
56.00	1914.0
57.00	3452.0
58.00	203.0
60.00	1413.0
61.00	6383.0
62.00	6428.0
63.00	5766.0
64.00	749.0
65.00	1309.0
65.80	125.0
67.00	457.0
68.00	13740.0
69.00	13306.0
70.00	1075.0
72.00	805.0
73.00	6007.0
74.00	21944.0
75.00	65416.0
76.00	6067.0
77.00	787.0
78.00	650.0
78.90	5699.0
80.00	1677.0
80.90	5539.0
81.90	1309.0
82.80	139.0
86.00	308.0
87.00	5690.0
88.00	5820.0
91.00	496.0
92.00	3941.0
93.00	5890.0
94.00	15733.0
95.00	129288.0
96.00	8496.0
97.10	209.0
103.00	128.0
103.90	517.0
104.80	176.0
105.90	682.0
106.90	180.0
110.80	132.0
111.80	144.0
112.90	108.0
116.00	535.0
117.00	905.0
118.00	489.0
118.90	964.0
127.90	651.0
128.90	214.0
129.90	655.0
130.80	256.0
135.00	182.0
136.90	179.0
139.90	112.0
141.00	1508.0
142.00	165.0
143.00	2154.0
144.00	169.0
144.90	639.0
145.90	261.0
146.80	159.0
147.80	363.0
149.80	135.0
152.70	156.0
155.00	390.0
156.90	272.0
159.00	190.0
161.00	152.0
170.80	294.0
171.20	326.0
171.90	1539.0
173.00	1371.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202

174.00	112120.0
175.00	7800.0
176.00	107048.0
177.00	6243.0
178.00	212.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202