

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052322\
 Data File : VV025951.D
 Acq On : 23 May 2022 10:50
 Operator : SY/MD
 Sample : VV0523WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK362

Quant Time: May 24 05:30:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue May 24 05:29:18 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	170003	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	179093	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	80561	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	58304	4.152	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.000%
7) Chloroethane-d5	1.571	69	58284	4.848	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.000%
11) 1,1-Dichloroethene-d2	2.108	63	96324	3.099	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.000%
20) 2-Butanone-d5	3.902	46	61897	38.067	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	76.140%
24) Chloroform-d	4.346	84	125139	5.456	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	109.200%
26) 1,2-Dichloroethane-d4	5.031	65	53513	5.502	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.000%
32) Benzene-d6	5.047	84	236326	5.082	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.600%
36) 1,2-Dichloropropane-d6	6.066	67	76332	5.646	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	113.000%
41) Toluene-d8	7.314	98	192513	4.453	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.000%
43) trans-1,3-Dichloroprop...	7.625	79	18187	4.113	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.200%
46) 2-Hexanone-d5	8.088	63	80066	48.769	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.540%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	47859	5.495	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	110.000%
66) 1,2-Dichlorobenzene-d4	11.622	152	68370	5.961	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	119.200%
Target Compounds						
16) Methylene chloride	2.513	84	3643	0.220	ug/L	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052322\
Data File : VV025951.D
Acq On : 23 May 2022 10:50
Operator : SY/MD
Sample : VV0523WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK362

Quant Time: May 24 05:30:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue May 24 05:29:18 2022
Response via : Initial Calibration

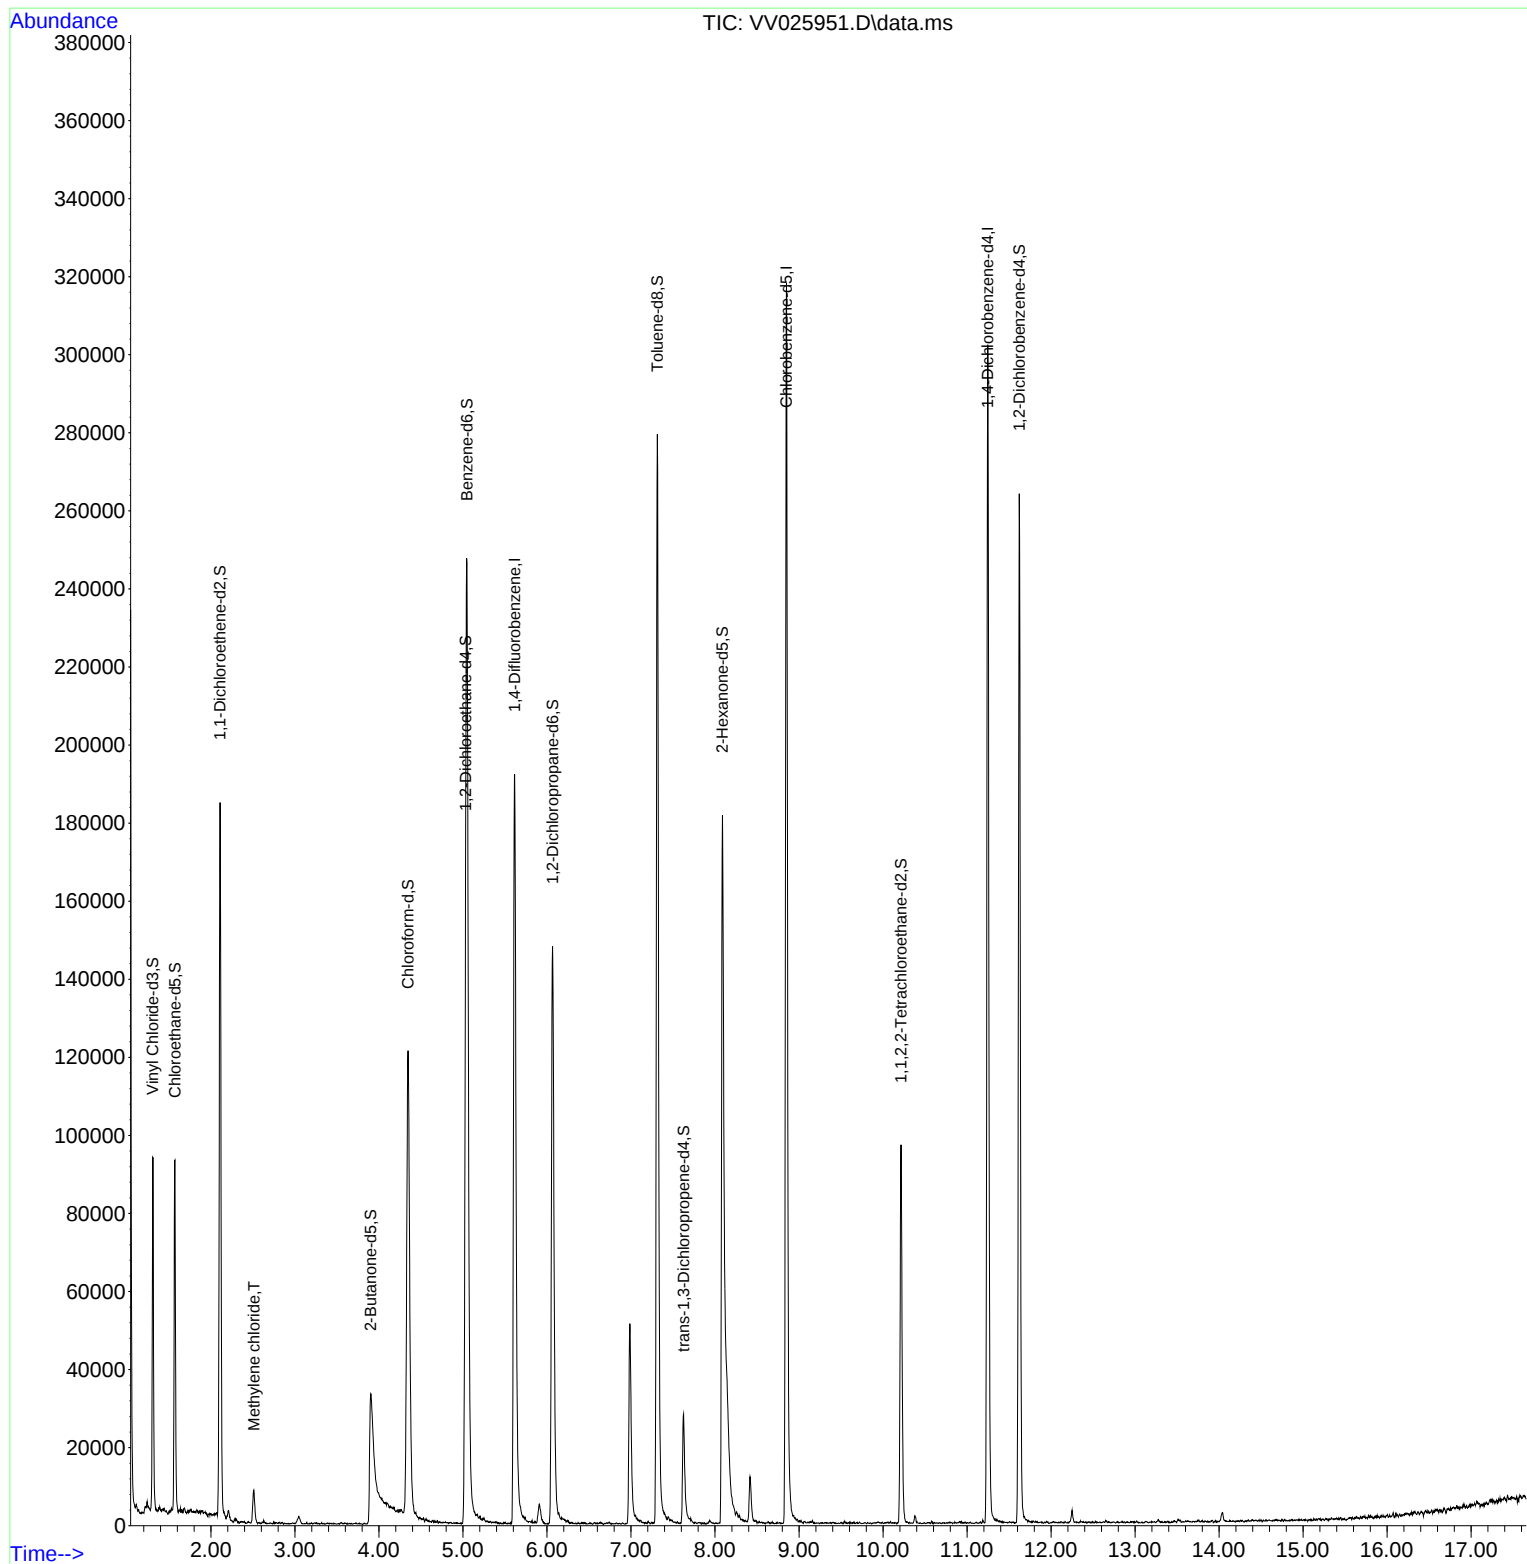

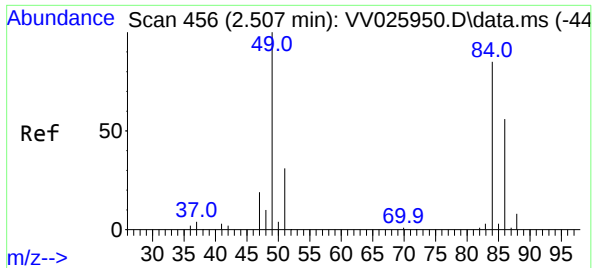

#16
Methylene chloride
Concen: 0.220 ug/L
RT: 2.513 min Scan# 4
Delta R.T. 0.007 min
Lab File: VV025951.D
Acq: 23 May 2022 10:50

Instrument :
MSVOA_V
ClientSampleId :
VBLK362

Tgt Ion: 84 Resp: 3643

Ion	Ratio	Lower	Upper
84	100		
86	57.3	45.4	84.2
49	113.1	85.6	159.0

