

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052322\
 Data File : VV025951.D
 Acq On : 23 May 2022 10:50
 Operator : SY/MD
 Sample : VV0523WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK362

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025951.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	95	rVB	90478	95208	15.32%	1.918%
2	1.571	157	165	177	rVB	90277	105318	16.94%	2.121%
3	2.108	322	332	345	rBV	182687	262480	42.22%	5.286%
4	2.510	446	457	471	rVB2	8610	15069	2.42%	0.303%
5	3.902	877	890	918	rBV3	33386	127207	20.46%	2.562%
6	4.346	1012	1028	1052	rVB	118391	294512	47.38%	5.932%
7	5.044	1229	1245	1274	rBV2	247277	621642	100.00%	12.520%
8	5.616	1411	1423	1459	rBV	192047	404592	65.08%	8.149%
9	5.908	1503	1514	1524	rBV6	4850	10030	1.61%	0.202%
10	6.066	1551	1563	1584	rBV2	147685	311177	50.06%	6.267%
11	6.986	1839	1849	1868	rBV	51196	98096	15.78%	1.976%
12	7.314	1938	1951	1977	rBV	279013	496024	79.79%	9.990%
13	7.625	2038	2048	2067	rBV	27988	53790	8.65%	1.083%
14	8.088	2182	2192	2240	rBV	181393	477650	76.84%	9.620%
15	8.416	2284	2294	2308	rBV4	11662	20564	3.31%	0.414%
16	8.850	2416	2429	2453	rBV	317684	526297	84.66%	10.600%
17	10.214	2841	2853	2871	rBV	96972	156343	25.15%	3.149%
18	11.246	3163	3174	3199	rBV	301877	476608	76.67%	9.599%
19	11.622	3279	3291	3308	rBV	263619	412575	66.37%	8.309%




Sum of corrected areas: 4965182

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052322\
Data File : VV025951.D
Acq On : 23 May 2022 10:50
Operator : SY/MD
Sample : VV0523WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK362

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

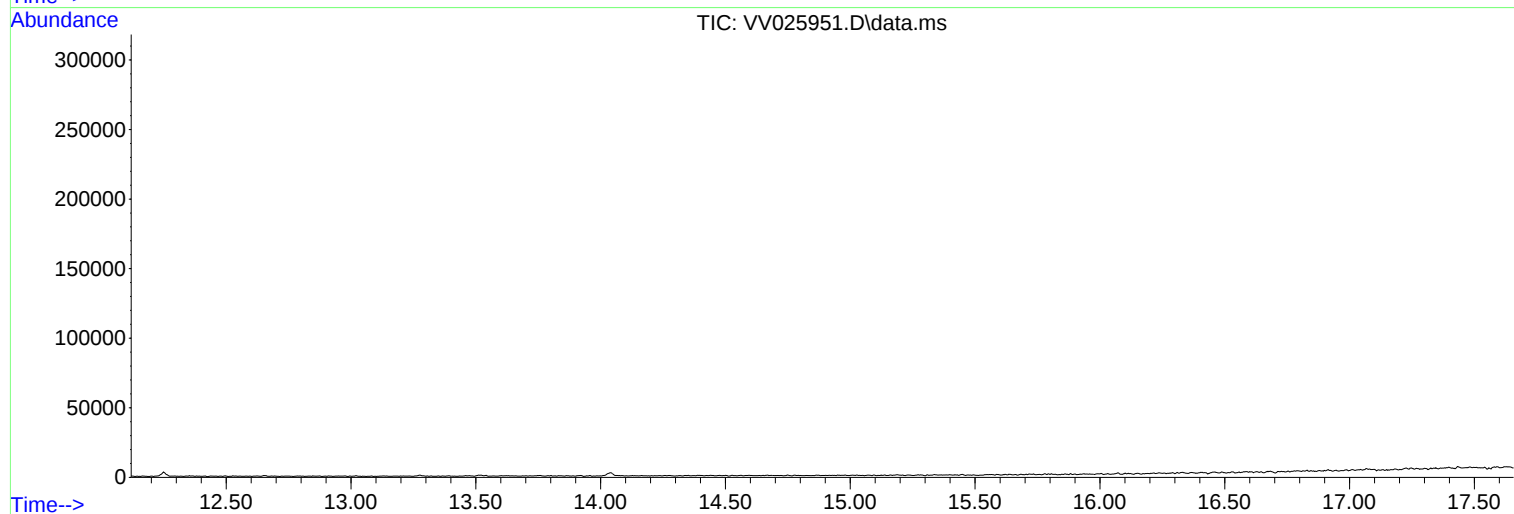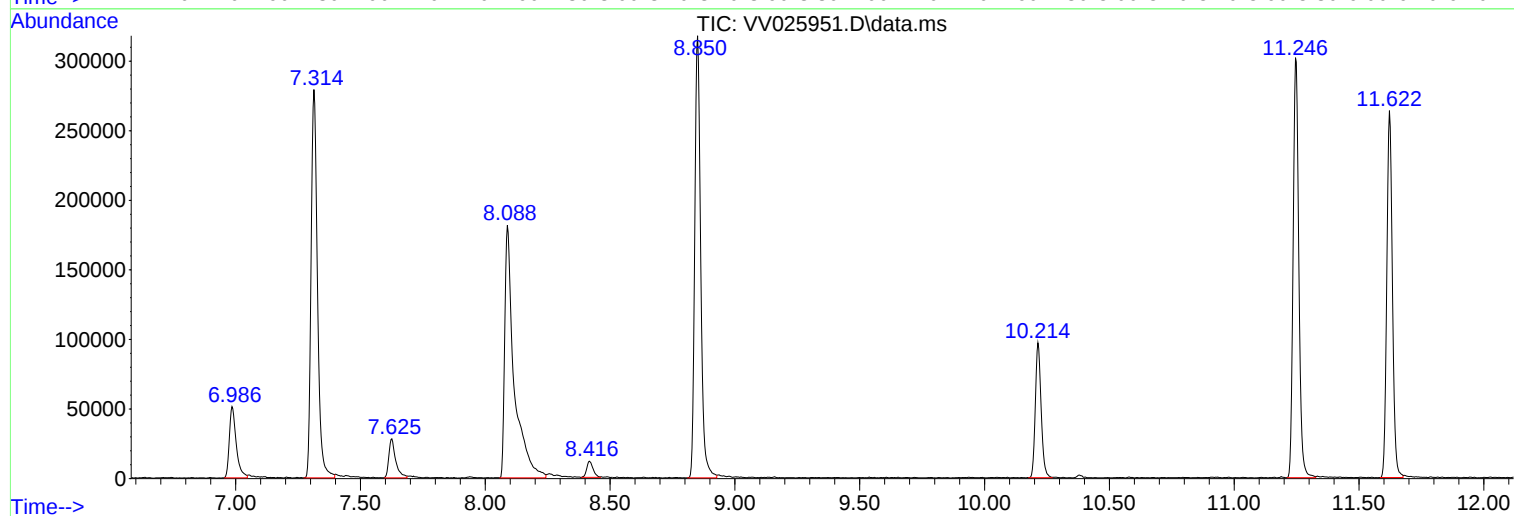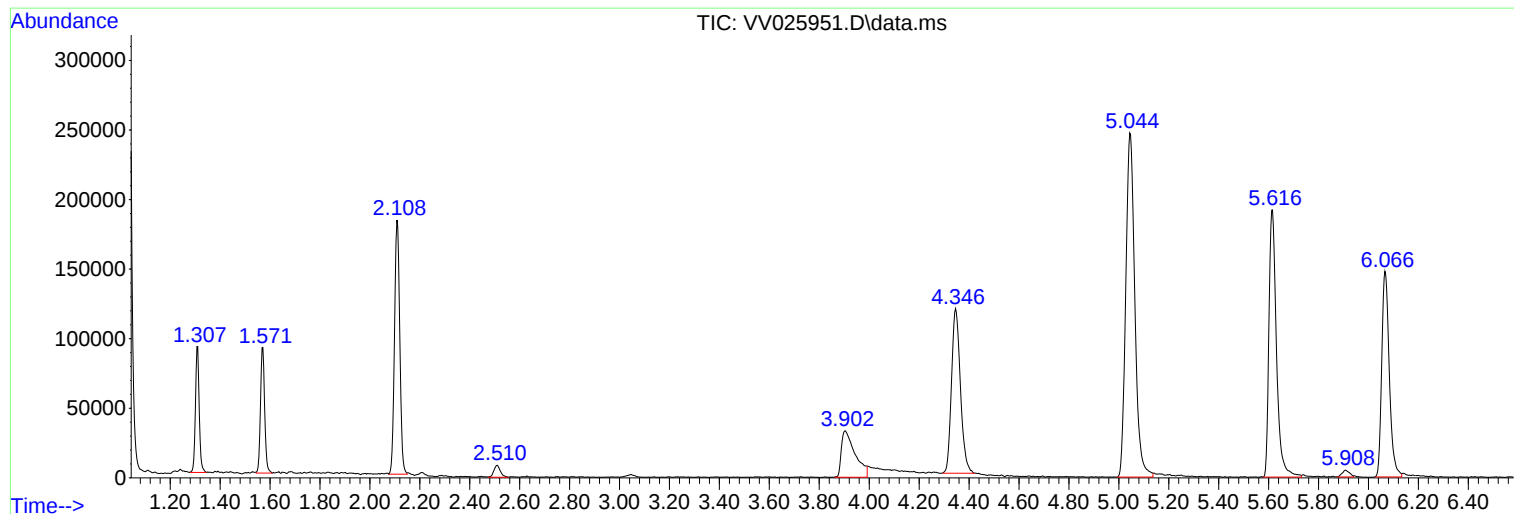

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052322\
Data File : VV025951.D
Acq On : 23 May 2022 10:50
Operator : SY/MD
Sample : VV0523WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK362

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052322\
Data File : VV025951.D
Acq On : 23 May 2022 10:50
Operator : SY/MD
Sample : VV0523WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK362

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc