

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052524\
 Data File : VV035783.D
 Acq On : 25 May 2024 09:59
 Operator : SY/MD
 Sample : VV0525SBL01
 Misc : 5.00g/10.0mL/MSVOA_V/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: May 27 01:42:02 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon May 27 01:41:30 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	517630	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	523356	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	233048	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	204407	25.549	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	102.200%
7) Chloroethane-d5	1.529	69	161039	24.950	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	99.800%
11) 1,1-Dichloroethene-d2	2.053	65	86792	24.504	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	98.000%
21) 2-Butanone-d5	3.854	46	51263	22.578	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	45.160%
24) Chloroform-d	4.243	84	343895	22.347	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.400%
26) 1,2-Dichloroethane-d4	4.937	65	176646	23.219	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.880%
32) Benzene-d6	4.953	84	682805	23.834	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.320%
36) 1,2-Dichloropropane-d6	5.985	67	212944	24.086	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.360%
41) Toluene-d8	7.239	98	583329	22.878	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	91.520%
43) trans-1,3-Dichloroprop...	7.555	79	82262	21.756	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.040%
47) 2-Hexanone-d5	8.034	63	44726	28.134	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	56.260%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	149420	17.539	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	70.160%
66) 1,2-Dichlorobenzene-d4	11.558	152	204530	25.289	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.160%
Target Compounds						
					Qvalue	
48) 2-Hexanone	8.034	43	5480	1.350	ug/L	# 38
71) Naphthalene	13.445	128	9022	0.483	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052524\
Data File : VV035783.D
Acq On : 25 May 2024 09:59
Operator : SY/MD
Sample : VV0525SBL01
Misc : 5.00g/10.0mL/MSVOA_V/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: May 27 01:42:02 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 27 01:41:30 2024
Response via : Initial Calibration

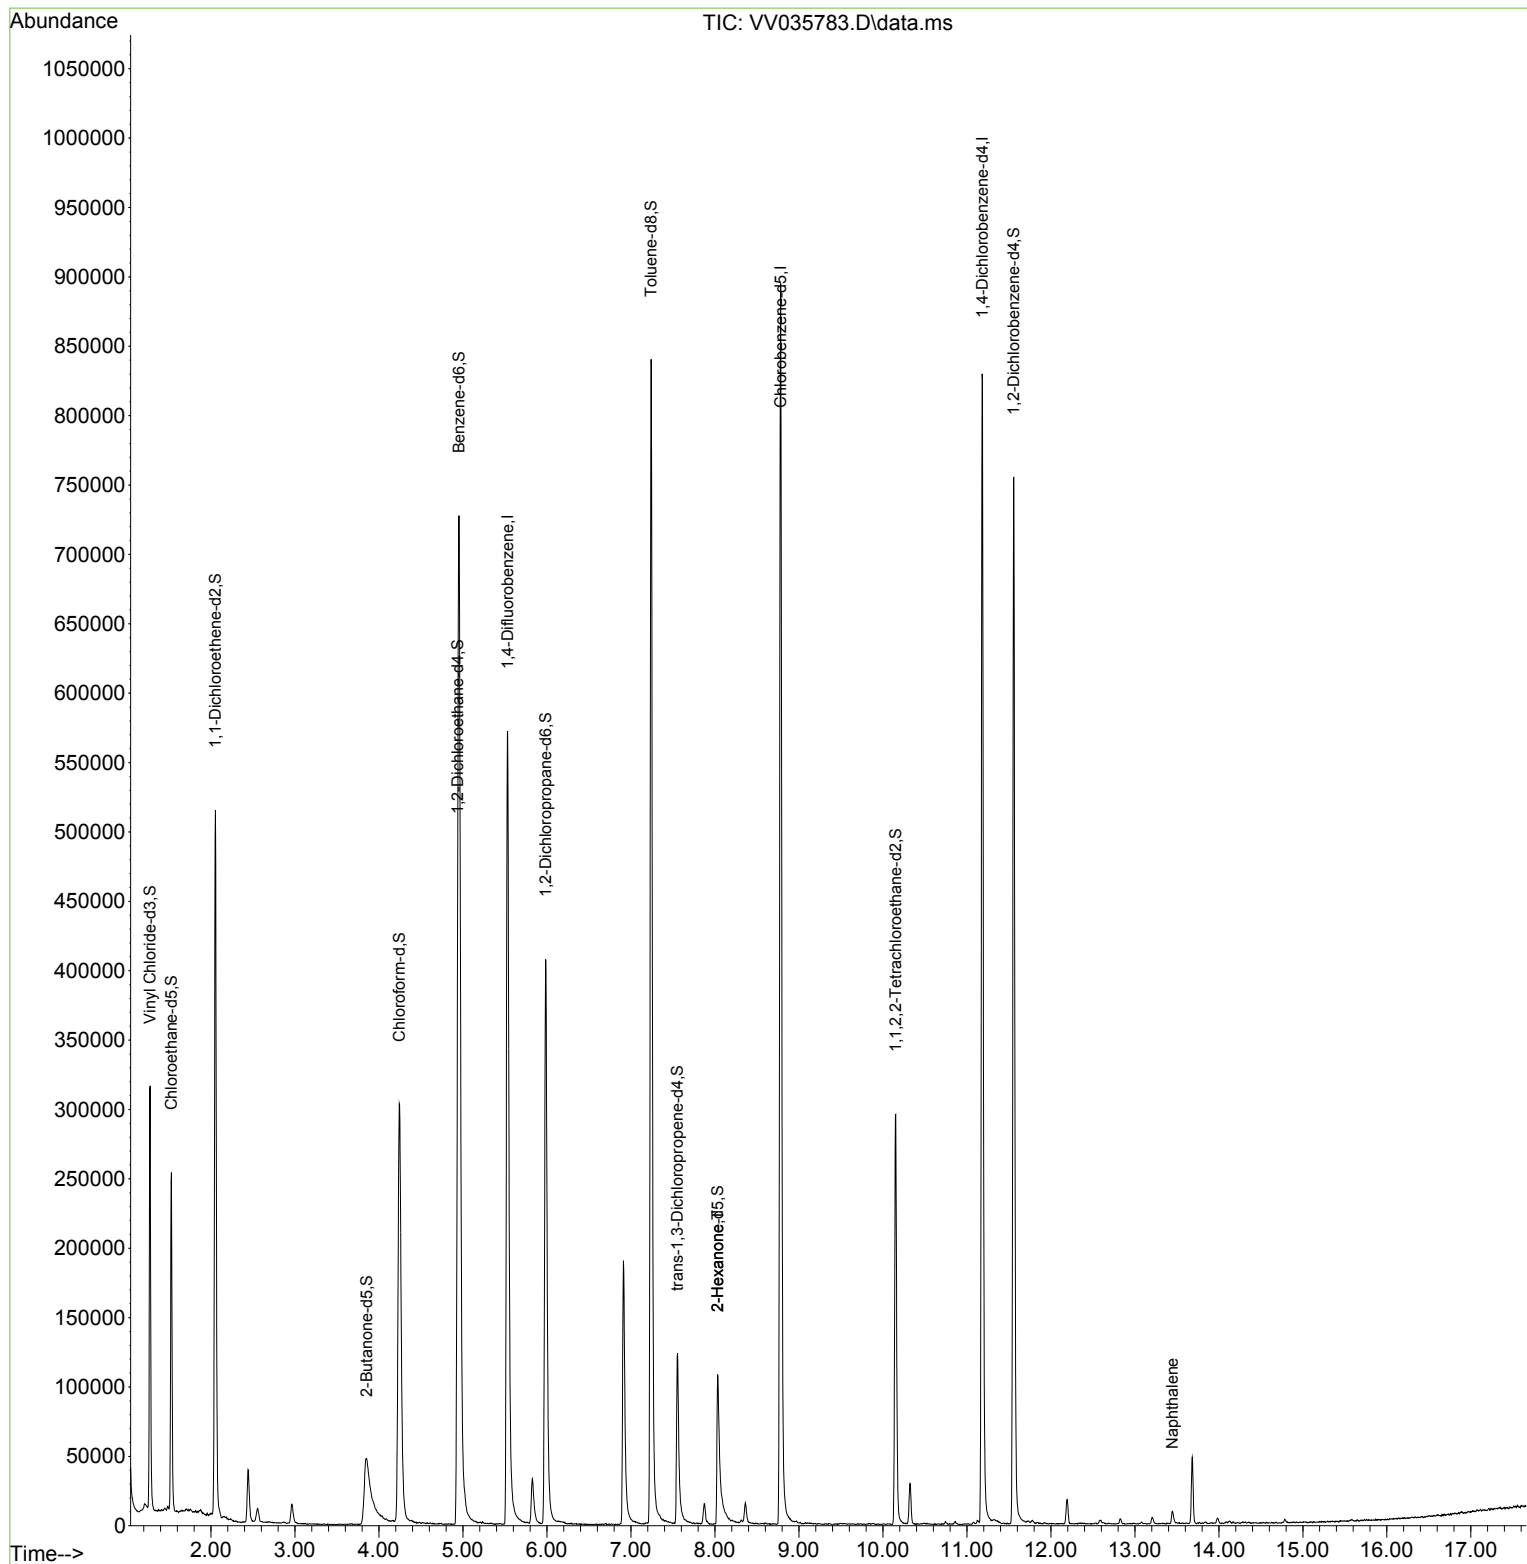



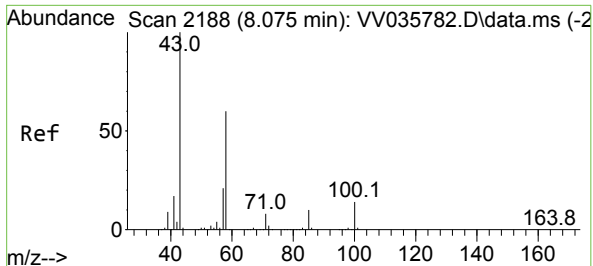


#48
2-Hexanone
Concen: 1.350 ug/L
RT: 8.034 min Scan# 2188
Delta R.T. -0.042 min
Lab File: VV035783.D
Acq: 25 May 2024 09:59

Instrument :
MSVOA_V
ClientSampleId :

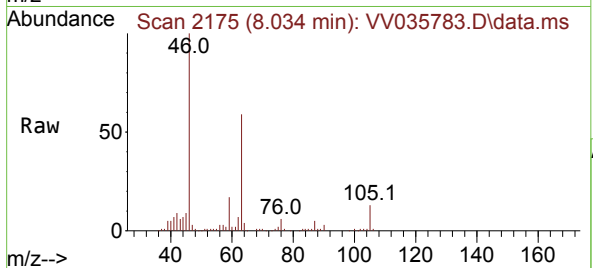

Tgt Ion: 43 Resp: 5480
Ion Ratio Lower Upper
43 100
58 0.0 48.8 73.2#
57 37.7 16.9 25.3#
100 4.3 11.7 17.5#

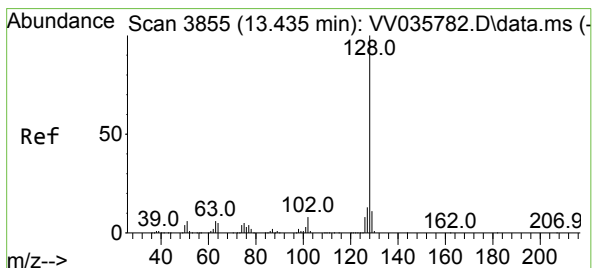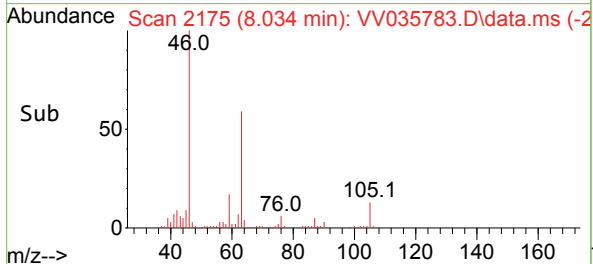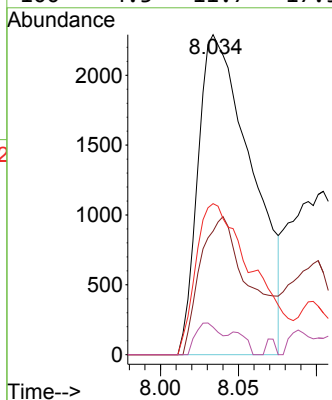

#71
Naphthalene
Concen: 0.483 ug/L
RT: 13.445 min Scan# 3858
Delta R.T. 0.010 min
Lab File: VV035783.D
Acq: 25 May 2024 09:59

Tgt Ion: 128 Resp: 9022
Ion Ratio Lower Upper
128 100
127 11.5 10.4 15.6
129 10.0 8.6 13.0

