

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052524\
 Data File : VV035787.D
 Acq On : 25 May 2024 11:30
 Operator : SY/MD
 Sample : P2577-06
 Misc : 6.14g/10.0mL/MSVOA_V/SOIL/B
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: May 27 01:43:02 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon May 27 01:41:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	469908	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	423180	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	131755	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	155217	21.371	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.480%
7) Chloroethane-d5	1.529	69	124004	21.164	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.640%
11) 1,1-Dichloroethene-d2	2.053	65	63573	19.771	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	79.080%
21) 2-Butanone-d5	3.847	46	17439	8.461	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	16.920%#
24) Chloroform-d	4.246	84	263392	18.854	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	75.400%
26) 1,2-Dichloroethane-d4	4.941	65	148561	21.511	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	86.040%
32) Benzene-d6	4.957	84	503843	21.750	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	87.000%
36) 1,2-Dichloropropane-d6	5.989	67	166922	23.350	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.400%
41) Toluene-d8	7.243	98	385278	18.688	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	74.760%
43) trans-1,3-Dichloroprop...	7.555	79	58629	19.176	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	76.720%
47) 2-Hexanone-d5	8.037	63	38016	29.574	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	59.140%
56) 1,1,2,2-Tetrachloroeth...	10.153	84	131988	19.160	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	76.640%
66) 1,2-Dichlorobenzene-d4	11.561	152	97410	21.303	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	85.200%
Target Compounds						Qvalue
35) Methylcyclohexane	5.985	83	40925	3.403	ug/L	# 21


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052524\
Data File : VV035787.D
Acq On : 25 May 2024 11:30
Operator : SY/MD
Sample : P2577-06
Misc : 6.14g/10.0mL/MSVOA_V/SOIL/B
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: May 27 01:43:02 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 27 01:41:30 2024
Response via : Initial Calibration

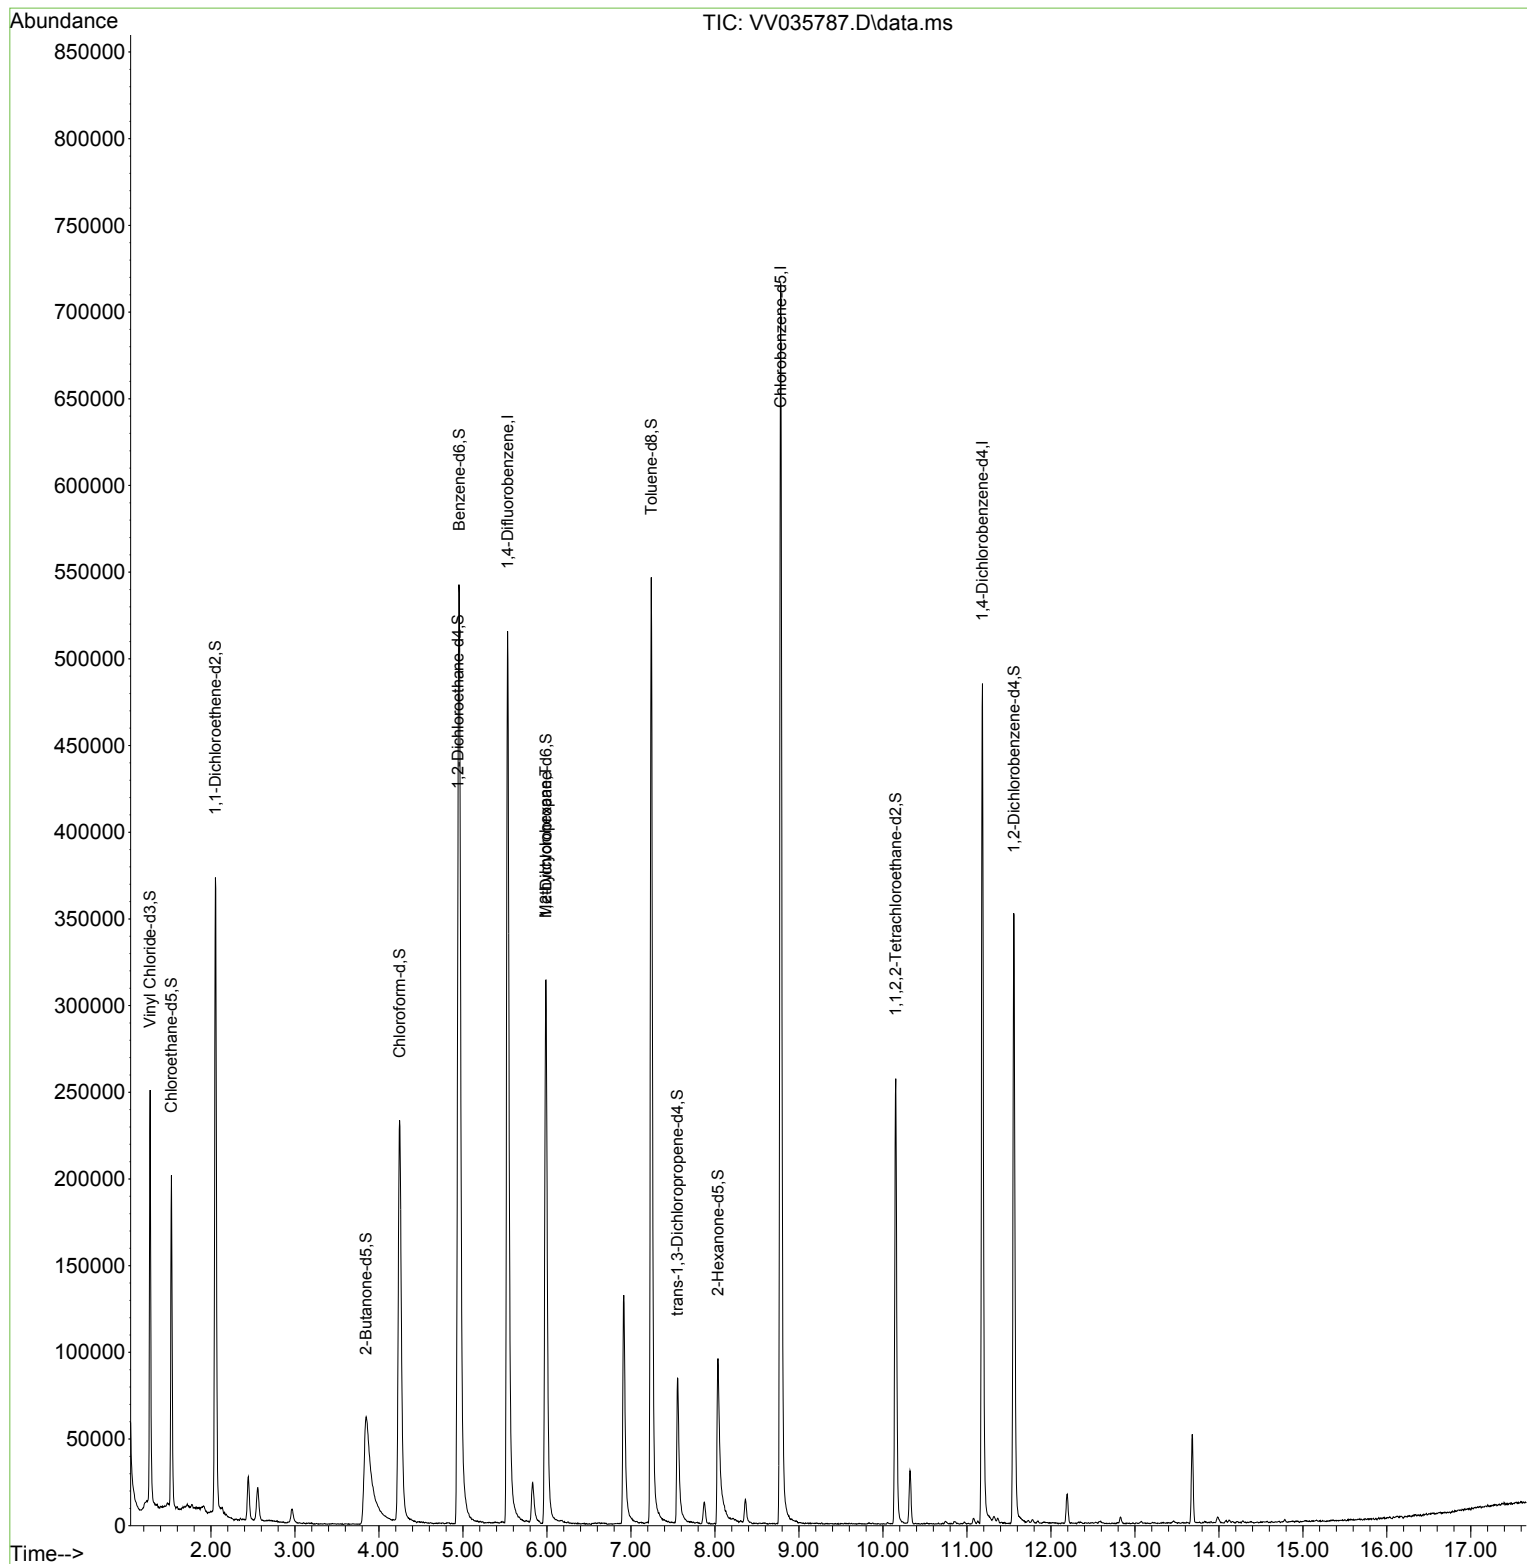

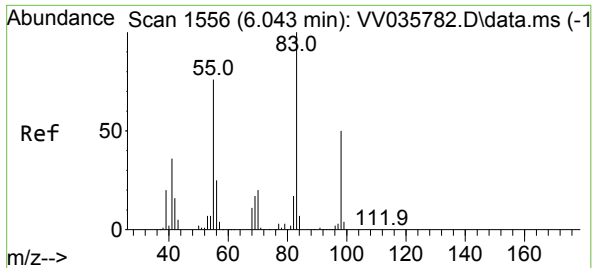

#35
Methylcyclohexane
Concen: 3.403 ug/L
RT: 5.985 min Scan# 11
Delta R.T. -0.058 min
Lab File: VV035787.D
Acq: 25 May 2024 11:30

Instrument :
MSVOA_V
ClientSampleId :

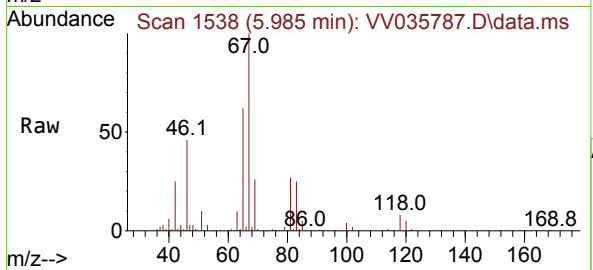

Tgt Ion:	83	Resp:	40925
Ion	Ratio	Lower	Upper
83	100		
55	0.5	57.5	86.3#
98	0.8	38.6	58.0#

