

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052524\
 Data File : VV035822.D
 Acq On : 26 May 2024 01:16
 Operator : SY/MD
 Sample : P2586-16
 Misc : 4.69g/10.0mL/MSVOA_V/SOIL/A
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: May 27 05:34:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon May 27 05:15:54 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	527582	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	426238	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	129065	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.272	65	162339	19.908	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.640%
7) Chloroethane-d5	1.526	69	138711	21.086	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.360%
11) 1,1-Dichloroethene-d2	2.053	65	67425	18.677	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	74.720%
21) 2-Butanone-d5	3.883	46	8483	3.666	ug/L	0.04
Spiked Amount	50.000	Range	20 - 135	Recovery	=	7.340%#
24) Chloroform-d	4.243	84	302710	19.300	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	77.200%
26) 1,2-Dichloroethane-d4	4.941	65	165918	21.398	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	85.600%
32) Benzene-d6	4.957	84	523497	22.437	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	89.760%
36) 1,2-Dichloropropane-d6	5.985	67	184228	25.586	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	102.360%
41) Toluene-d8	7.243	98	384014	18.493	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	73.960%
43) trans-1,3-Dichloroprop...	7.561	79	27490	8.927	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	35.720%
47) 2-Hexanone-d5	8.133	63	261	0.202	ug/L	0.10
Spiked Amount	50.000	Range	20 - 135	Recovery	=	0.400%#
56) 1,1,2,2-Tetrachloroeth...	10.153	84	117303	16.906	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	67.640%
66) 1,2-Dichlorobenzene-d4	11.558	152	75177	16.784	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	67.120%#
Target Compounds						
					Qvalue	
13) Acetone	2.166	43	16760	4.948	ug/L	97
60) Isopropylbenzene	9.837	105	22152	1.288	ug/L #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052524\
Data File : VV035822.D
Acq On : 26 May 2024 01:16
Operator : SY/MD
Sample : P2586-16
Misc : 4.69g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: May 27 05:34:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 27 05:15:54 2024
Response via : Initial Calibration

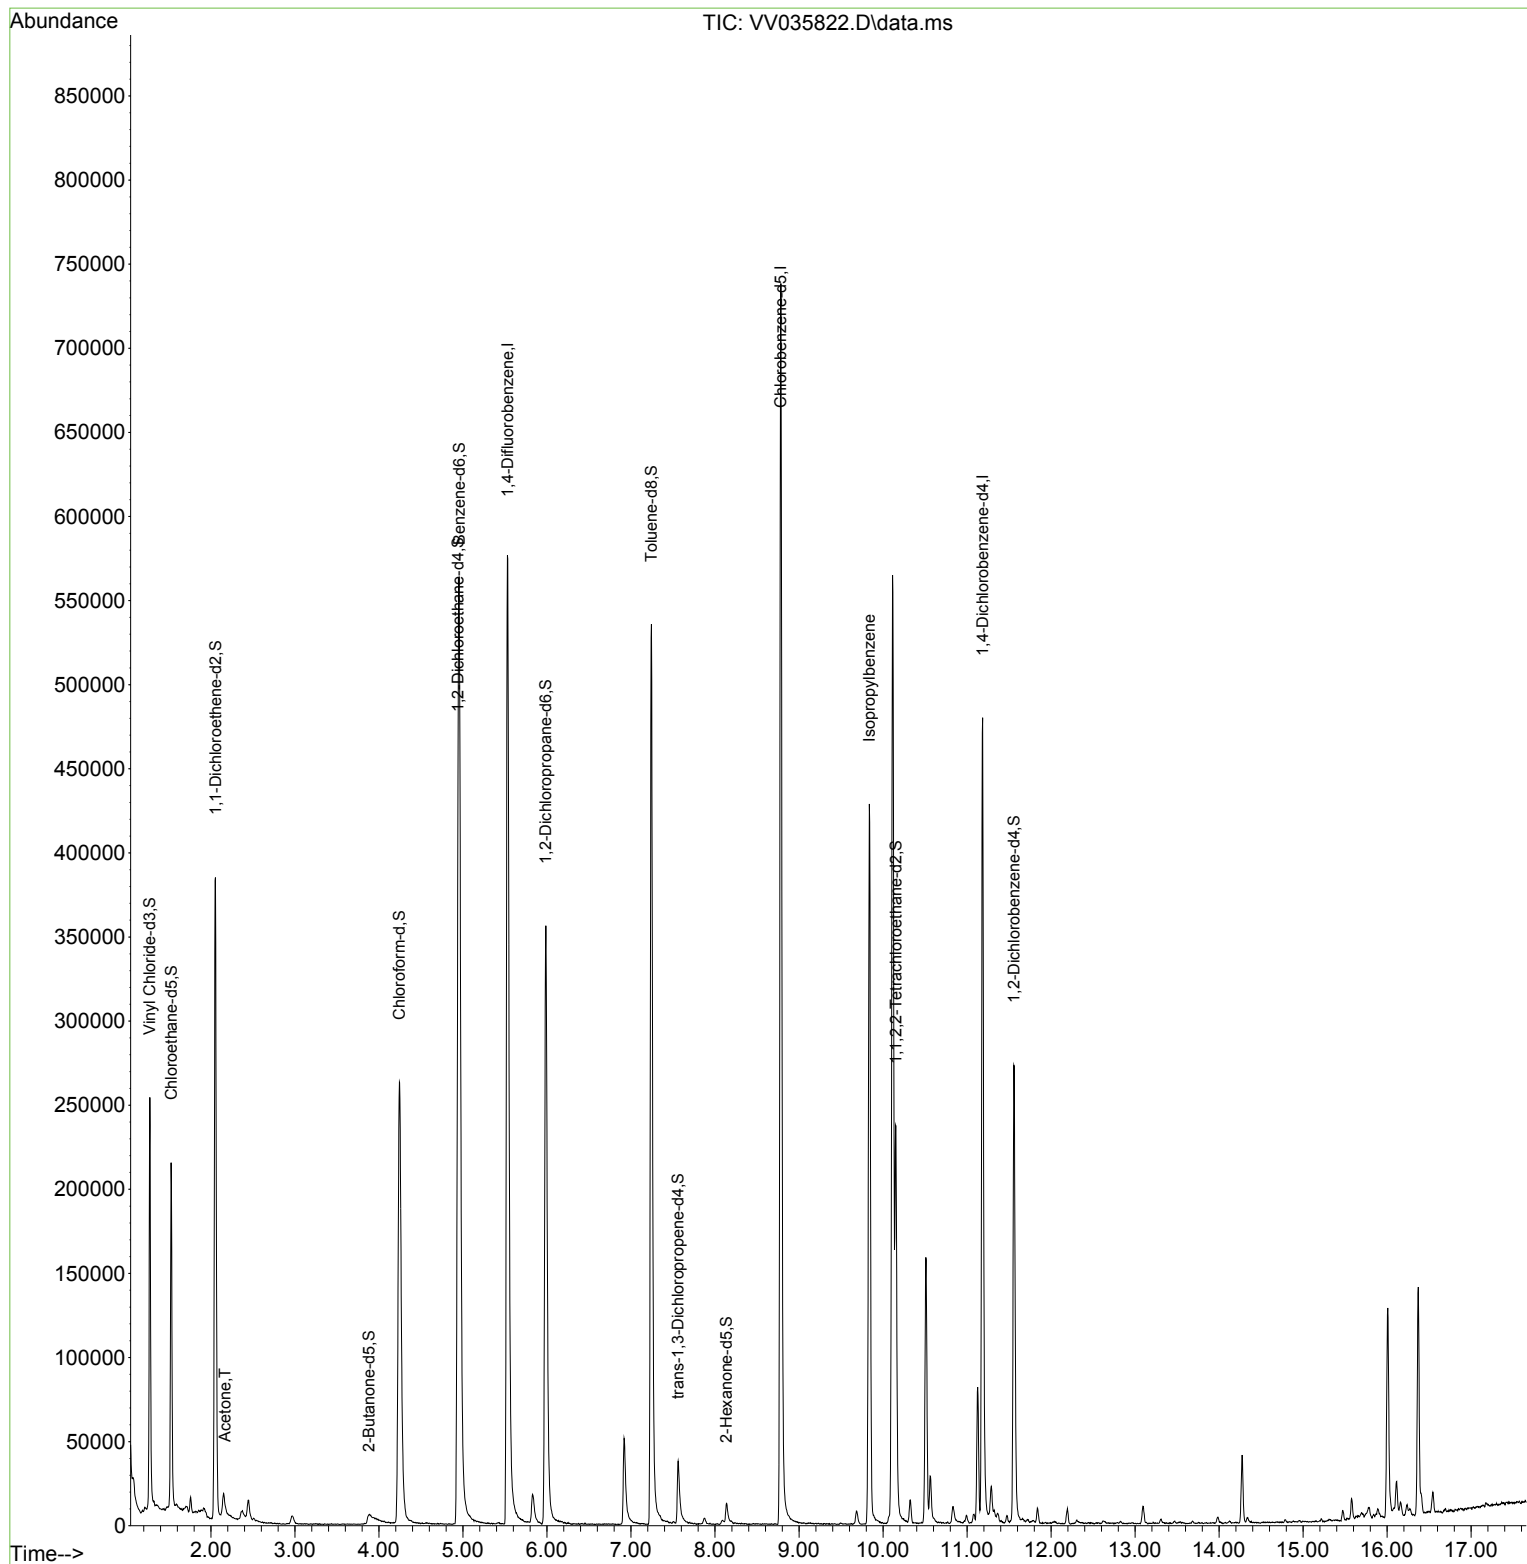

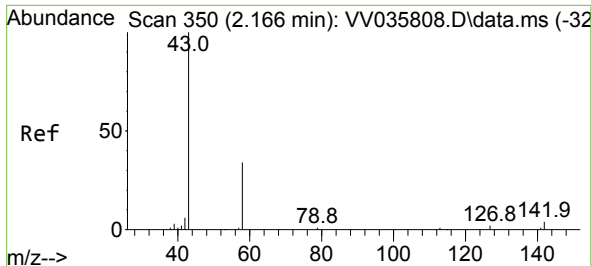

#13

Acetone

Concen: 4.948 ug/L

RT: 2.166 min Scan# 31

Delta R.T. 0.000 min

Lab File: VV035822.D

Acq: 26 May 2024 01:16

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 43 Resp: 16760

Ion Ratio Lower Upper

43 100

58 12.4 0.0 22.8

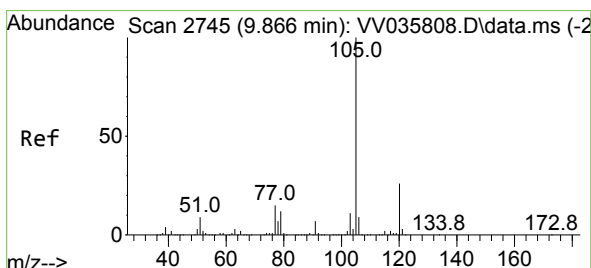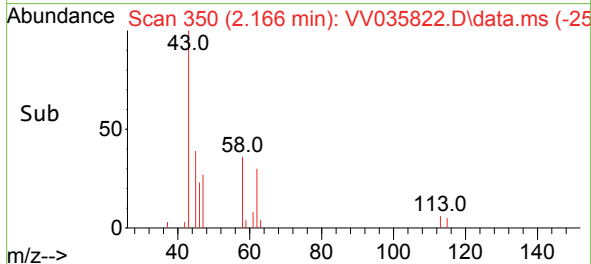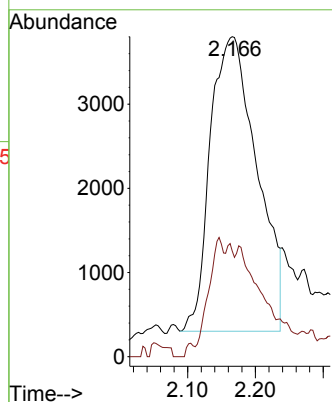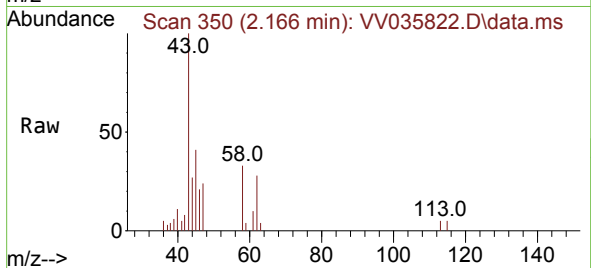

#60

Isopropylbenzene

Concen: 1.288 ug/L

RT: 9.837 min Scan# 2736

Delta R.T. -0.029 min

Lab File: VV035822.D

Acq: 26 May 2024 01:16

Tgt Ion:105 Resp: 22152

Ion Ratio Lower Upper

105 100

120 11.6 21.3 31.9#

77 223.5 12.2 18.2#

