




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052524\
Data File : VV035786.D
Acq On : 25 May 2024 11:07
Operator : SY/MD
Sample : P2577-05
Misc : 5.93g/10.0mL/MSVOA_V/SOIL/B
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHBN3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/28/2024
Supervised By :Mahesh Dadoda 05/28/2024

Quant Time: May 27 02:30:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 27 01:41:30 2024
Response via : Initial Calibration

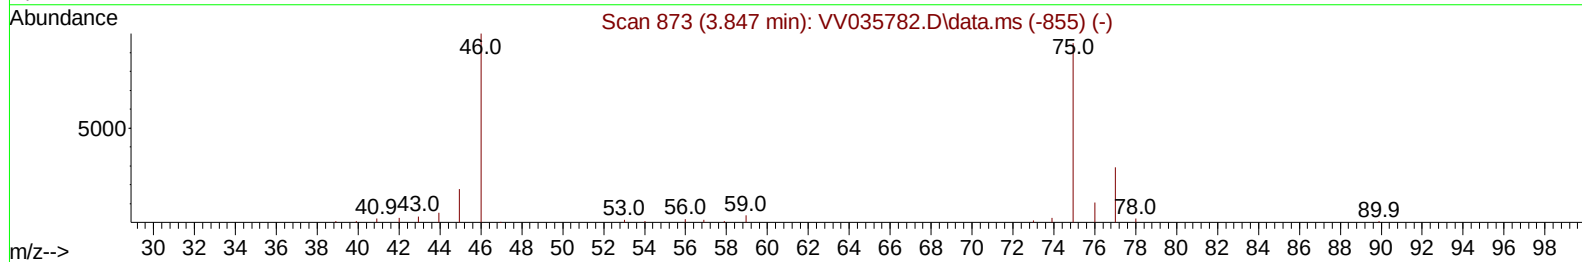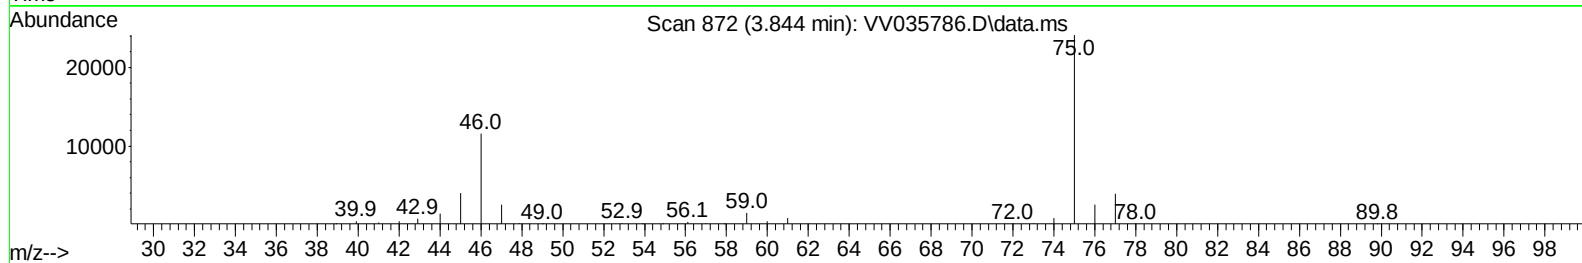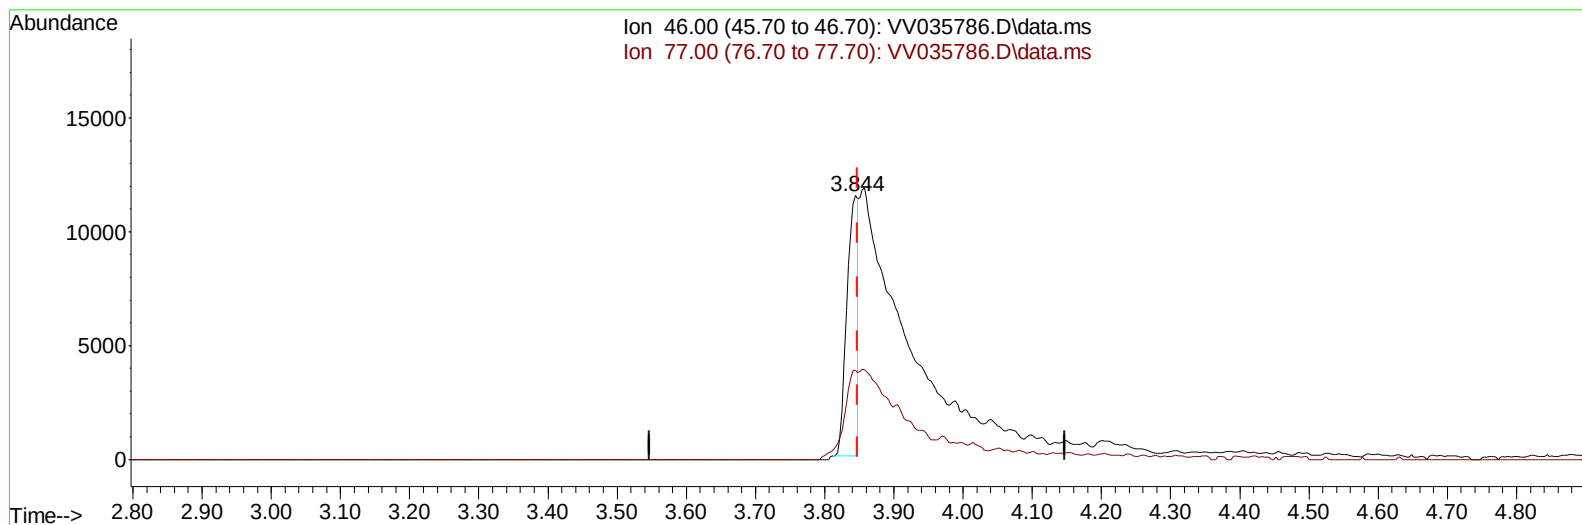

TIC: VV035786.D\data.ms

(21) 2-Butanone-d5 (S)

3.844min (-0.003) 5.21 ug/L

response 12659

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	13.10	41.94#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052524\
Data File : VV035786.D
Acq On : 25 May 2024 11:07
Operator : SY/MD
Sample : P2577-05
Misc : 5.93g/10.0mL/MSVOA_V/SOIL/B
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHBN3

Manual IntegrationsAPPROVED

Quant Time: May 27 02:30:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 27 01:41:30 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/28/2024
Supervised By :Mahesh Dadoda 05/28/2024

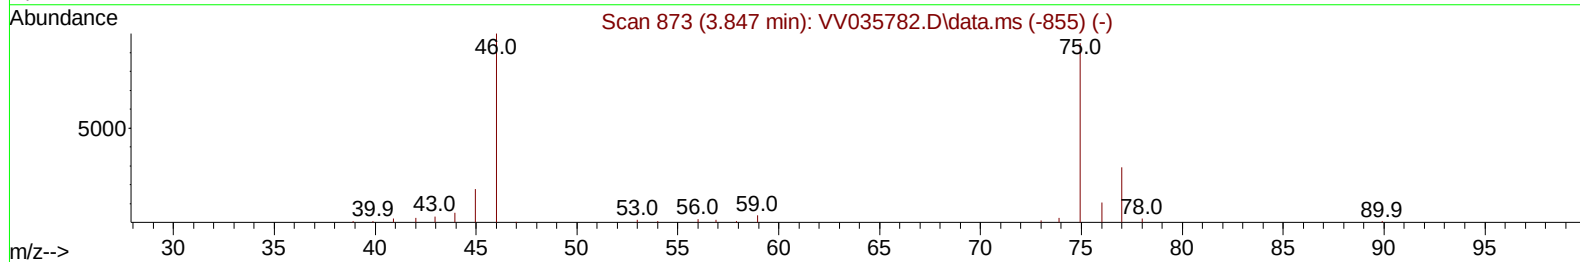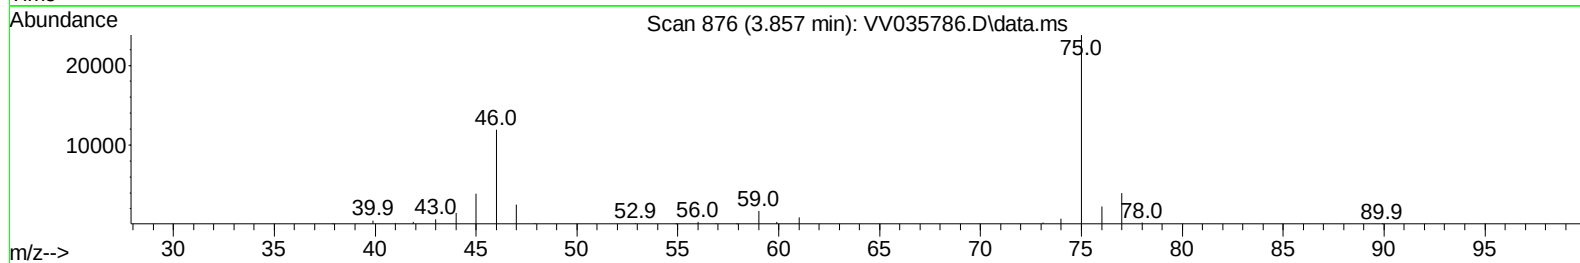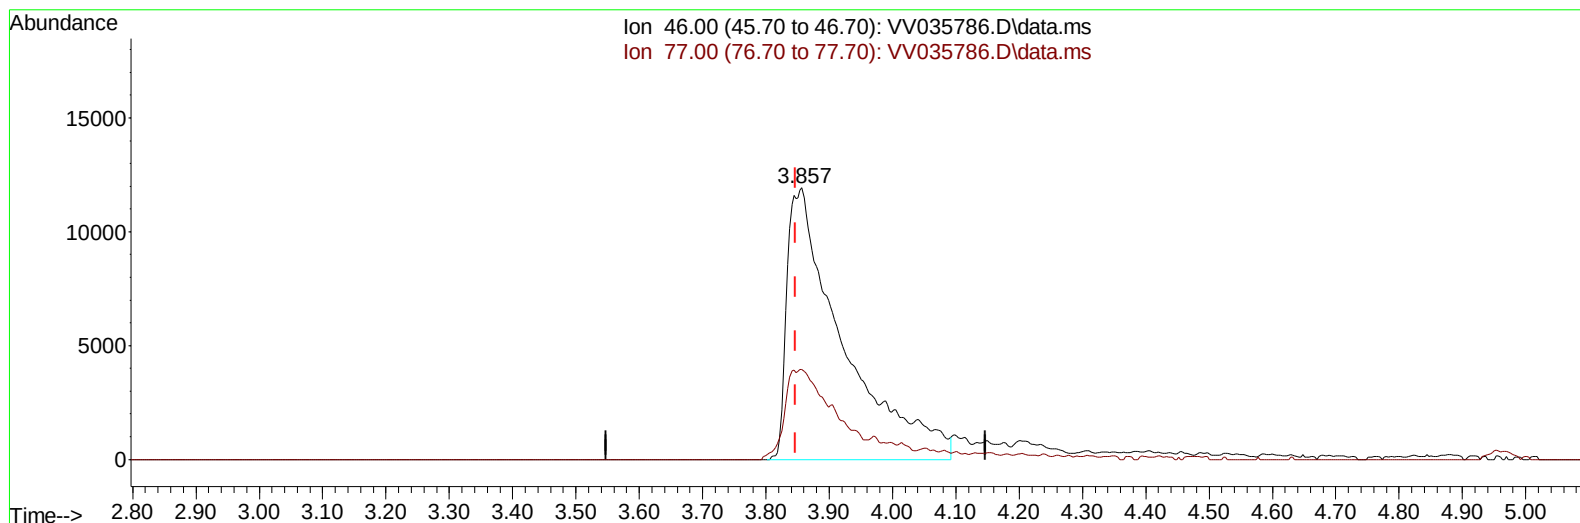

TIC: VV035786.D\data.ms

(21) 2-Butanone-d5 (S)

3.857min (+ 0.010) 29.99 ug/L m

response 72854

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	13.10	7.29#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052524\
 Data File : VV035786.D
 Acq On : 25 May 2024 11:07
 Operator : SY/MD
 Sample : P2577-05
 Misc : 5.93g/10.0mL/MSVOA_V/SOIL/B
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHBN3

Manual IntegrationsAPPROVED

Quant Time: May 27 02:30:01 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon May 27 01:41:30 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/28/2024
 Supervised By :Mahesh Dadoda 05/28/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	553800	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	494685	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	157589	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	160528	18.754	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	75.000%	
7) Chloroethane-d5	1.529	69	127788	18.506	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	74.040%	
11) 1,1-Dichloroethene-d2	2.053	65	66393	17.520	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	70.080%	
21) 2-Butanone-d5	3.857	46	72854m	29.992	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	59.980%	
24) Chloroform-d	4.246	84	272956	16.579	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	66.320%	
26) 1,2-Dichloroethane-d4	4.941	65	153580	18.869	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	75.480%	
32) Benzene-d6	4.957	84	519821	19.197	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	76.800%	
36) 1,2-Dichloropropane-d6	5.986	67	169473	20.280	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	81.120%	
41) Toluene-d8	7.243	98	410452	17.031	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	68.120%	
43) trans-1,3-Dichloroprop...	7.555	79	61388	17.176	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	68.720%	
47) 2-Hexanone-d5	8.034	63	38928	25.906	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	51.820%	
56) 1,1,2,2-Tetrachloroeth...	10.149	84	133404	16.567	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	66.280%	
66) 1,2-Dichlorobenzene-d4	11.561	152	109121	19.952	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	79.800%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052524\
Data File : VV035786.D
Acq On : 25 May 2024 11:07
Operator : SY/MD
Sample : P2577-05
Misc : 5.93g/10.0mL/MSVOA_V/SOIL/B
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHBN3

Manual IntegrationsAPPROVED

Quant Time: May 27 02:30:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 27 01:41:30 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/28/2024
Supervised By :Mahesh Dadoda 05/28/2024

