




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052524\
Data File : VV035817.D
Acq On : 25 May 2024 23:21
Operator : SY/MD
Sample : P2586-10
Misc : 5.1g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4D21

Manual IntegrationsAPPROVED

Quant Time: May 27 05:33:12 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 27 05:15:54 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/28/2024
Supervised By :Mahesh Dadoda 05/28/2024

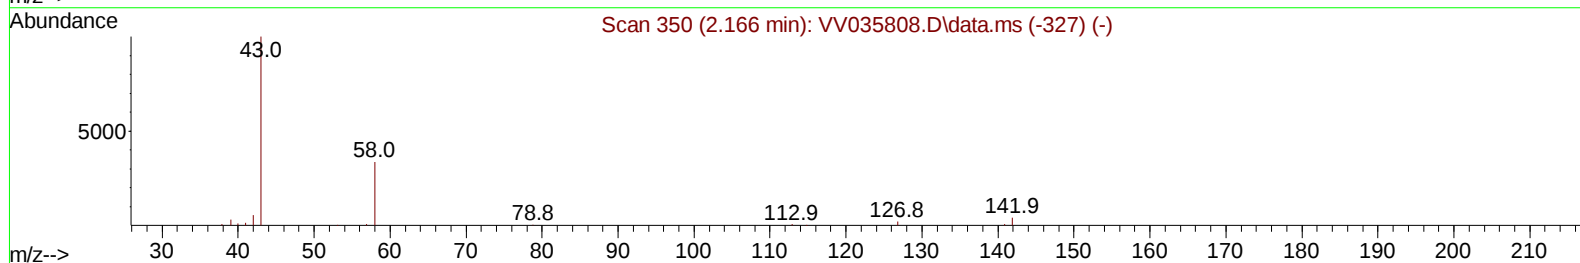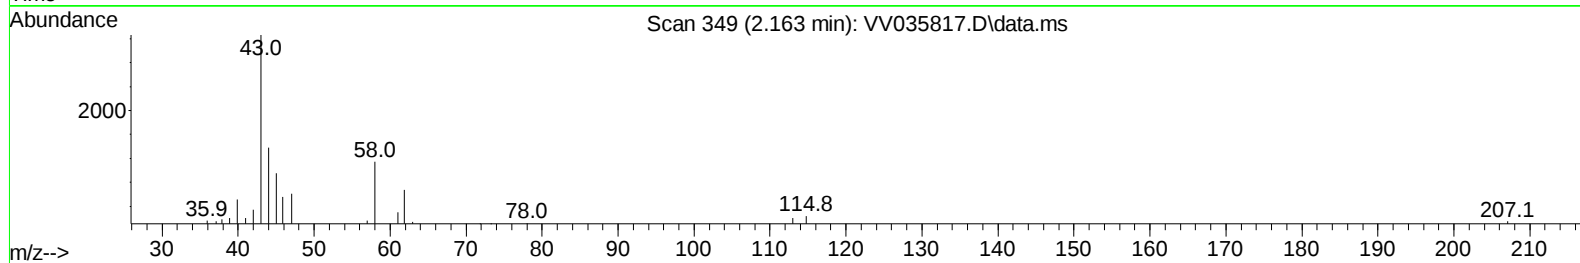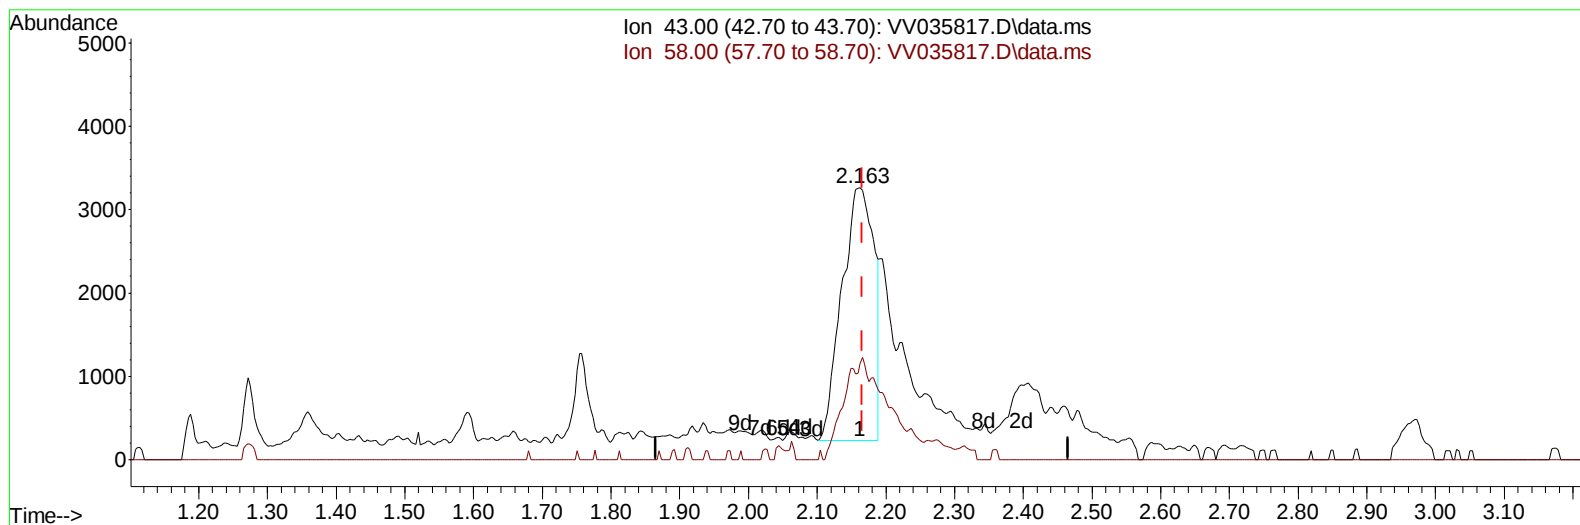

TIC: VV035817.D\data.ms

(13) Acetone (T)

2.163min (-0.003) 3.65 ug/L

response 9818

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	11.40	2.67
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052524\
Data File : VV035817.D
Acq On : 25 May 2024 23:21
Operator : SY/MD
Sample : P2586-10
Misc : 5.1g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4D21

Manual IntegrationsAPPROVED

Quant Time: May 27 05:33:12 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 27 05:15:54 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/28/2024
Supervised By :Mahesh Dadoda 05/28/2024

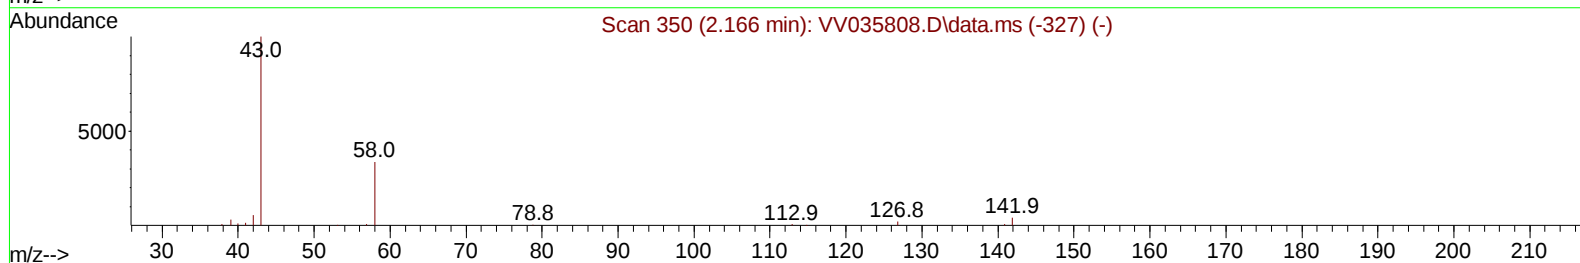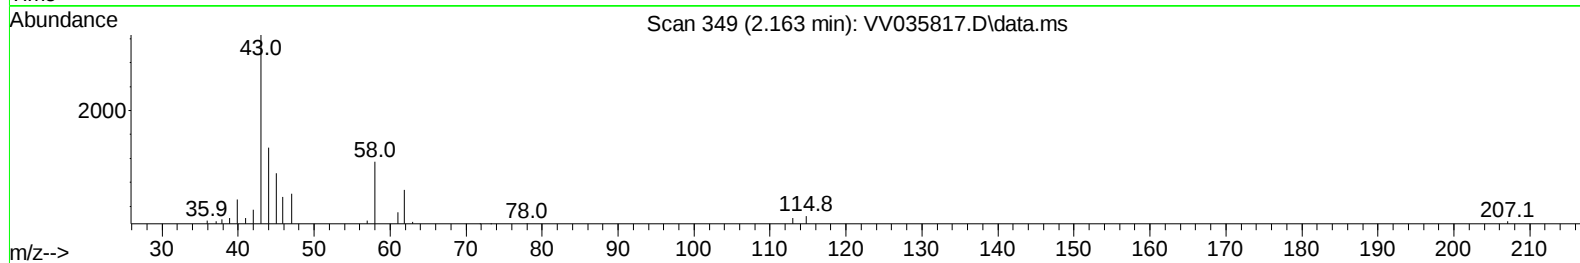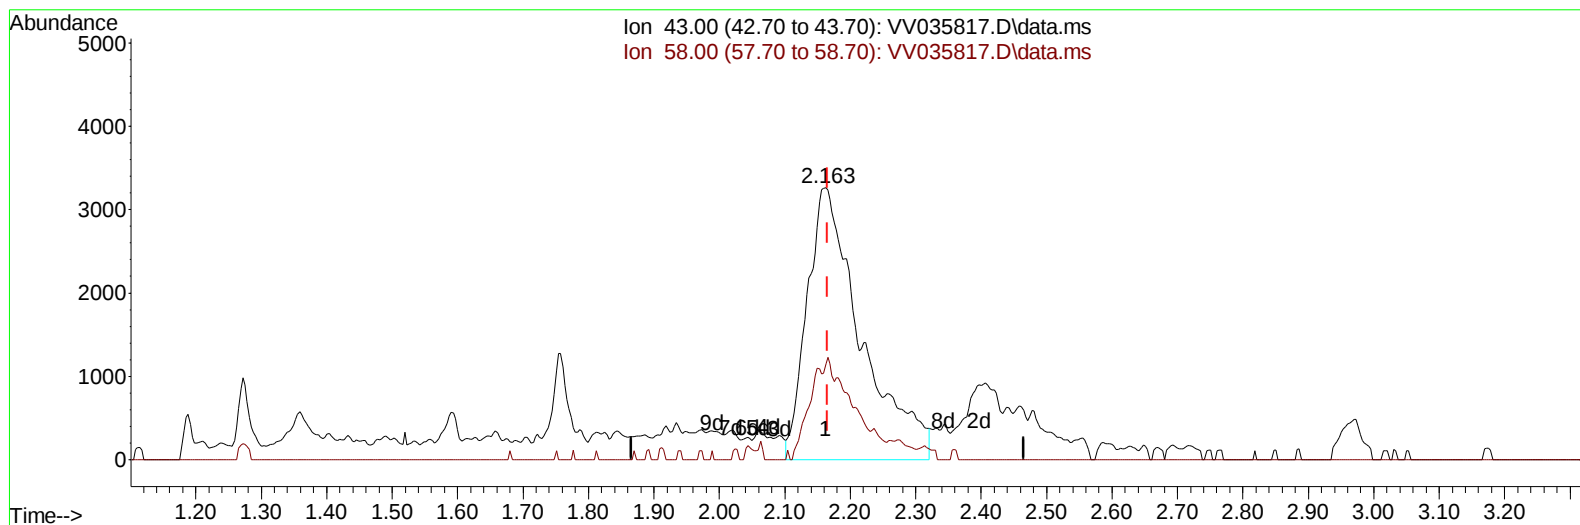

TIC: VV035817.D\data.ms

(13) Acetone (T)

2.163min (-0.003) 6.94 ug/L m

response 18677

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	11.40	1.40
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052524\
 Data File : VV035817.D
 Acq On : 25 May 2024 23:21
 Operator : SY/MD
 Sample : P2586-10
 Misc : 5.1g/10.0mL/MSVOA_V/SOIL/A
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4D21

Manual IntegrationsAPPROVED

Quant Time: May 27 05:33:12 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon May 27 05:15:54 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/28/2024
 Supervised By :Mahesh Dadoda 05/28/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.532	114		419014	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117		312775	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152		70354	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.272	65		177654	27.431	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	109.720%	
7) Chloroethane-d5	1.526	69		147992	28.325	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	113.320%	
11) 1,1-Dichloroethene-d2	2.050	65		74595	26.017	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	104.080%	
21) 2-Butanone-d5	3.851	46		46515	25.308	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	50.620%	
24) Chloroform-d	4.243	84		326514	26.211	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	104.840%	
26) 1,2-Dichloroethane-d4	4.937	65		172137	27.952	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	111.800%	
32) Benzene-d6	4.953	84		572679	33.449	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	133.800%	
36) 1,2-Dichloropropane-d6	5.986	67		201925	38.217	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	152.880%#	
41) Toluene-d8	7.243	98		405907	26.638	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	106.560%	
43) trans-1,3-Dichloroprop...	7.558	79		33158	14.674	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	58.680%	
47) 2-Hexanone-d5	8.040	63		15789	16.618	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	33.240%	
56) 1,1,2,2-Tetrachloroeth...	10.153	84		129939	25.521	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	102.080%	
66) 1,2-Dichlorobenzene-d4	11.561	152		65307	26.748	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	107.000%	
Target Compounds							
13) Acetone	2.163	43		18677m	6.942	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052524\
Data File : VV035817.D
Acq On : 25 May 2024 23:21
Operator : SY/MD
Sample : P2586-10
Misc : 5.1g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4D21

Manual IntegrationsAPPROVED

Quant Time: May 27 05:33:12 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 27 05:15:54 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/28/2024
Supervised By :Mahesh Dadoda 05/28/2024

