




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052524\
 Data File : VV035824.D
 Acq On : 26 May 2024 02:02
 Operator : SY/MD
 Sample : P2586-18
 Misc : 4.16g/10.0mL/MSVOA_V/SOIL/A
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4C38

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/28/2024
 Supervised By :Mahesh Dadoda 05/28/2024

Quant Time: May 27 05:34:52 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon May 27 05:15:54 2024
 Response via : Initial Calibration

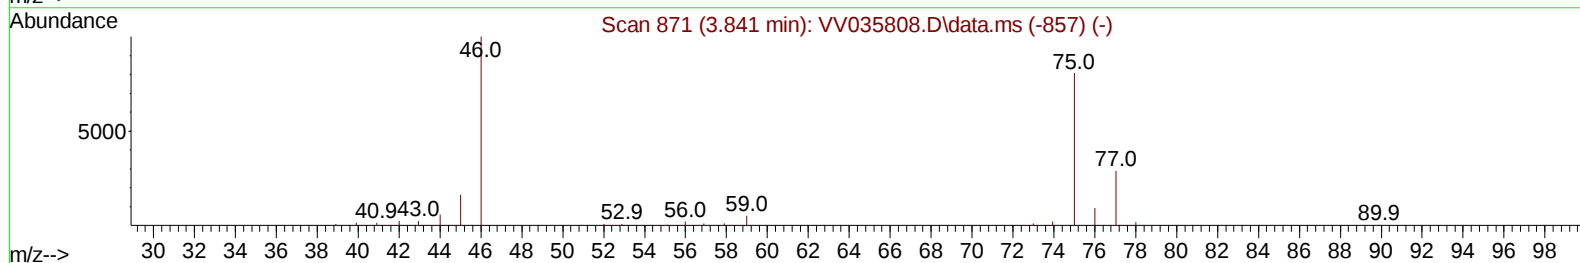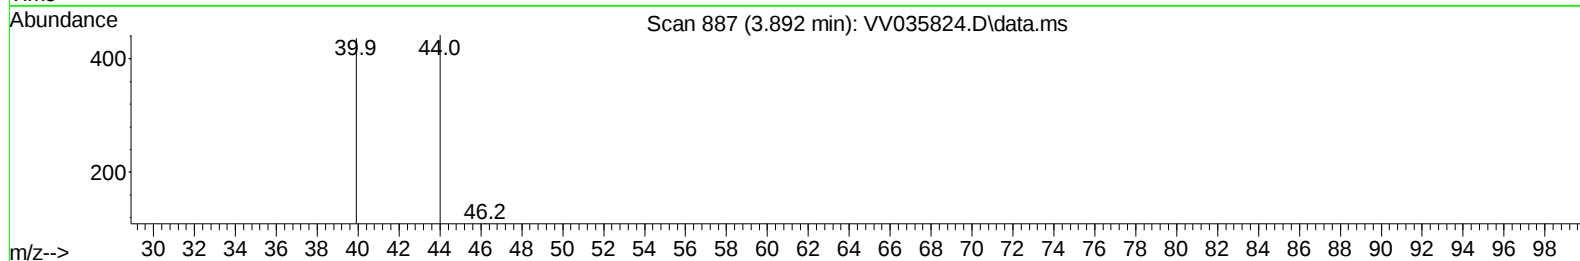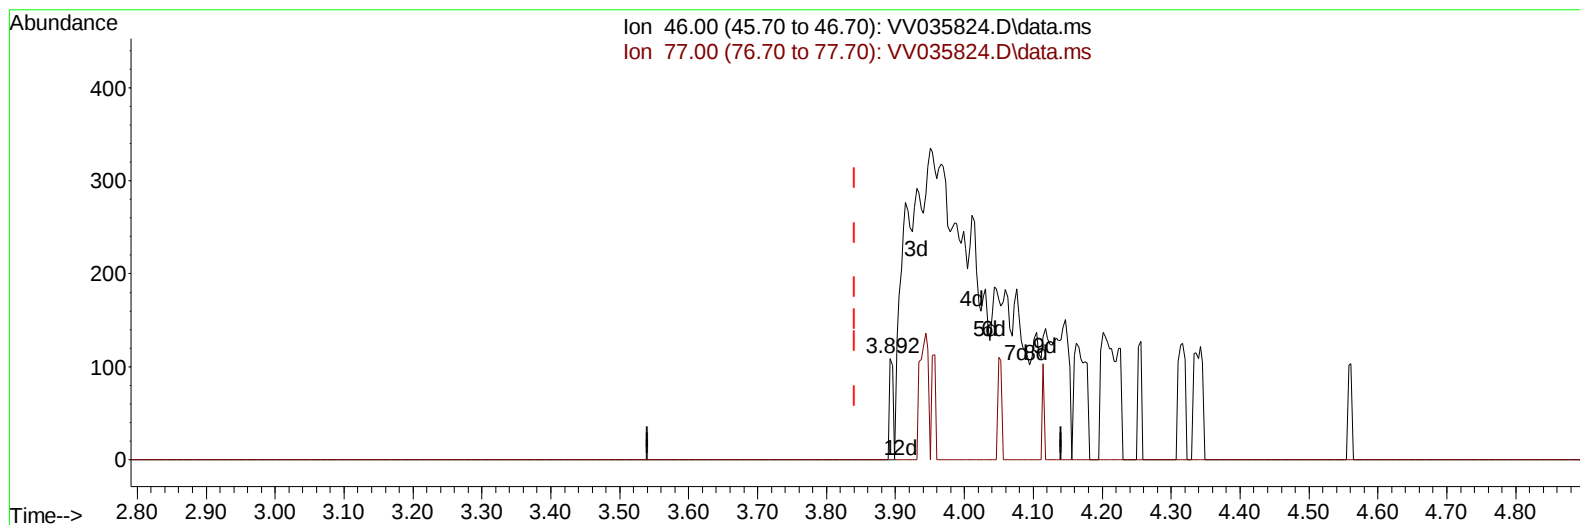

TIC: VV035824.D\data.ms

(21) 2-Butanone-d5 (S)

3.892min (+ 0.051) 0.43 ug/L

response 40

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	13.10	0.00#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052524\
Data File : VV035824.D
Acq On : 26 May 2024 02:02
Operator : SY/MD
Sample : P2586-18
Misc : 4.16g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4C38

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/28/2024
Supervised By :Mahesh Dadoda 05/28/2024

Quant Time: May 27 05:34:52 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 27 05:15:54 2024
Response via : Initial Calibration

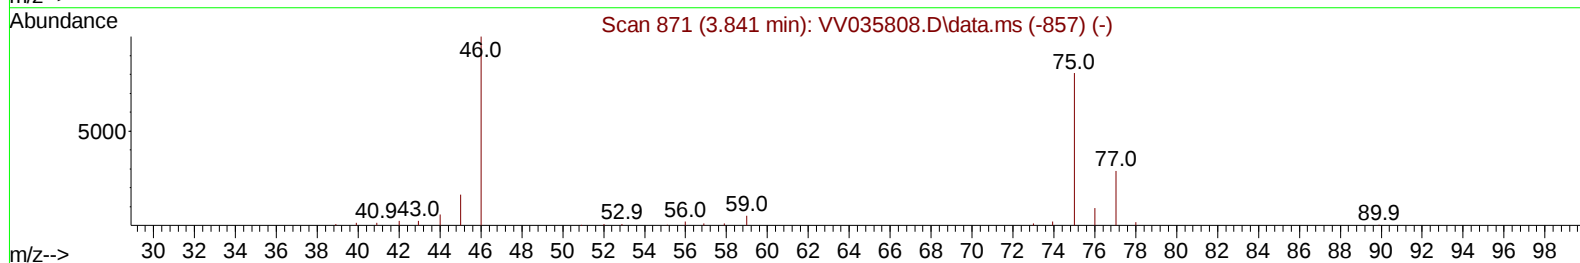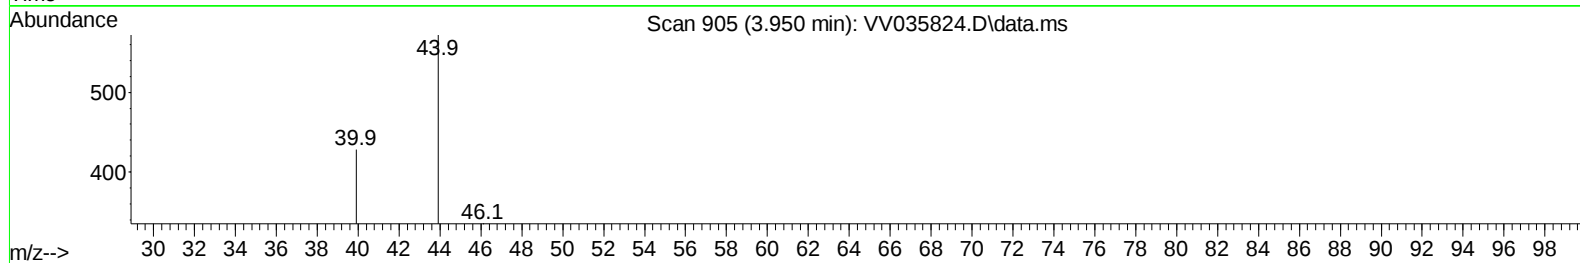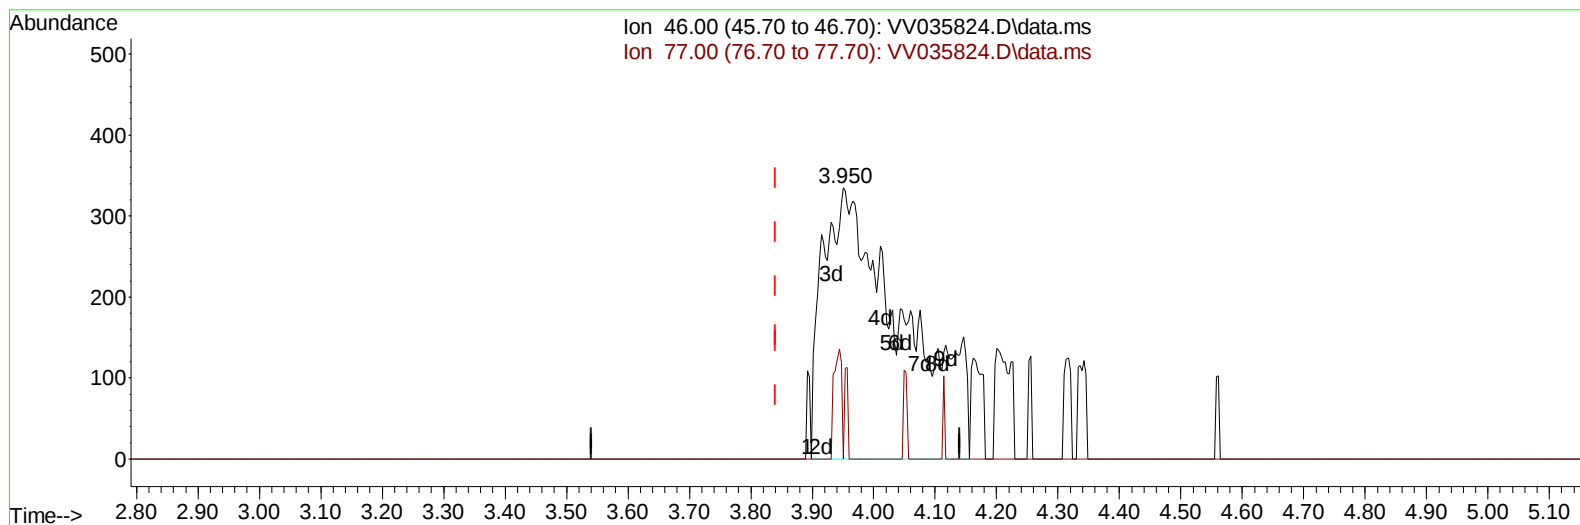

TIC: VV035824.D\data.ms

(21) 2-Butanone-d5 (S)

3.950min (+ 0.109) 32.42 ug/L m

response 3024

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	13.10	0.00#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052524\
Data File : VV035824.D
Acq On : 26 May 2024 02:02
Operator : SY/MD
Sample : P2586-18
Misc : 4.16g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4C38

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/28/2024
Supervised By :Mahesh Dadoda 05/28/2024

Quant Time: May 27 05:34:52 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 27 05:15:54 2024
Response via : Initial Calibration

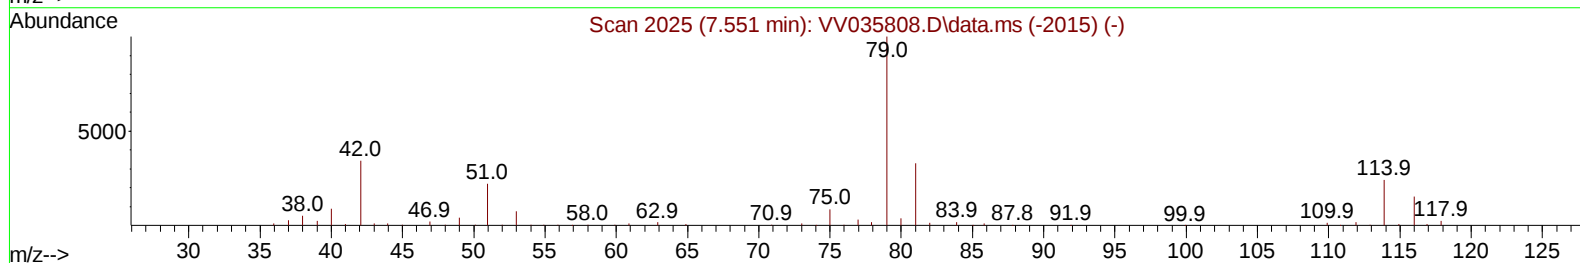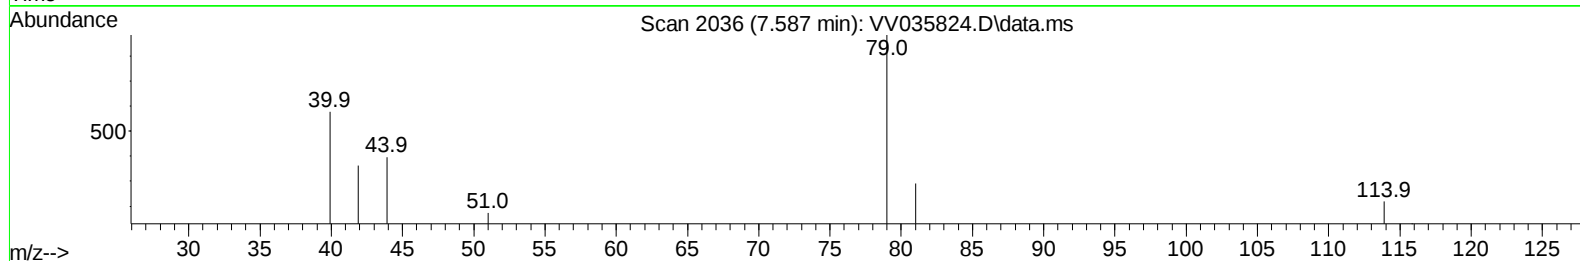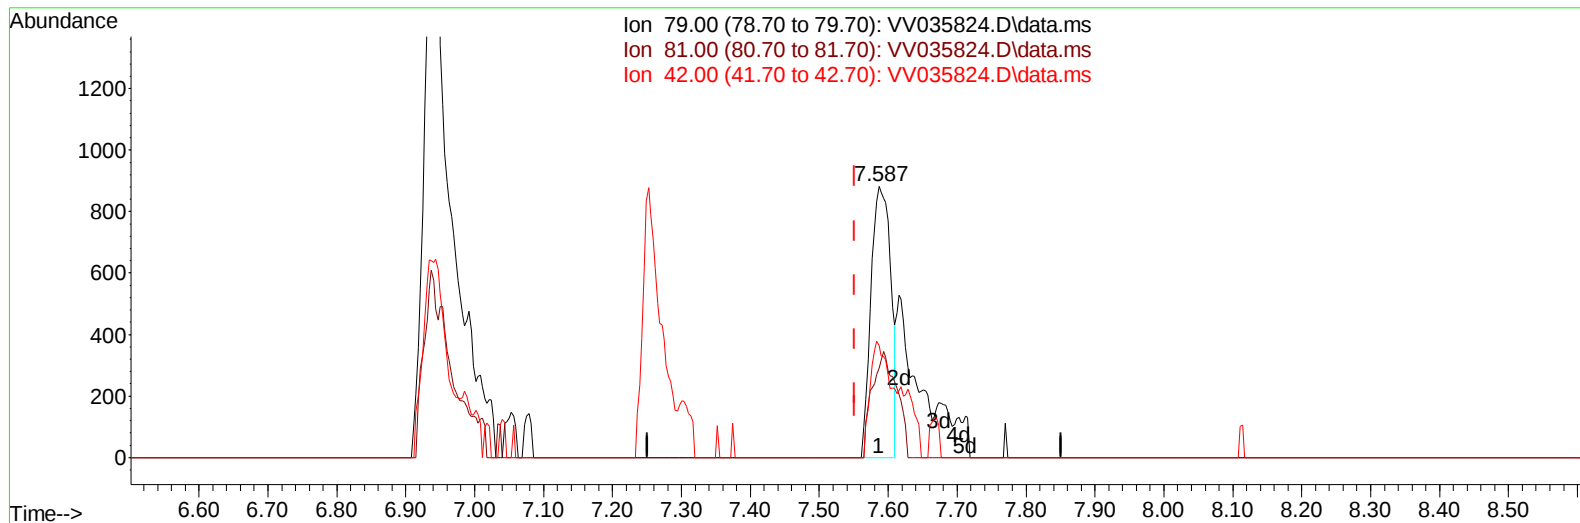

TIC: VV035824.D\data.ms

(43) trans-1,3-Dichloropropene-d4 (S)

7.587min (+ 0.035) 8.75 ug/L

response 1750

Ion	Exp%	Act%
79.00	100.00	100.00
81.00	32.30	48.97#
42.00	33.30	37.09
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052524\
Data File : VV035824.D
Acq On : 26 May 2024 02:02
Operator : SY/MD
Sample : P2586-18
Misc : 4.16g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4C38

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/28/2024
Supervised By :Mahesh Dadoda 05/28/2024

Quant Time: May 27 05:34:52 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 27 05:15:54 2024
Response via : Initial Calibration

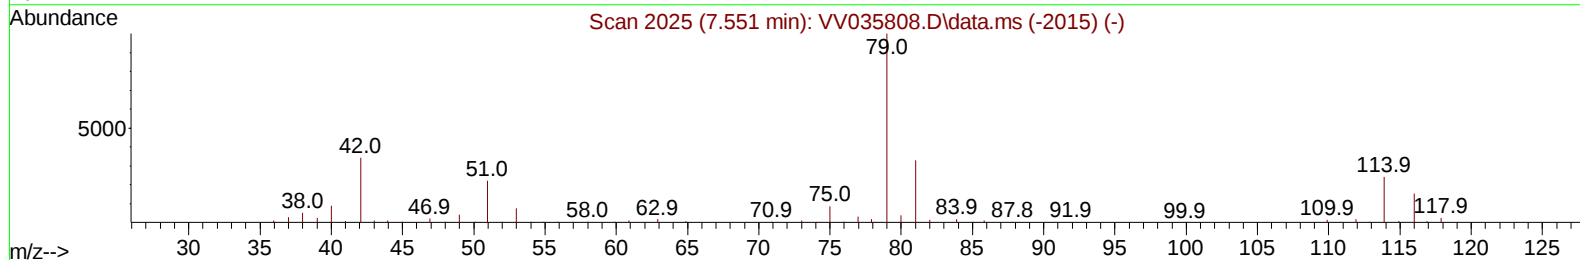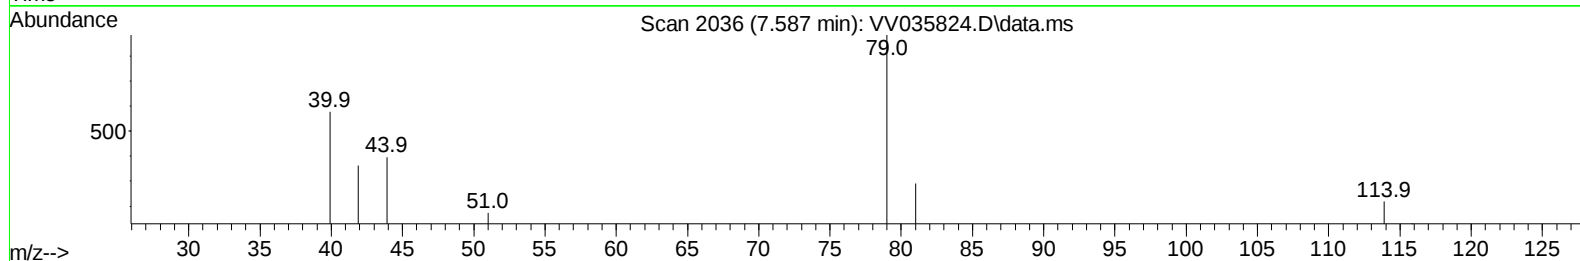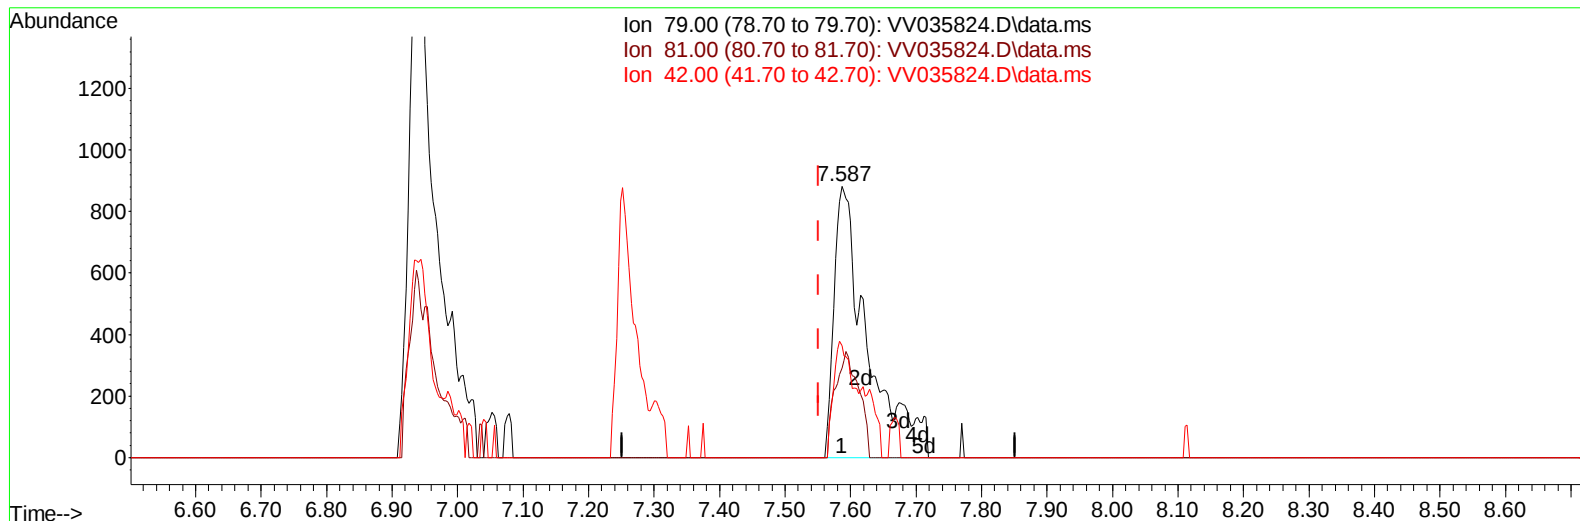

TIC: VV035824.D\data.ms

(43) trans-1,3-Dichloropropene-d4 (S)

7.587min (+ 0.035) 15.70 ug/L m

response 3140

Ion	Exp%	Act%
79.00	100.00	100.00
81.00	32.30	27.29
42.00	33.30	20.67#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052524\
Data File : VV035824.D
Acq On : 26 May 2024 02:02
Operator : SY/MD
Sample : P2586-18
Misc : 4.16g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4C38

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/28/2024
Supervised By :Mahesh Dadoda 05/28/2024

Quant Time: May 27 05:34:52 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 27 05:15:54 2024
Response via : Initial Calibration

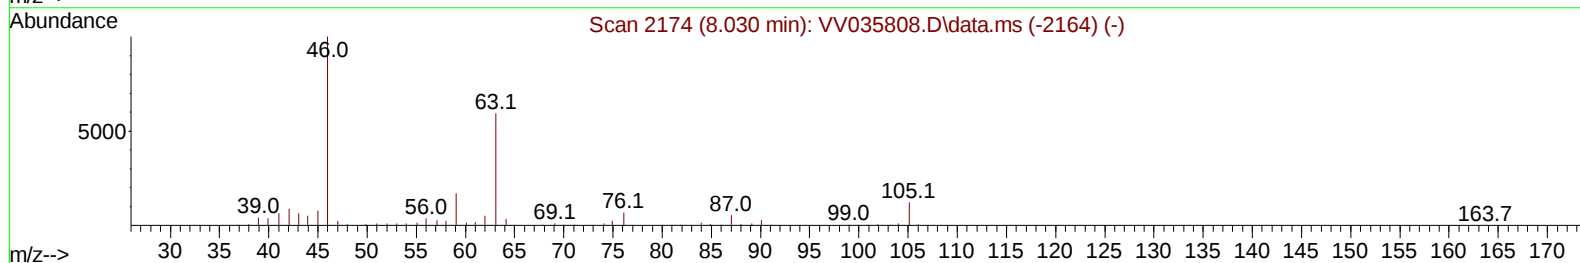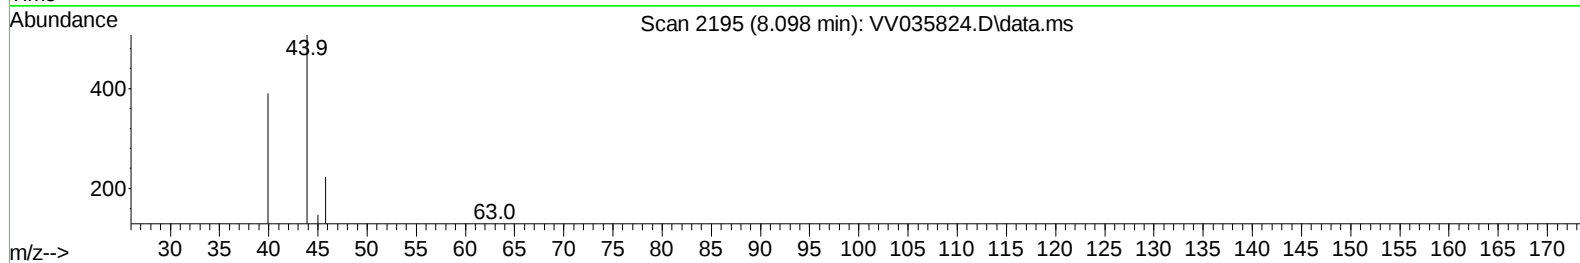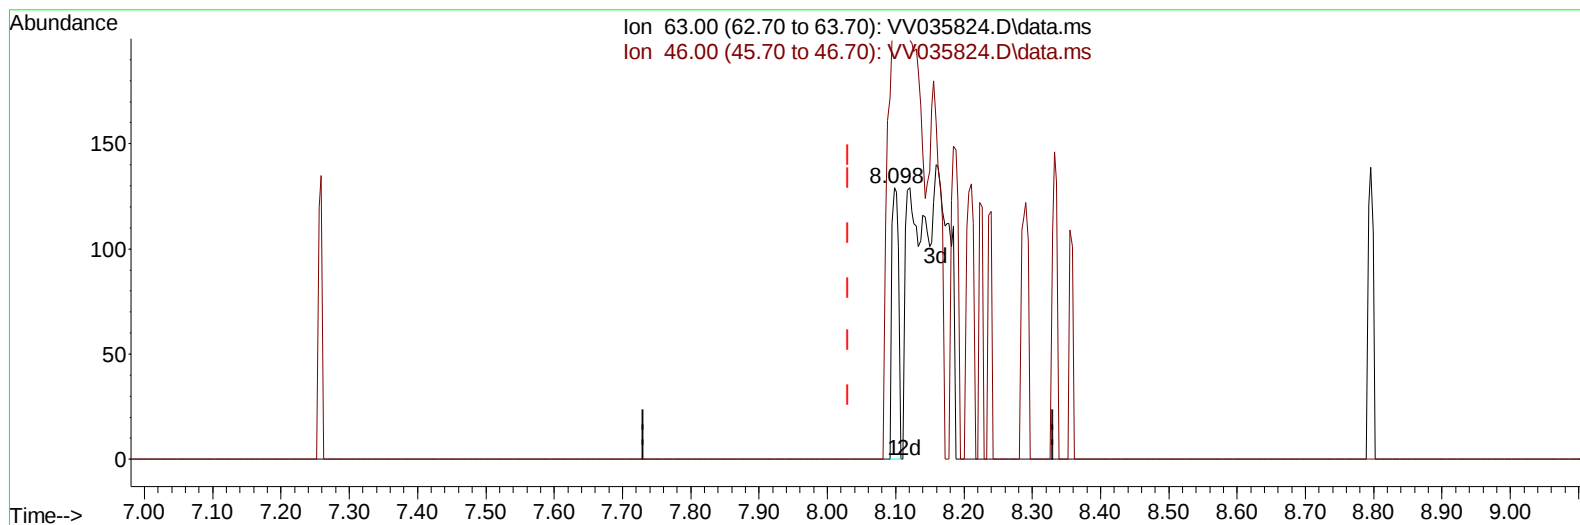

TIC: VV035824.D\data.ms

(47) 2-Hexanone-d5 (S)

8.098min (+ 0.068) 1.07 ug/L

response 90

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	161.70	785.56#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052524\
 Data File : VV035824.D
 Acq On : 26 May 2024 02:02
 Operator : SY/MD
 Sample : P2586-18
 Misc : 4.16g/10.0mL/MSVOA_V/SOIL/A
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4C38

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/28/2024
 Supervised By :Mahesh Dadoda 05/28/2024

Quant Time: May 27 05:34:52 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon May 27 05:15:54 2024
 Response via : Initial Calibration

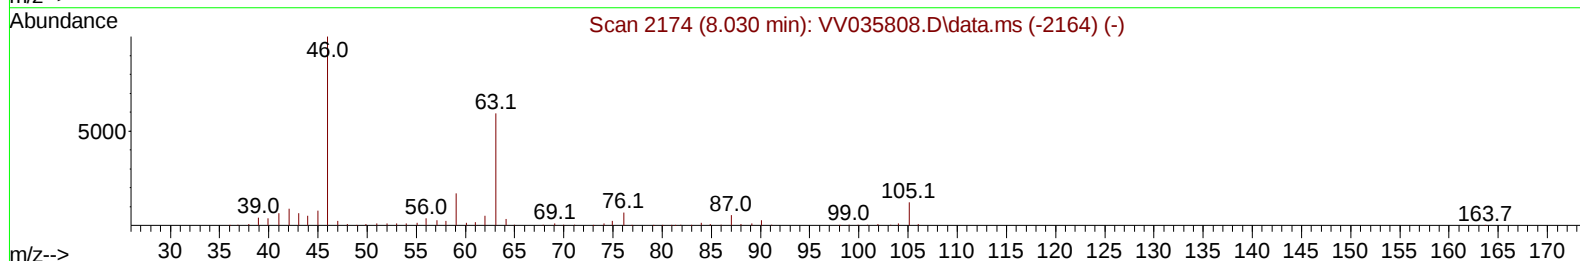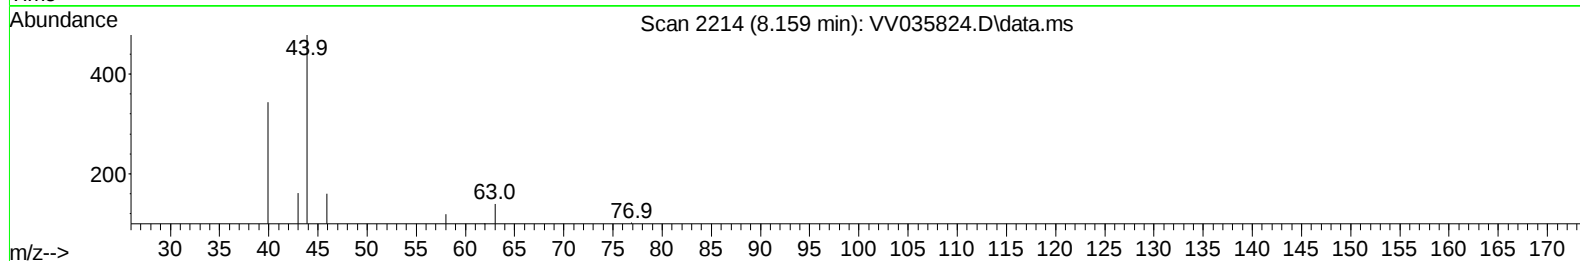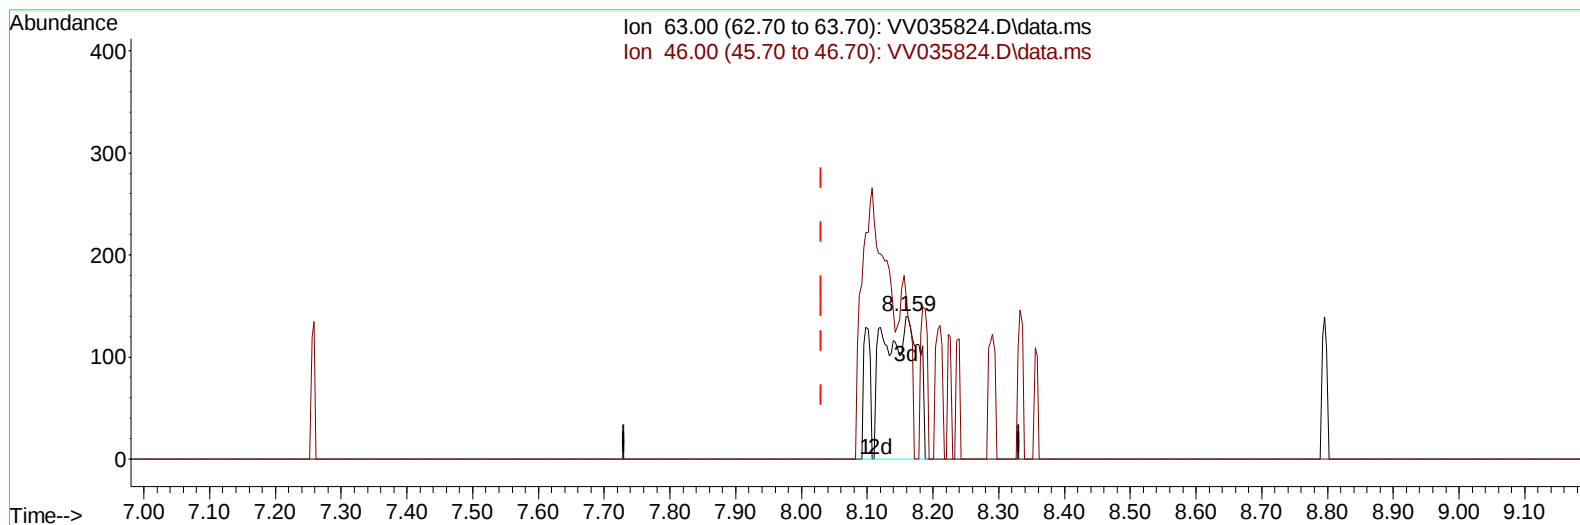

TIC: VV035824.D\data.ms

(47) 2-Hexanone-d5 (S)

8.159min (+ 0.129) 7.16 ug/L m

response 602

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	161.70	117.44
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052524\
 Data File : VV035824.D
 Acq On : 26 May 2024 02:02
 Operator : SY/MD
 Sample : P2586-18
 Misc : 4.16g/10.0mL/MSVOA_V/SOIL/A
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4C38

Manual IntegrationsAPPROVED

Quant Time: May 27 05:34:52 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon May 27 05:15:54 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/28/2024
 Supervised By :Mahesh Dadoda 05/28/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.551	114	21262	25.000	ug/L	0.02
28) Chlorobenzene-d5	8.792	117	27681	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	11953	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	5448	16.578	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery =	66.320%		
7) Chloroethane-d5	1.532	69	6220	23.461	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery =	93.840%		
11) 1,1-Dichloroethene-d2	2.060	65	2475	17.012	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery =	68.040%		
21) 2-Butanone-d5	3.950	46	3024m	32.425	ug/L	0.11
Spiked Amount 50.000	Range 20	- 135	Recovery =	64.840%		
24) Chloroform-d	4.256	84	16521	26.136	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery =	104.560%		
26) 1,2-Dichloroethane-d4	4.960	65	10383	33.227	ug/L	0.02
Spiked Amount 25.000	Range 70	- 130	Recovery =	132.920%#		
32) Benzene-d6	4.969	84	25894	17.089	ug/L	0.02
Spiked Amount 25.000	Range 20	- 135	Recovery =	68.360%		
36) 1,2-Dichloropropane-d6	5.998	67	10452	22.352	ug/L	0.01
Spiked Amount 25.000	Range 70	- 120	Recovery =	89.400%		
41) Toluene-d8	7.256	98	19093	14.158	ug/L	0.02
Spiked Amount 25.000	Range 30	- 130	Recovery =	56.640%		
43) trans-1,3-Dichloroprop...	7.587	79	3140m	15.701	ug/L	0.04
Spiked Amount 25.000	Range 30	- 135	Recovery =	62.800%		
47) 2-Hexanone-d5	8.159	63	602m	7.159	ug/L	0.13
Spiked Amount 50.000	Range 20	- 135	Recovery =	14.320%#		
56) 1,1,2,2-Tetrachloroeth...	10.156	84	7249	16.087	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery =	64.360%		
66) 1,2-Dichlorobenzene-d4	11.564	152	8387	20.218	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery =	80.880%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052524\
Data File : VV035824.D
Acq On : 26 May 2024 02:02
Operator : SY/MD
Sample : P2586-18
Misc : 4.16g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4C38

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/28/2024
Supervised By :Mahesh Dadoda 05/28/2024

Quant Time: May 27 05:34:52 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 27 05:15:54 2024
Response via : Initial Calibration

