

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052524\
 Data File : VV035822.D
 Acq On : 26 May 2024 01:16
 Operator : SY/MD
 Sample : P2586-16
 Misc : 4.69g/10.0mL/MSVOA_V/SOIL/A
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4C31

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/28/2024
 Supervised By :Mahesh Dadoda 05/28/2024

Quant Time: May 27 05:34:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon May 27 05:15:54 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	527582	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	426238	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	129065	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.272	65	162339	19.908	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	79.640%		
7) Chloroethane-d5	1.526	69	138711	21.086	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	84.360%		
11) 1,1-Dichloroethene-d2	2.053	65	67425	18.677	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	74.720%		
21) 2-Butanone-d5	3.883	46	24550m	10.609	ug/L	0.04
Spiked Amount 50.000	Range 20 - 135		Recovery =	21.220%		
24) Chloroform-d	4.243	84	302710	19.300	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	77.200%		
26) 1,2-Dichloroethane-d4	4.941	65	165918	21.398	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	85.600%		
32) Benzene-d6	4.957	84	523497	22.437	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	89.760%		
36) 1,2-Dichloropropane-d6	5.985	67	184228	25.586	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	102.360%		
41) Toluene-d8	7.243	98	384014	18.493	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	73.960%		
43) trans-1,3-Dichloroprop...	7.561	79	27490	8.927	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	35.720%		
47) 2-Hexanone-d5	8.088	63	2361m	1.824	ug/L	0.06
Spiked Amount 50.000	Range 20 - 135		Recovery =	3.640%#		
56) 1,1,2,2-Tetrachloroeth...	10.153	84	117303	16.906	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	67.640%		
66) 1,2-Dichlorobenzene-d4	11.558	152	75177	16.784	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	67.120%#		
Target Compounds					Qvalue	
13) Acetone	2.166	43	22150m	6.539	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052524\
Data File : VV035822.D
Acq On : 26 May 2024 01:16
Operator : SY/MD
Sample : P2586-16
Misc : 4.69g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 44 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
A4C31

Quant Time: May 27 05:34:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 27 05:15:54 2024
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 05/28/2024
Supervised By :Mahesh Dadoda 05/28/2024

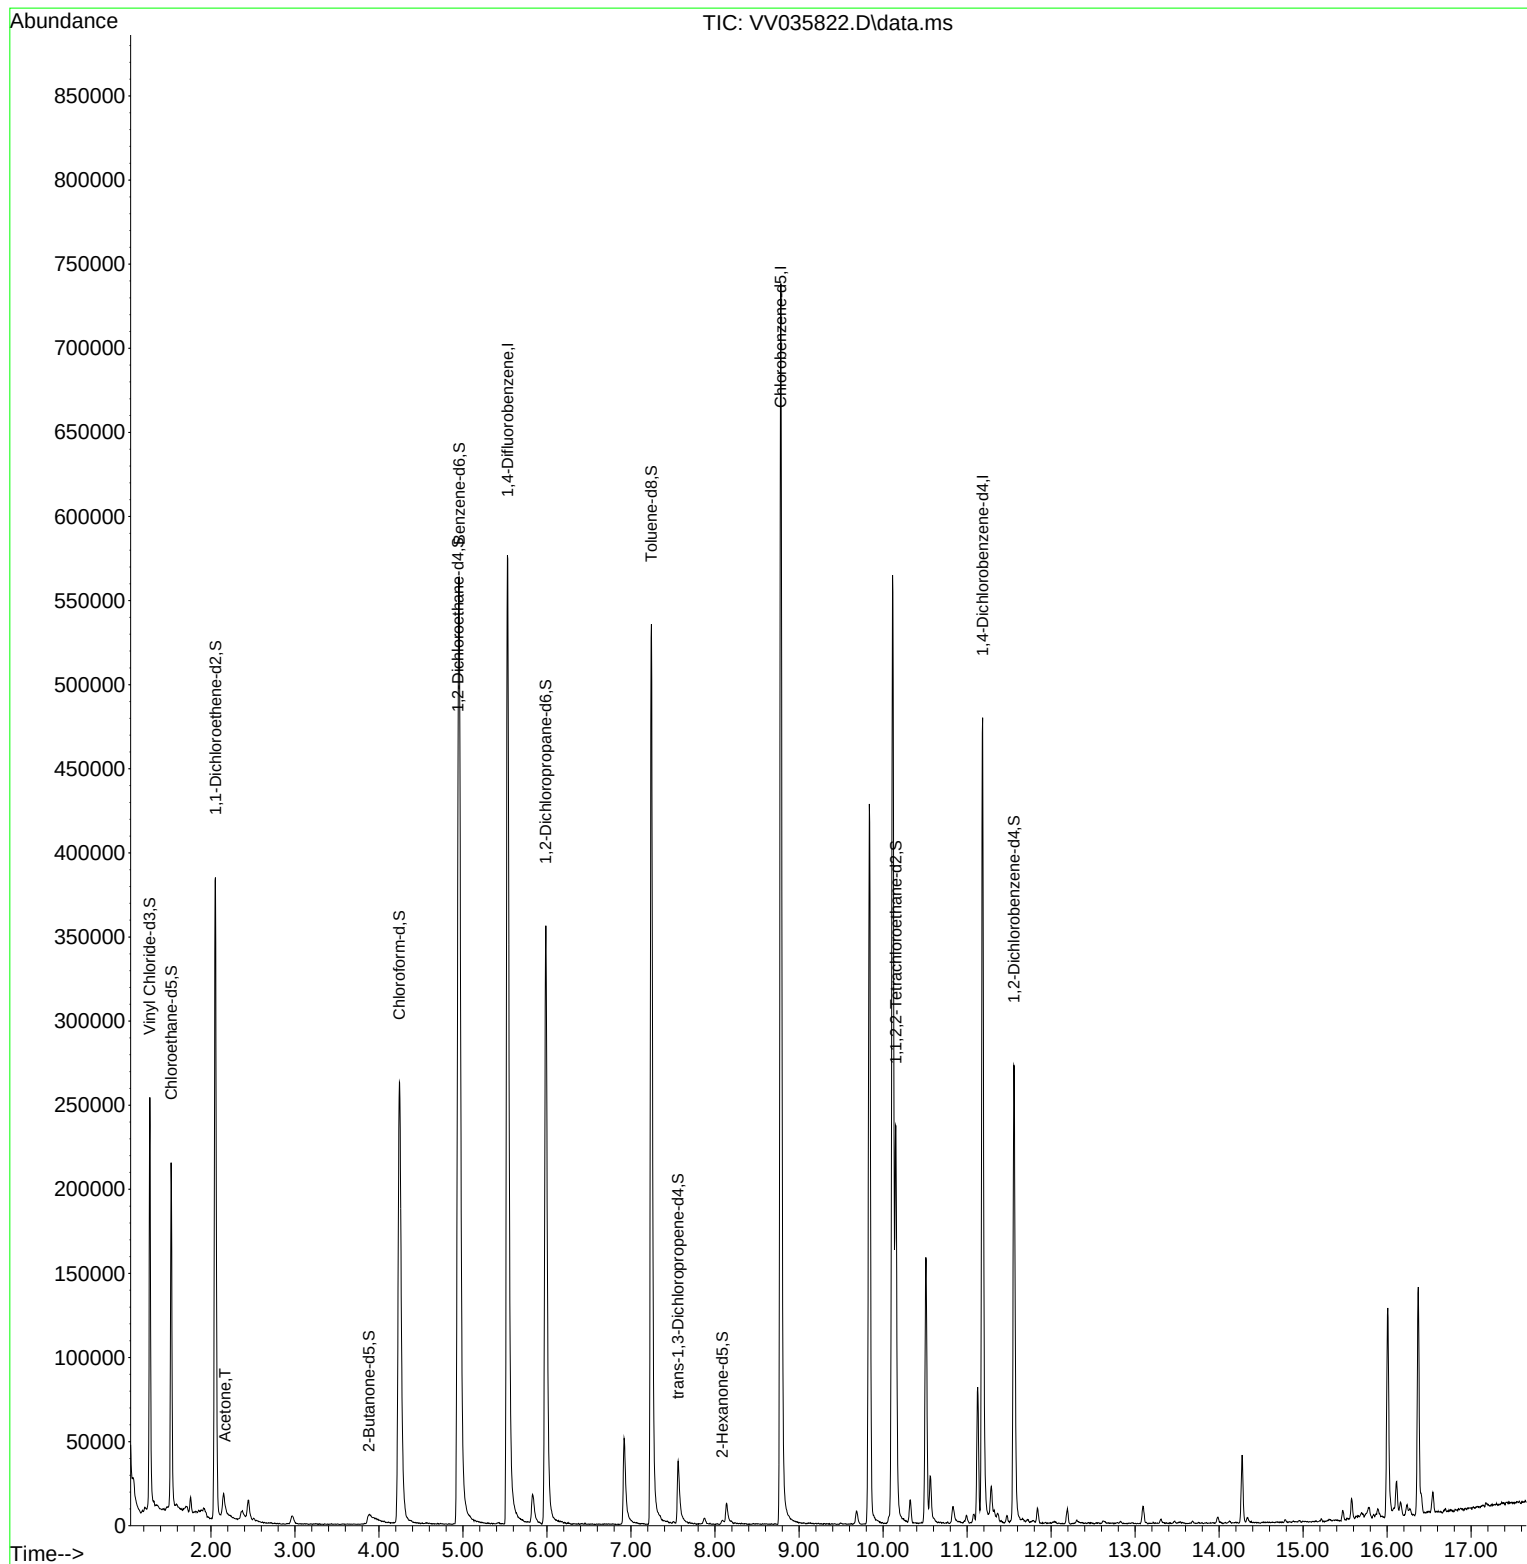

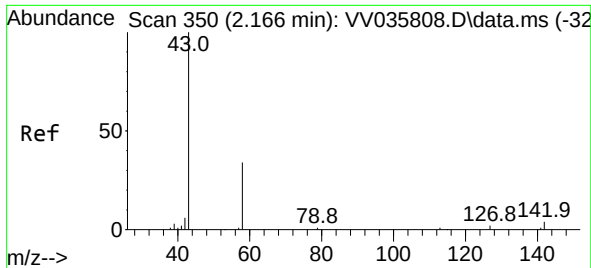

#13
Acetone
Concen: 6.539 ug/L m
RT: 2.166 min Scan# 31
Delta R.T. 0.000 min
Lab File: VV035822.D
Acq: 26 May 2024 01:16

Instrument :
MSVOA_V
ClientSampleId :
A4C31

Tgt Ion: 43 Resp: 22150
Ion Ratio Lower Upper
43 100
58 9.4 0.0 22.8

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 05/28/2024
Supervised By :Mahesh Dadoda 05/28/2024

