
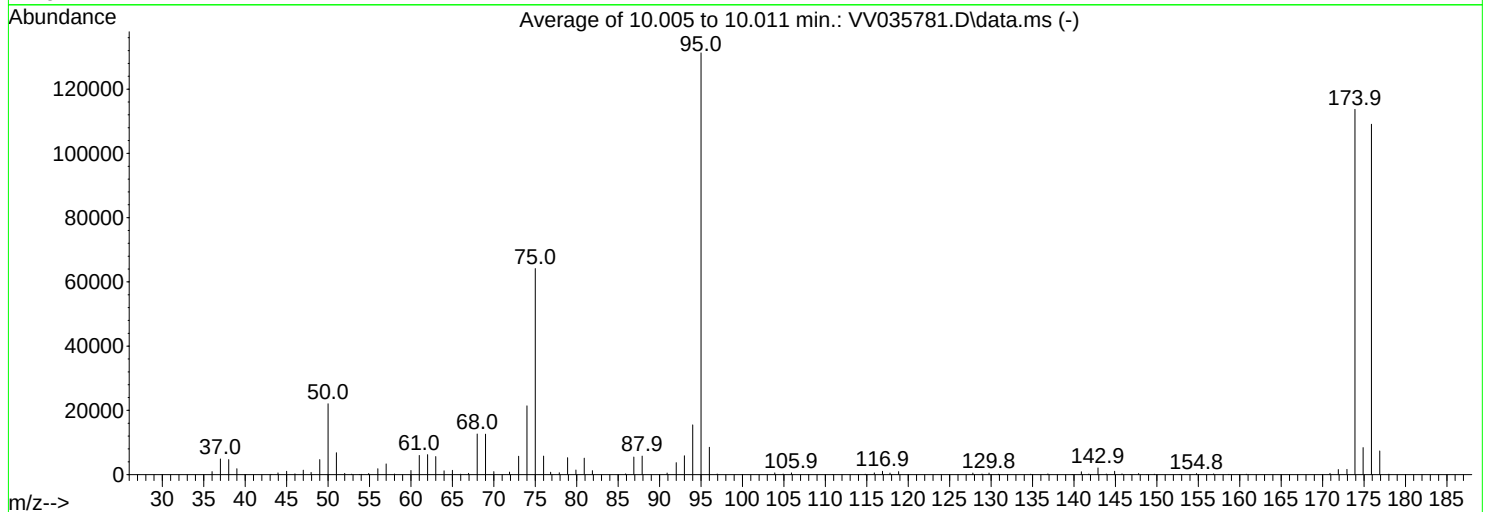


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV052524\
Data File : VV035781.D
Acq On : 25 May 2024 08:38
Operator : SY/MD
Sample : BFB309
Misc : 5.00g/10.0mL/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB309

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050624SMA.M
Title : VOC Analysis
Last Update : Mon May 27 05:15:54 2024

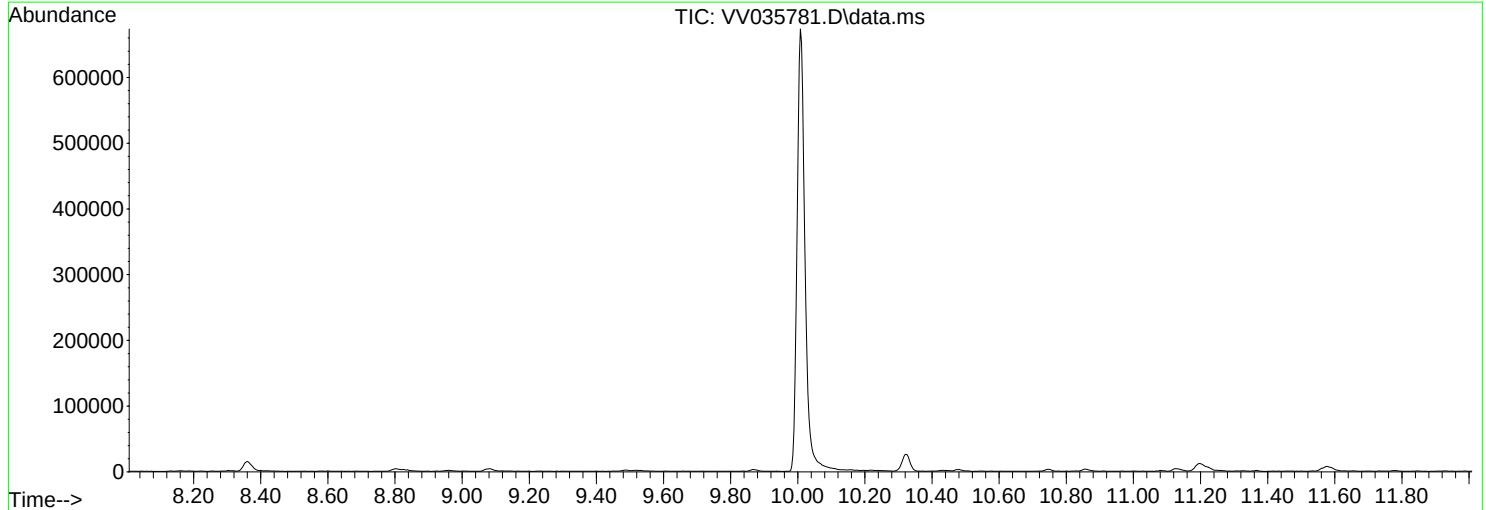

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2778

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.8	22059	PASS
75	95	30	80	48.8	64131	PASS
95	95	100	100	100.0	131304	PASS
96	95	5	9	6.5	8534	PASS
173	174	0.00	2	1.4	1628	PASS
174	95	50	120	86.6	113688	PASS
175	174	5	9	7.4	8447	PASS
176	174	95	101	95.9	109056	PASS
177	176	5	9	6.8	7377	PASS

m/z	Abundance
39.90	418.0
43.90	432.0
76.80	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB309

m/z	Abundance
36.00	849.0
37.00	4745.0
38.00	4566.0
39.00	1918.0
40.00	375.0
43.10	108.0
44.00	1013.0
45.00	975.0
46.00	281.0
47.00	1356.0
47.90	720.0
49.00	4673.0
50.00	21472.0
51.00	6787.0
52.00	421.0
52.80	156.0
53.80	127.0
54.90	393.0
56.00	1811.0
57.00	3107.0
58.00	179.0
60.00	1250.0
61.00	5951.0
62.00	6191.0
63.00	5528.0
64.00	1243.0
65.00	1264.0
66.00	165.0
66.90	398.0
68.00	12238.0
69.00	12132.0
70.00	907.0
71.90	832.0
73.00	5269.0
74.00	20872.0
75.00	62184.0
76.00	5834.0
76.90	863.0
77.90	549.0
78.90	5055.0
79.90	1442.0
80.90	4898.0
81.90	1223.0
85.90	196.0
86.90	5311.0
87.90	5570.0
90.90	487.0
92.00	3656.0
93.00	5751.0
94.00	14637.0
95.00	127792.0
96.00	8305.0
97.00	210.0
103.90	489.0
104.90	201.0
105.90	547.0
114.80	134.0
115.90	485.0
116.90	1069.0
117.80	488.0
118.90	930.0
127.80	470.0
128.90	167.0
129.80	505.0
131.00	165.0
134.80	156.0
136.90	230.0
140.90	772.0
141.80	210.0
142.90	2040.0
144.00	182.0
144.90	1043.0
145.80	248.0
147.80	354.0
148.80	127.0
149.70	132.0
152.80	111.0
154.80	326.0
156.80	251.0
160.90	169.0
170.90	487.0
171.90	1497.0
173.00	1533.0
173.90	107544.0
174.90	8263.0
175.90	102296.0
176.90	7060.0
178.00	141.0

Instrument :
MSVOA_V
ClientSampleId :
BFB309

m/z	Abundance
36.00	1004.0
37.00	5008.0
38.00	4832.0
39.00	1902.0
40.00	438.0
43.10	124.0
44.00	1002.0
45.00	1067.0
46.00	291.0
47.00	1461.0
48.00	746.0
49.00	4869.0
50.00	22864.0
51.00	7075.0
52.00	413.0
52.80	177.0
54.00	127.0
54.90	387.0
56.00	1900.0
57.00	3468.0
58.00	191.0
60.00	1358.0
61.00	6210.0
62.00	6480.0
63.00	5909.0
64.00	1256.0
65.00	1400.0
66.00	188.0
66.90	449.0
68.00	13172.0
69.00	13005.0
70.00	1006.0
71.90	813.0
73.00	5942.0
74.00	22136.0
75.00	66416.0
76.00	5941.0
76.90	898.0
77.90	635.0
78.90	5532.0
79.90	1517.0
80.90	5286.0
81.90	1329.0
85.90	282.0
86.90	5679.0
87.90	6071.0
90.90	535.0
92.00	3853.0
93.00	6114.0
94.00	16102.0
95.00	135808.0
96.00	8720.0
97.00	223.0
103.90	565.0
104.90	228.0
105.90	582.0
114.80	126.0
115.90	553.0
116.90	1079.0
117.80	526.0
118.80	984.0
127.80	517.0
128.90	242.0
129.70	508.0
130.90	159.0
134.80	162.0
136.80	251.0
139.80	103.0
140.90	914.0
141.80	209.0
142.90	2154.0
143.90	221.0
144.90	1108.0
145.80	266.0
146.80	104.0
147.80	346.0
149.70	153.0
152.80	139.0
154.80	339.0
156.90	292.0
158.70	127.0
160.80	138.0
170.90	438.0
171.90	1617.0
172.90	1714.0
173.90	117776.0
174.90	8760.0
175.90	112896.0
176.90	7655.0
178.00	145.0

Instrument :
MSVOA_V
ClientSampleId :
BFB309

m/z	Abundance
36.00	1025.0
37.00	4867.0
38.00	4619.0
39.00	1739.0
40.00	525.0
43.10	103.0
44.00	939.0
45.00	1049.0
46.00	235.0
47.00	1322.0
48.00	678.0
49.00	4538.0
50.00	21840.0
51.00	6645.0
52.00	342.0
52.90	178.0
54.10	132.0
54.90	324.0
56.00	1813.0
57.00	3472.0
58.00	179.0
60.00	1328.0
61.00	5809.0
62.00	6066.0
63.00	5529.0
64.00	1138.0
65.00	1435.0
66.00	156.0
67.00	436.0
68.00	12515.0
69.00	12729.0
70.00	914.0
71.90	698.0
73.00	5927.0
74.00	21312.0
75.00	63792.0
76.00	5535.0
76.90	885.0
77.90	675.0
78.90	5264.0
79.90	1416.0
80.90	5179.0
81.90	1199.0
85.90	335.0
86.90	5409.0
87.90	5671.0
90.90	547.0
92.00	3718.0
93.00	5743.0
94.00	15756.0
95.00	130312.0
96.00	8577.0
96.90	227.0
103.90	621.0
104.90	223.0
105.90	581.0
108.00	112.0
110.90	117.0
114.80	123.0
115.90	574.0
116.90	968.0
117.80	462.0
118.80	960.0
127.80	496.0
128.90	262.0
129.70	487.0
130.80	140.0
134.80	145.0
136.80	273.0
139.80	100.0
140.90	1056.0
141.80	158.0
142.90	2114.0
143.80	250.0
144.90	1084.0
145.80	244.0
146.80	125.0
147.80	298.0
149.70	137.0
152.80	130.0
154.80	378.0
156.90	287.0
158.70	148.0
160.70	133.0
170.90	357.0
171.90	1618.0
172.90	1638.0
173.90	115744.0
174.90	8319.0
175.90	111976.0
176.90	7415.0
178.00	148.0

Instrument :
MSVOA_V
ClientSampleId :
BFB309