




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053024\
 Data File : VV035911.D
 Acq On : 30 May 2024 21:20
 Operator : SY/MD
 Sample : P2659-12
 Misc : 4.13g/10.0mL/MSVOA_V/SOIL/A
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHC33

Manual IntegrationsAPPROVED

Quant Time: May 31 00:56:08 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 31 00:49:35 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/03/2024
 Supervised By :Semsettin Yesilyurt 06/03/2024

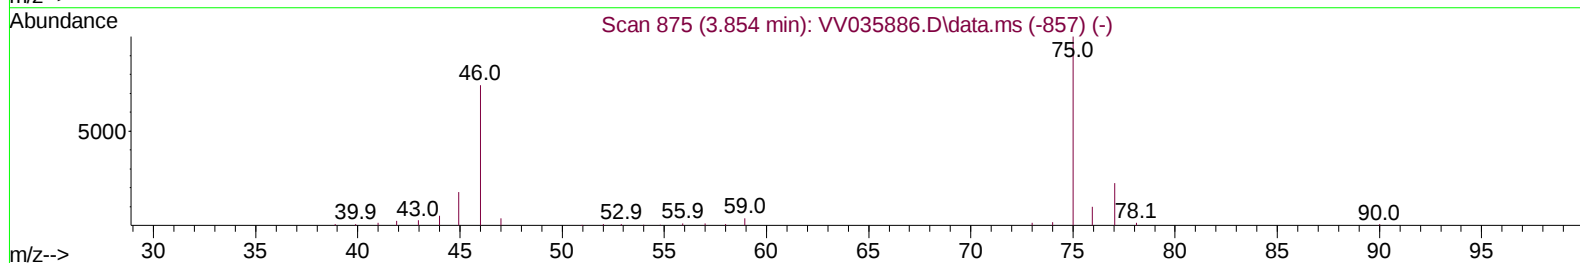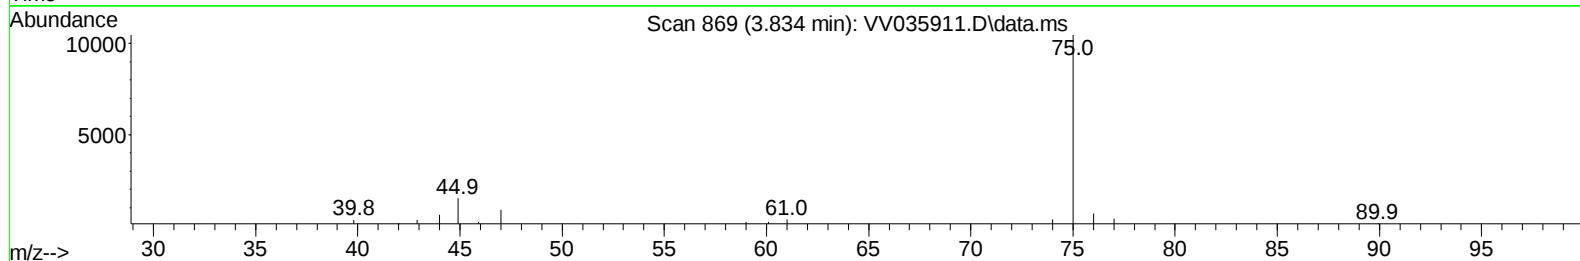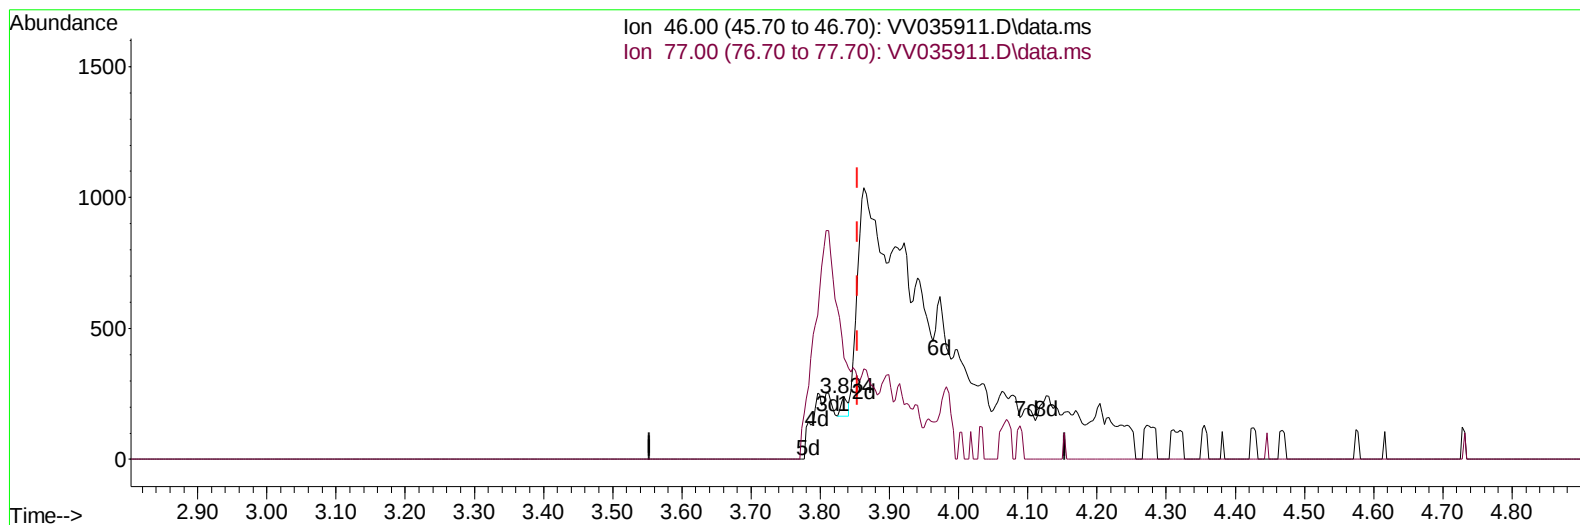

TIC: VV035911.D\data.ms

(21) 2-Butanone-d5 (S)

3.834min (-0.019) 0.31 ug/L

response 49

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	11.90	0.00#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053024\
Data File : VV035911.D
Acq On : 30 May 2024 21:20
Operator : SY/MD
Sample : P2659-12
Misc : 4.13g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHC33

Manual IntegrationsAPPROVED

Quant Time: May 31 00:56:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 31 00:49:35 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/03/2024
Supervised By :Semsettin Yesilyurt 06/03/2024

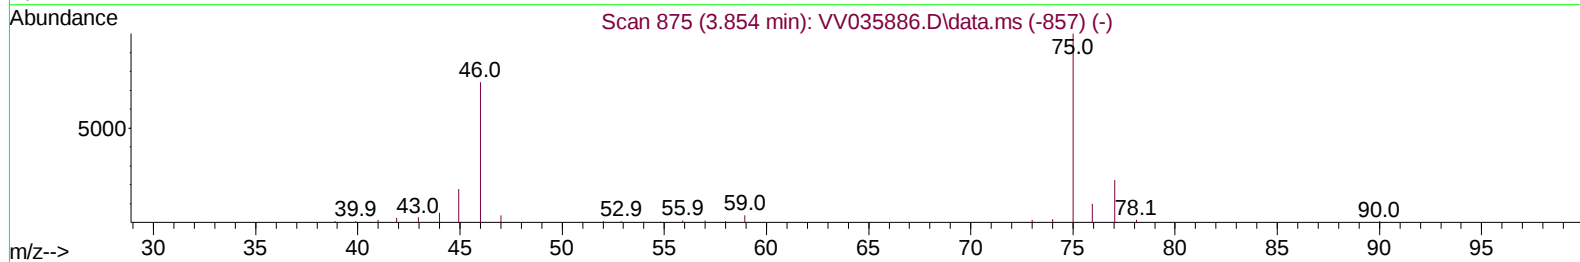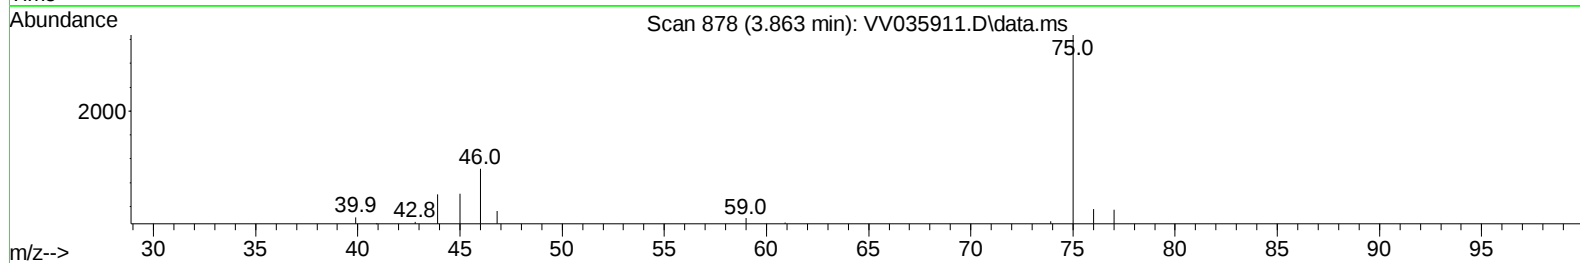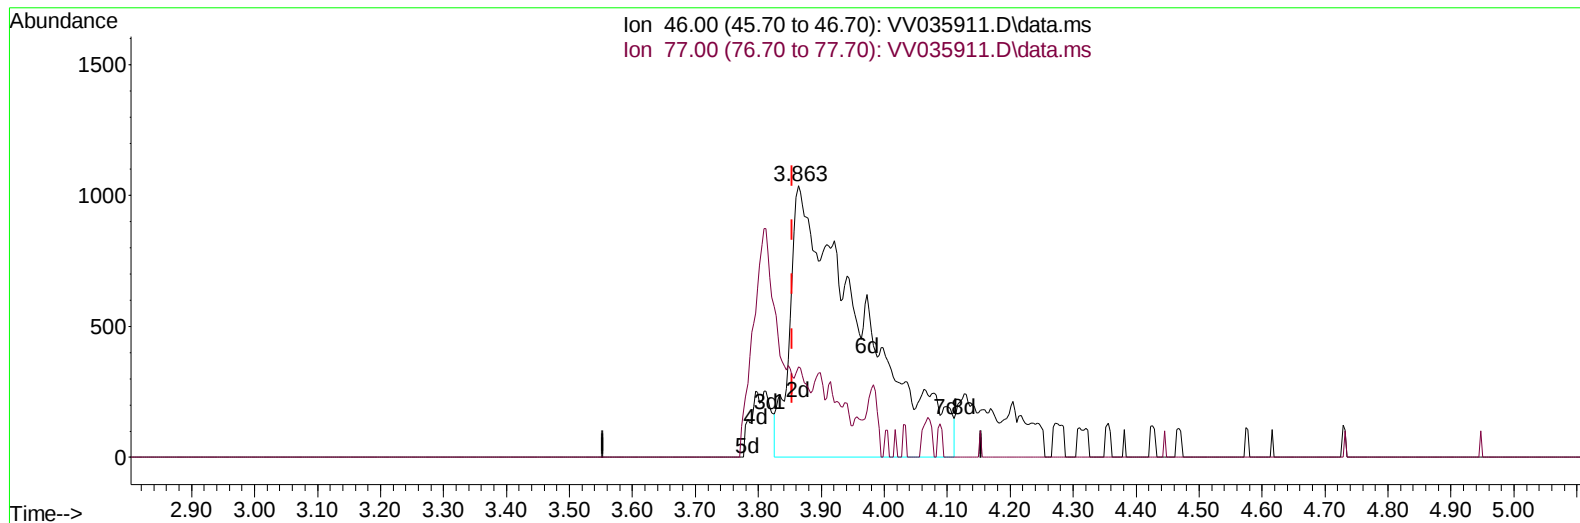

TIC: VV035911.D\data.ms

(21) 2-Butanone-d5 (S)

3.863min (+ 0.010) 51.95 ug/L m

response 8206

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	11.90	0.00#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053024\
Data File : VV035911.D
Acq On : 30 May 2024 21:20
Operator : SY/MD
Sample : P2659-12
Misc : 4.13g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHC33

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 06/03/2024
Supervised By :Semsettin Yesilyurt 06/03/2024

Quant Time: May 31 00:56:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 31 00:49:35 2024
Response via : Initial Calibration

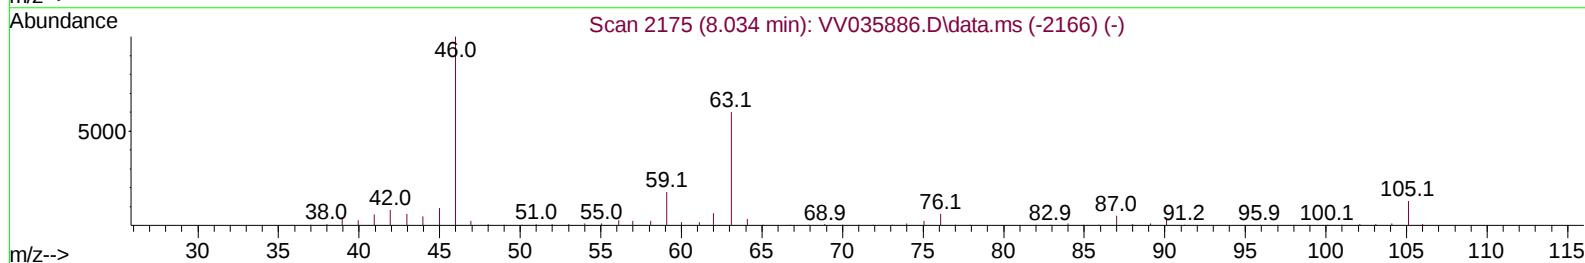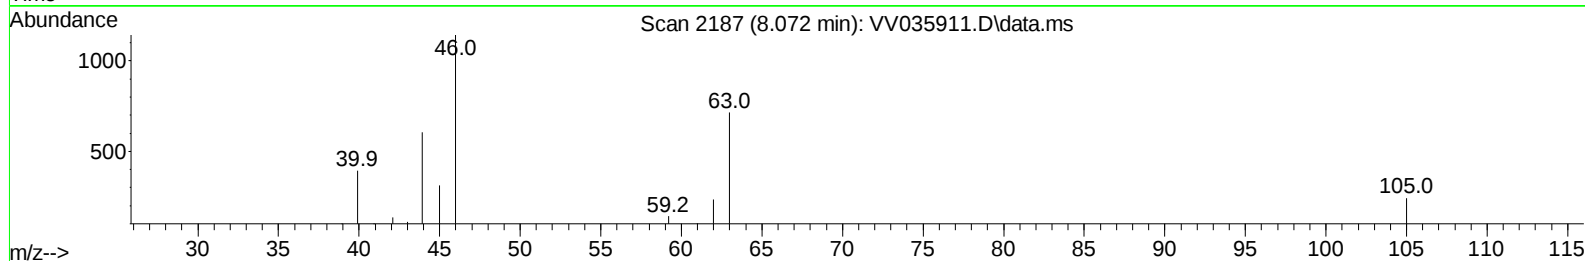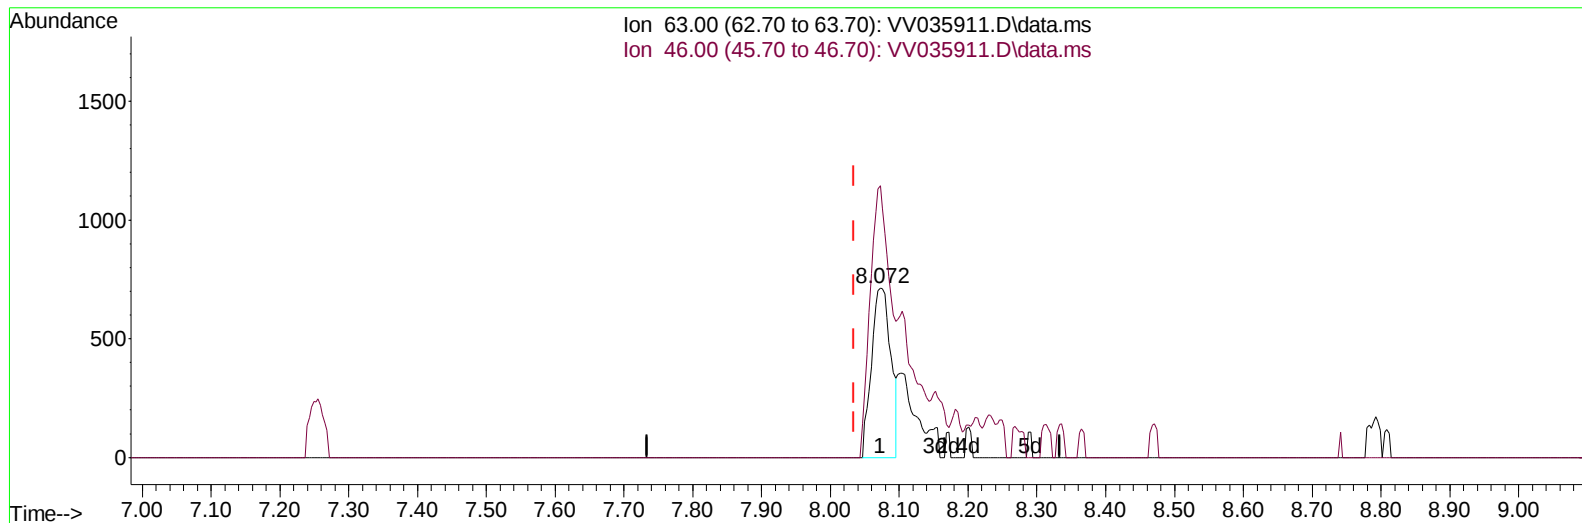

TIC: VV035911.D\data.ms

(47) 2-Hexanone-d5 (S)

8.072min (+ 0.039) 12.84 ug/L

response 1385

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	171.40	165.70
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053024\
Data File : VV035911.D
Acq On : 30 May 2024 21:20
Operator : SY/MD
Sample : P2659-12
Misc : 4.13g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHC33

Manual IntegrationsAPPROVED

Quant Time: May 31 00:56:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 31 00:49:35 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/03/2024
Supervised By :Semsettin Yesilyurt 06/03/2024

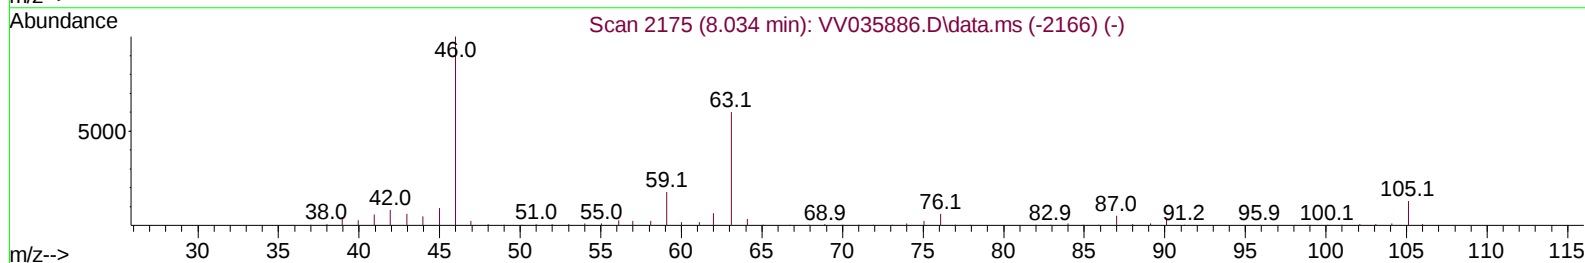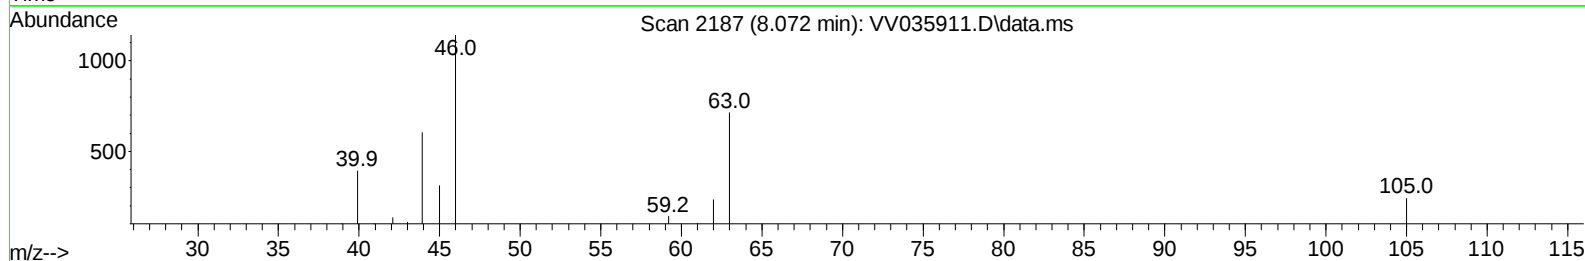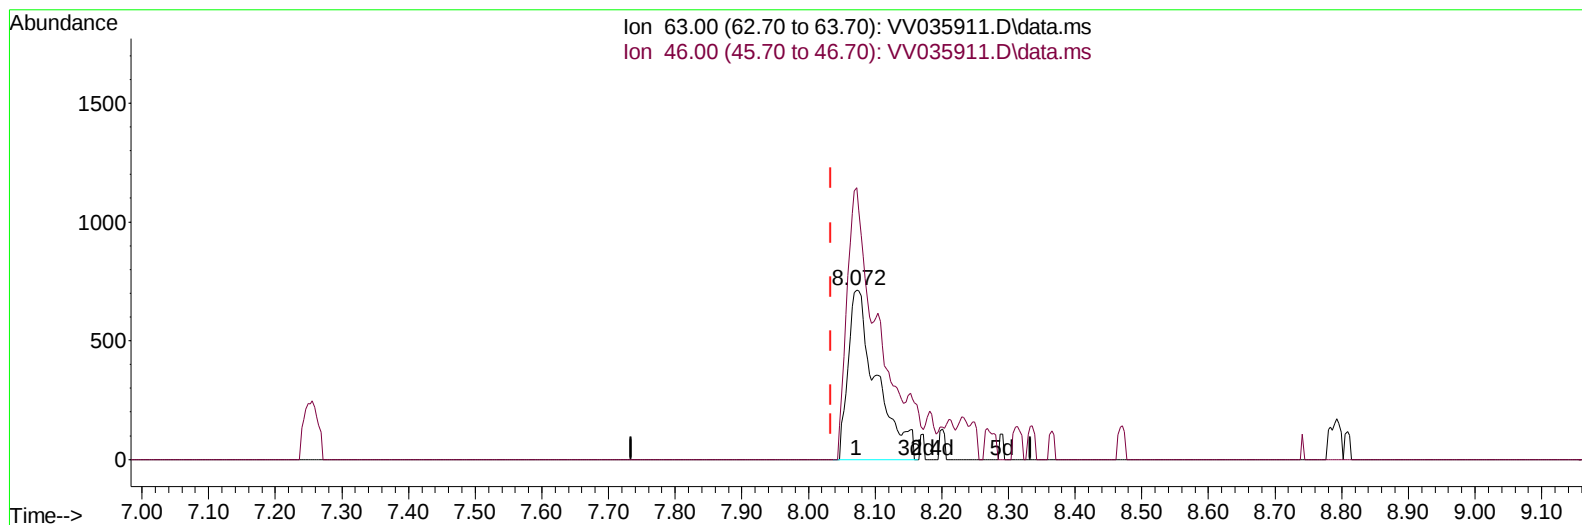

TIC: VV035911.D\data.ms

(47) 2-Hexanone-d5 (S)

8.072min (+ 0.039) 19.55 ug/L m

response 2109

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	171.40	108.82#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053024\
 Data File : VV035911.D
 Acq On : 30 May 2024 21:20
 Operator : SY/MD
 Sample : P2659-12
 Misc : 4.13g/10.0mL/MSVOA_V/SOIL/A
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHC33

Manual IntegrationsAPPROVED

Quant Time: May 31 00:56:08 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 31 00:49:35 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/03/2024
 Supervised By :Semsettin Yesilyurt 06/03/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.545	114		37446	25.000	ug/L	0.01
28) Chlorobenzene-d5	8.789	117		42531	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152		18211	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.278	65		10234	14.865	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150			Recovery =	59.480%		
7) Chloroethane-d5	1.532	69		11258	20.509	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150			Recovery =	82.040%		
11) 1,1-Dichloroethene-d2	2.053	65		5103	16.650	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110			Recovery =	66.600%		
21) 2-Butanone-d5	3.863	46		8206m	51.952	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135			Recovery =	103.900%		
24) Chloroform-d	4.256	84		28384	23.842	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150			Recovery =	95.360%		
26) 1,2-Dichloroethane-d4	4.953	65		16723	26.792	ug/L	0.01
Spiked Amount 25.000	Range 70 - 130			Recovery =	107.160%		
32) Benzene-d6	4.966	84		41896	16.572	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135			Recovery =	66.280%		
36) 1,2-Dichloropropane-d6	5.995	67		18002	22.612	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120			Recovery =	90.440%		
41) Toluene-d8	7.252	98		30717	13.770	ug/L	0.01
Spiked Amount 25.000	Range 30 - 130			Recovery =	55.080%		
43) trans-1,3-Dichloroprop...	7.580	79		4928	15.096	ug/L	0.03
Spiked Amount 25.000	Range 30 - 135			Recovery =	60.400%		
47) 2-Hexanone-d5	8.072	63		2109m	19.552	ug/L	0.04
Spiked Amount 50.000	Range 20 - 135			Recovery =	39.100%		
56) 1,1,2,2-Tetrachloroeth...	10.156	84		16736	28.131	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120			Recovery =	112.520%		
66) 1,2-Dichlorobenzene-d4	11.564	152		13310	19.931	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120			Recovery =	79.720%		
Target Compounds							
16) Methylene chloride	2.449	84		5686	6.711	ug/L	Qvalue 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053024\
Data File : VV035911.D
Acq On : 30 May 2024 21:20
Operator : SY/MD
Sample : P2659-12
Misc : 4.13g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHC33

Manual IntegrationsAPPROVED

Quant Time: May 31 00:56:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 31 00:49:35 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/03/2024
Supervised By :Semsettin Yesilyurt 06/03/2024

