
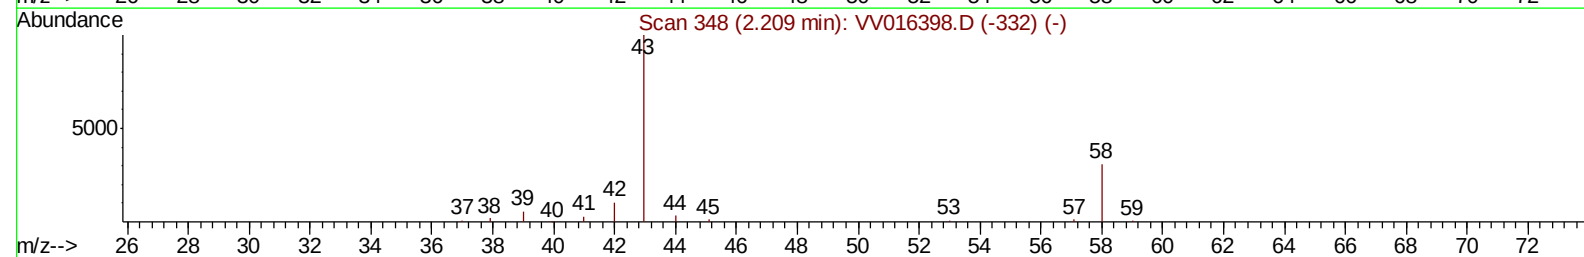
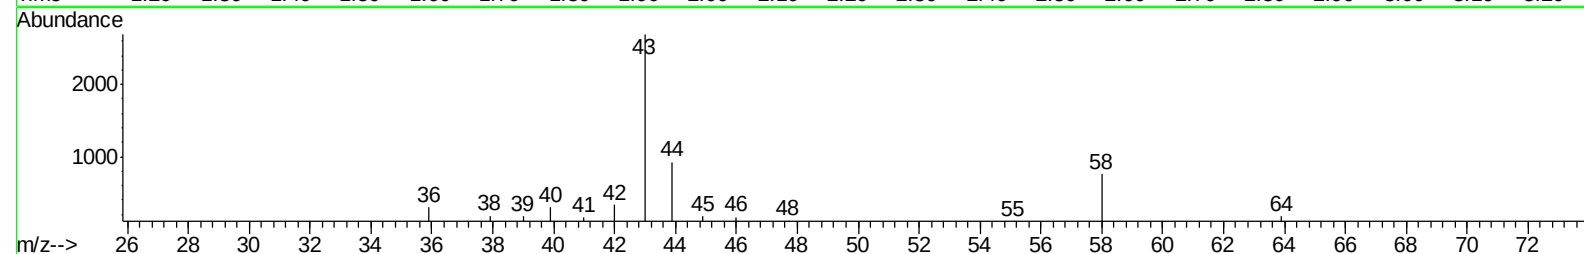


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060120\
 Data File : VV016415.D
 Acq On : 01 Jun 2020 16:57
 Operator : SY/MD
 Sample : L2780-06
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Quant Time: Jun 02 01:18:07 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053020WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jun 02 01:13:11 2020
 Response via : Initial Calibration

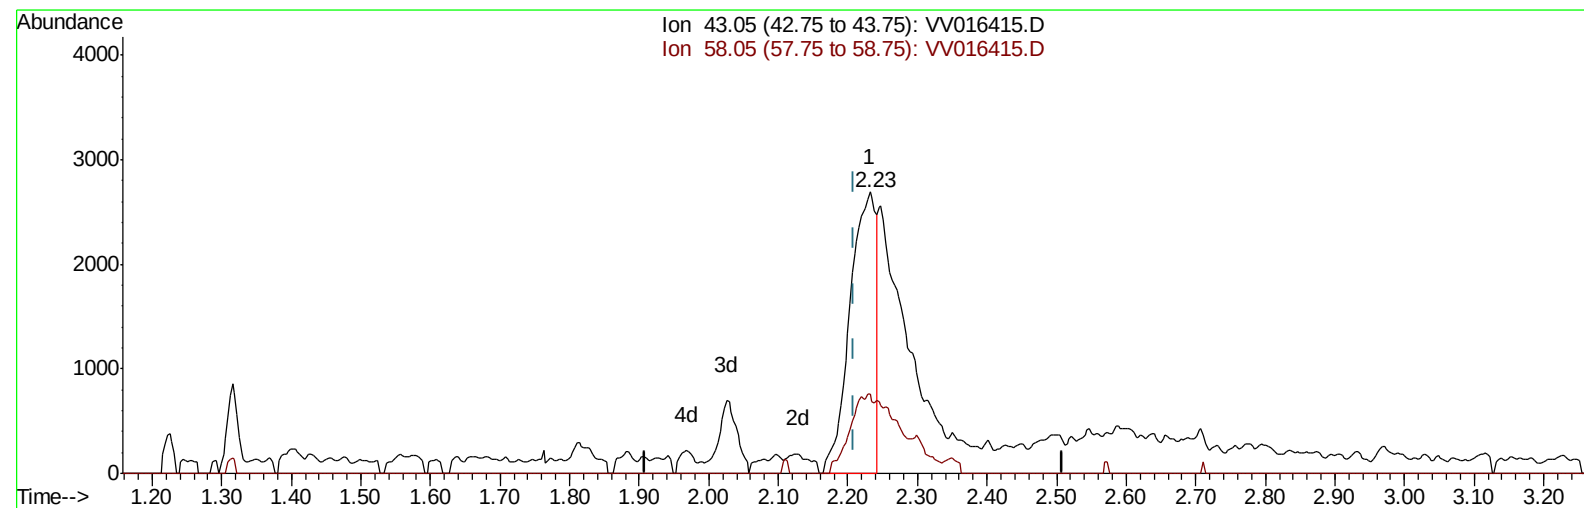

TIC: VV016415.D

(13) Acetone (T)

2.232min (+0.023) 6.52ug/L

response 7036

Ion	Exp%	Act%
43.05	100	100
58.05	29.60	17.96
0.00	0.00	0.00
0.00	0.00	0.00