
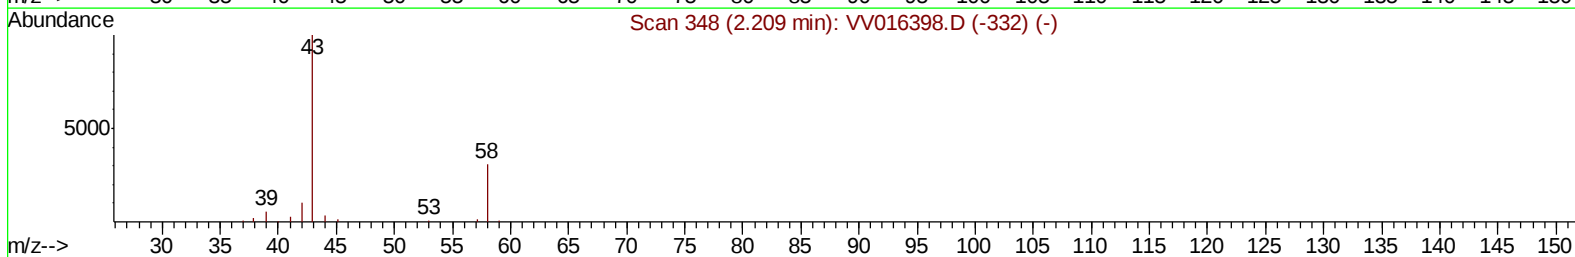
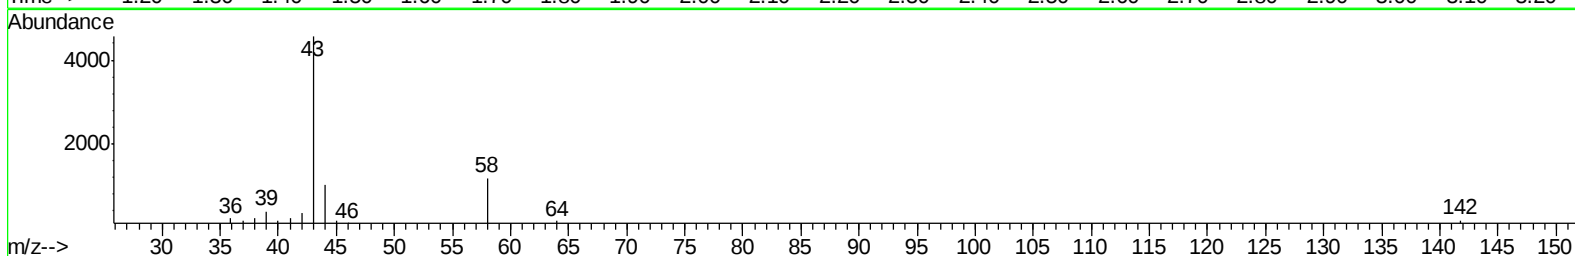


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060120\
Data File : VV016421.D
Acq On : 01 Jun 2020 19:21
Operator : SY/MD
Sample : VSTDCCC005EC
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 26 Sample Multiplier: 1

Quant Time: Jun 02 01:21:58 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053020WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jun 02 01:13:11 2020
Response via : Initial Calibration

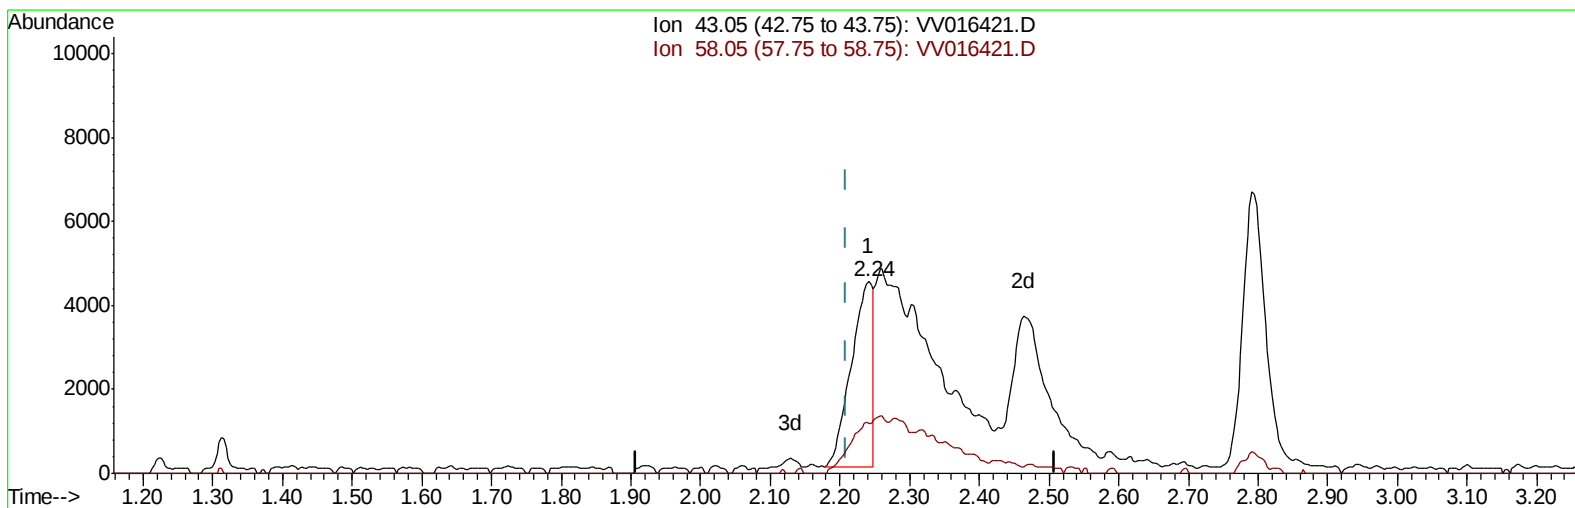

TIC: VV016421.D

(13) Acetone (T)

2.242min (+0.032) 8.56ug/L

response 9628

Ion	Exp%	Act%
43.05	100	100
58.05	29.60	24.96
0.00	0.00	0.00
0.00	0.00	0.00