

Quantitation Report (QT Reviewed)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060120\
 Data File : VV016403.D
 Acq On : 01 Jun 2020 11:37
 Operator : SY/MD
 Sample : L2826-10DL 10X
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CWKC3DL

Manual Integrations
 APPROVED

MMDadoda
 6/2/2020 4:48:55 PM

Quant Time: Jun 02 02:03:25 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053020WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jun 02 01:13:11 2020
 Response via : Initial Calibration

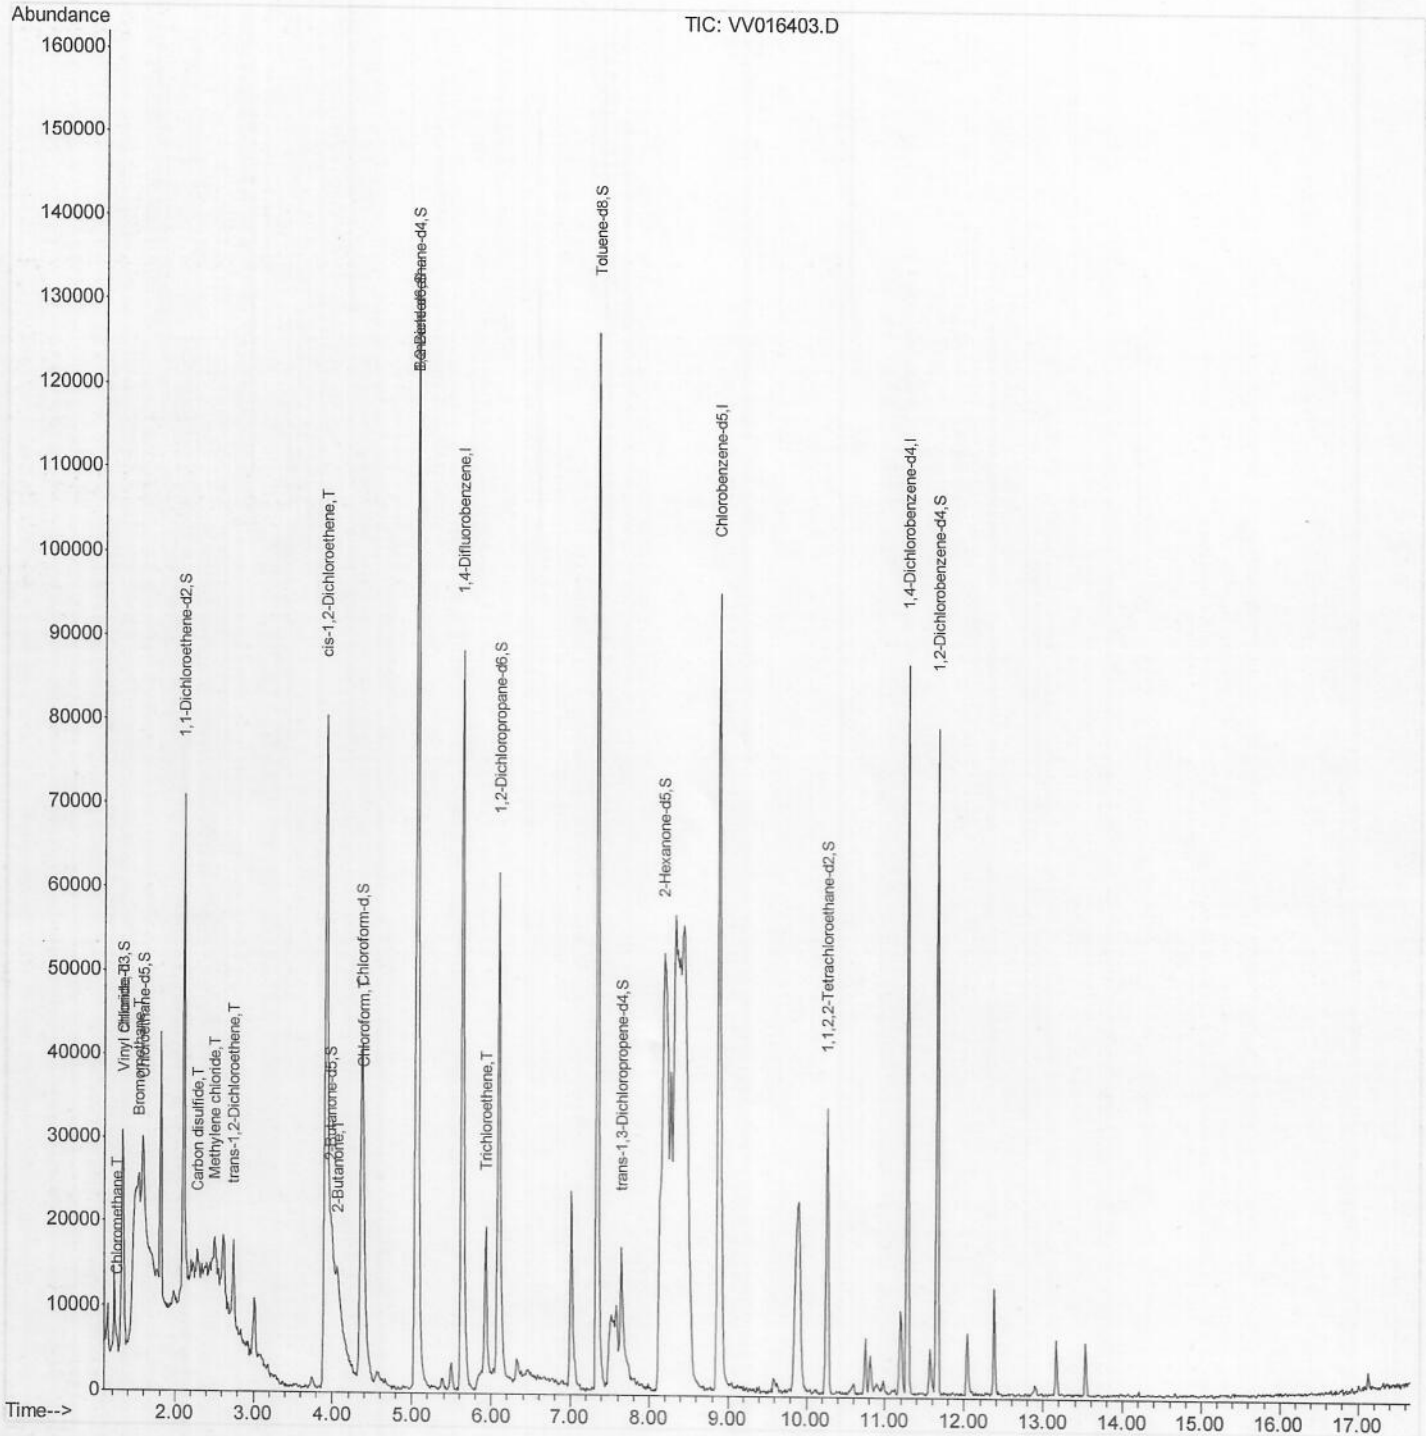

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060120\
 Data File : VV016403.D
 Acq On : 01 Jun 2020 11:37
 Operator : SY/MD
 Sample : L2826-10DL 10X
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CWKC3DL

Manual Integrations
 APPROVED

MMDadoda
 6/2/2020 4:48:55 PM

Quant Time: Jun 02 02:00:47 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053020WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jun 02 01:13:11 2020
 Response via : Initial Calibration

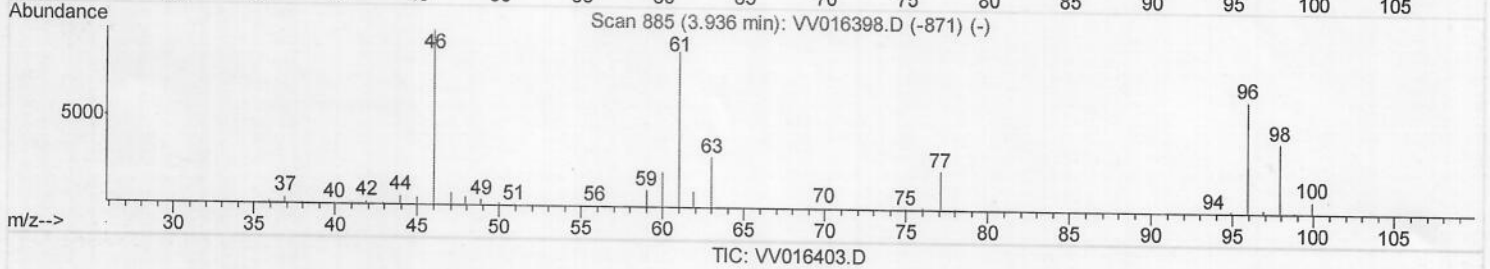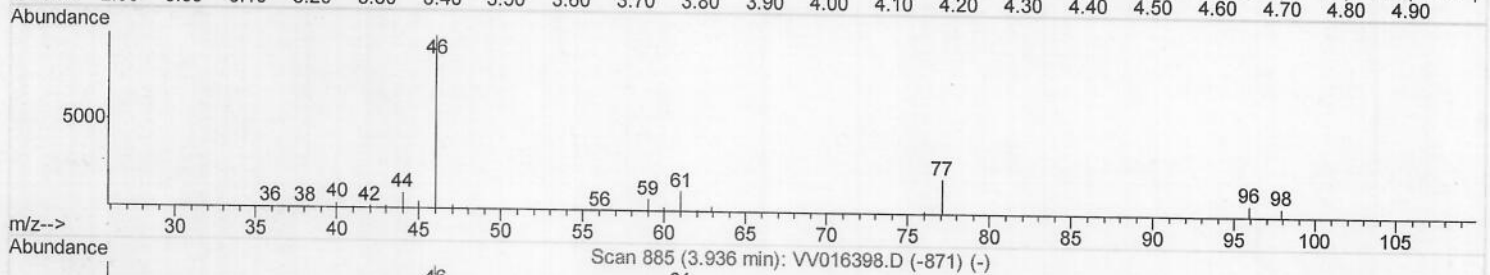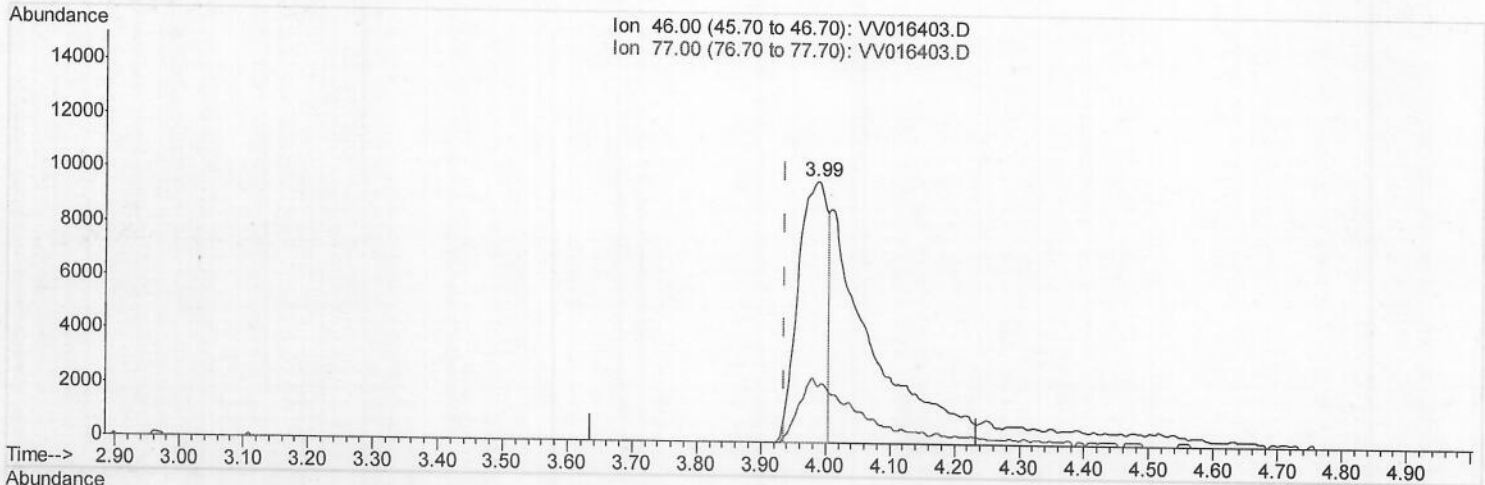

(20) 2-Butanone-d5 (S)

3.987min (+0.052) 19.03ug/L

response 29985

Ion	Exp%	Act%
46.00	100	100
77.00	21.60	15.67
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060120\
 Data File : VV016403.D
 Acq On : 01 Jun 2020 11:37
 Operator : SY/MD
 Sample : L2826-10DL 10X
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CWKC3DL

Manual Integrations
 APPROVED

MMDadoda
 6/2/2020 4:48:55 PM

Quant Time: Jun 02 02:00:47 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053020WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jun 02 01:13:11 2020
 Response via : Initial Calibration

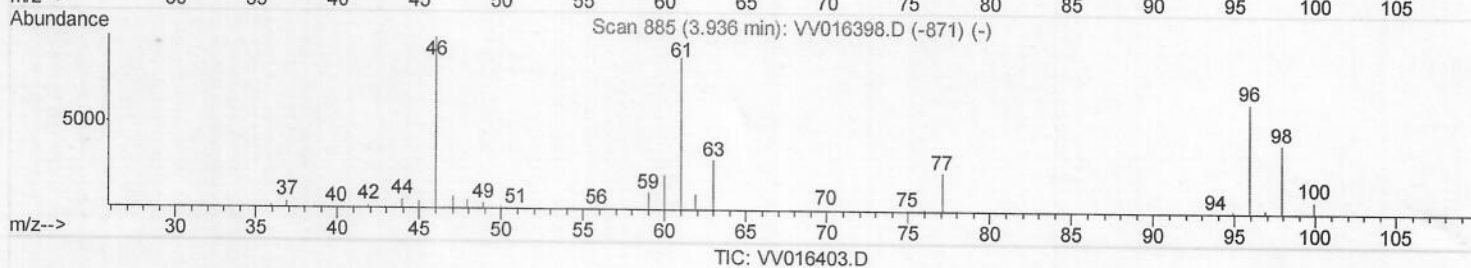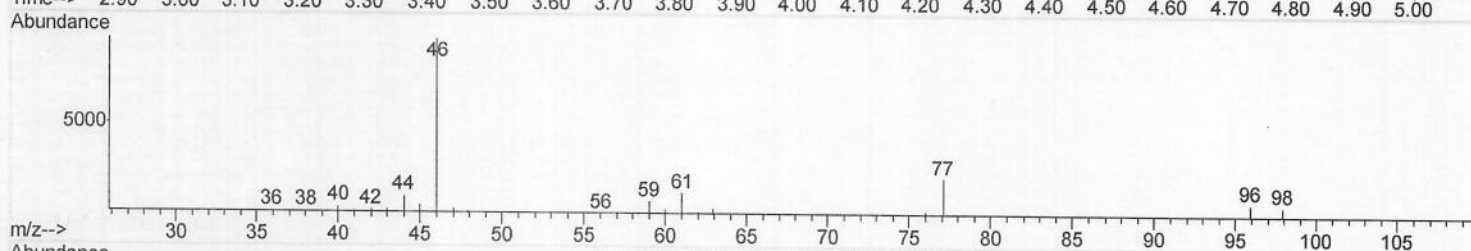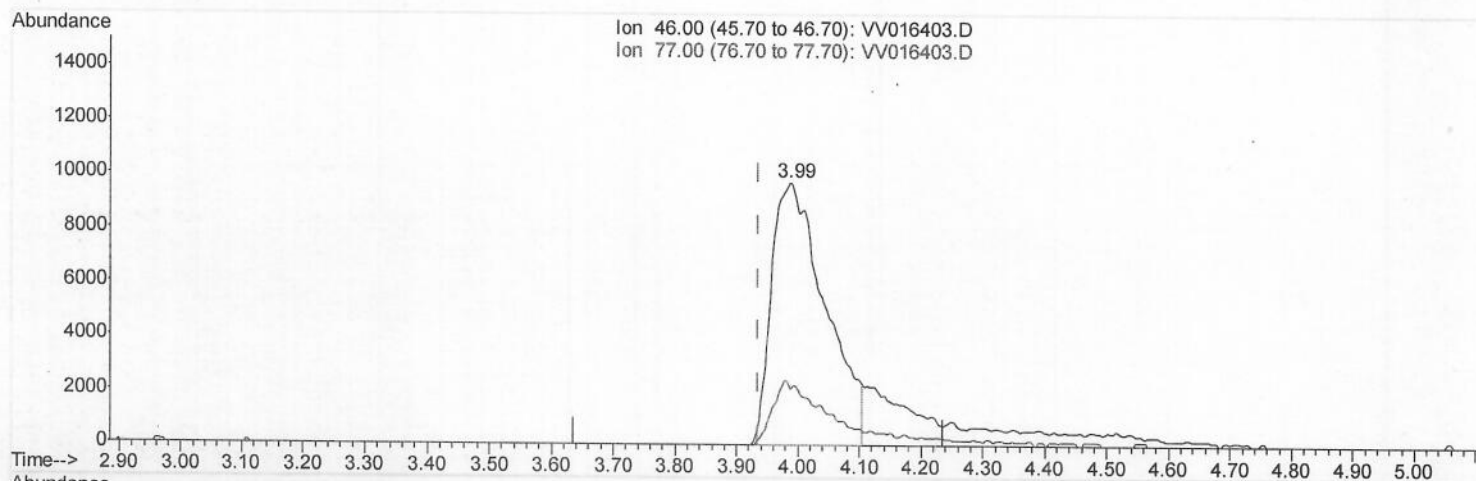

(20) 2-Butanone-d5 (S)

3.987min (+0.052) 37.37ug/L m

response 58885

Ion	Exp%	Act%
46.00	100	100
77.00	21.60	7.98#
0.00	0.00	0.00
0.00	0.00	0.00

2 MD
6/02/20

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060120\
 Data File : VV016403.D
 Acq On : 01 Jun 2020 11:37
 Operator : SY/MD
 Sample : L2826-10DL 10X
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CWKC3DL

Manual Integrations
 APPROVED

MMDadoda
 6/2/2020 4:48:55 PM

Quant Time: Jun 02 02:00:47 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053020WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jun 02 01:13:11 2020
 Response via : Initial Calibration

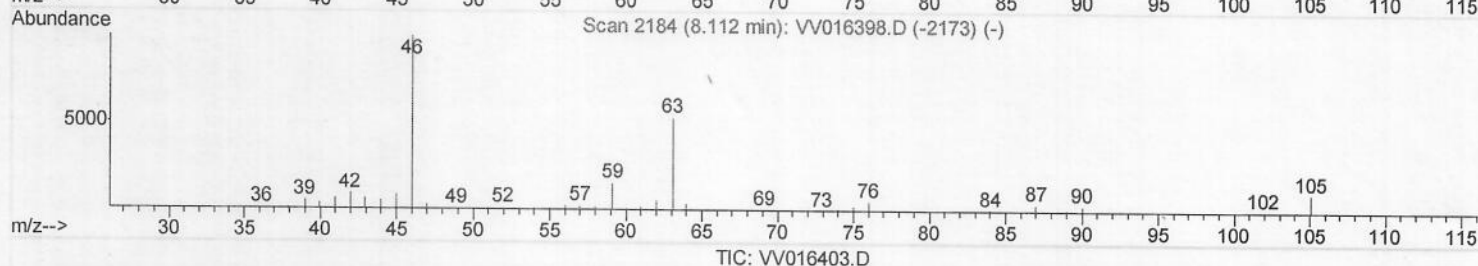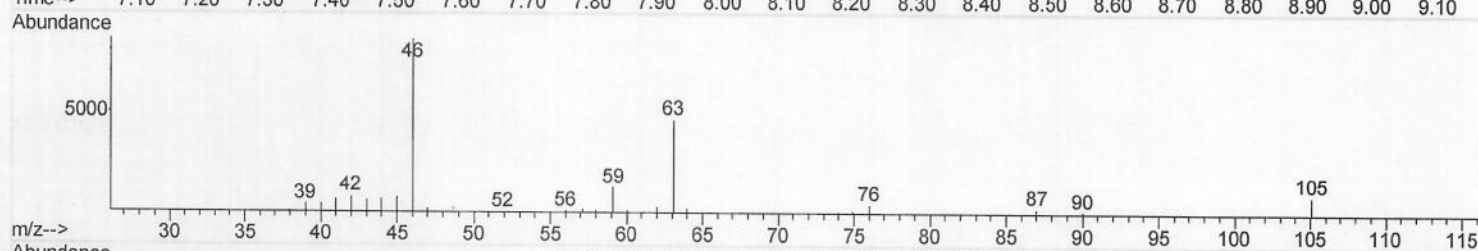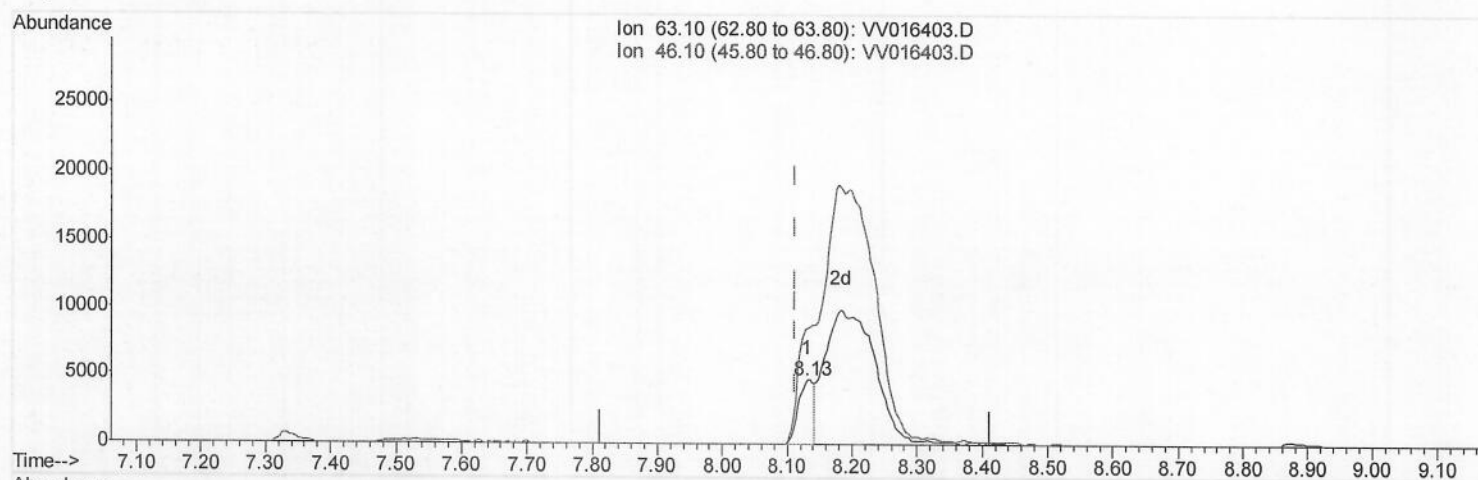

(48) 2-Hexanone-d5 (S)

8.132min (+0.019) 7.38ug/L

response 7816

Ion	Exp%	Act%
63.10	100	100
46.10	191.10	0.00#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060120\
 Data File : VV016403.D
 Acq On : 01 Jun 2020 11:37
 Operator : SY/MD
 Sample : L2826-10DL 10X
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CWKC3DL

Manual Integrations
 APPROVED

MMDadoda
 6/2/2020 4:48:55 PM

Quant Time: Jun 02 02:00:47 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053020WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jun 02 01:13:11 2020
 Response via : Initial Calibration

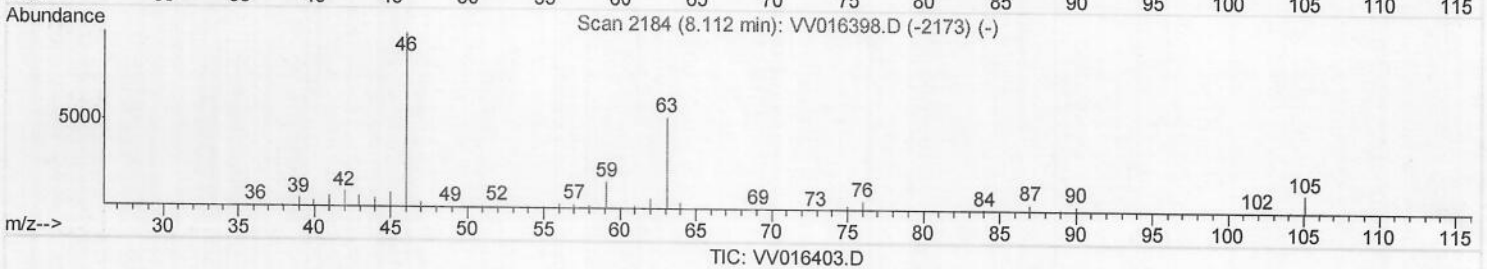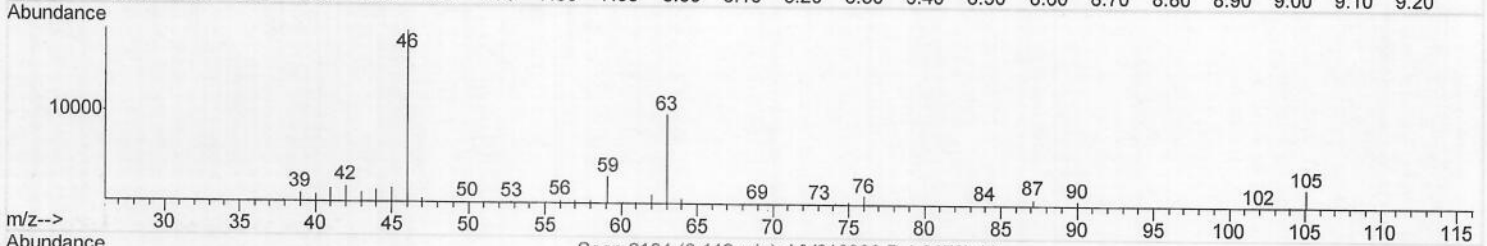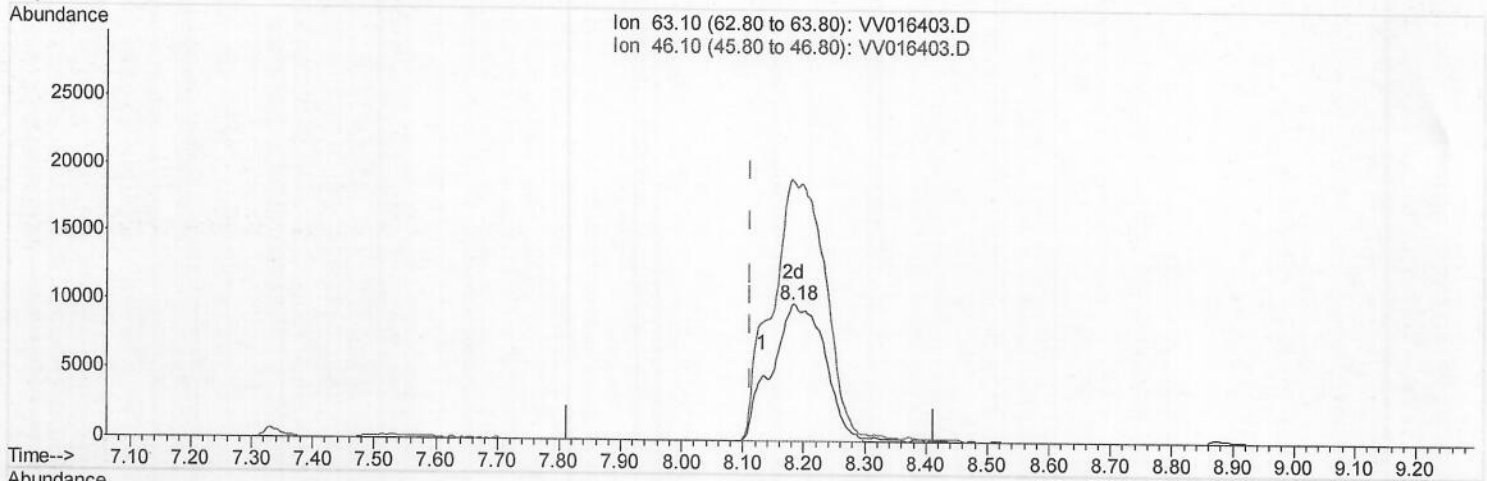

(48) 2-Hexanone-d5 (S)

8.183min (+0.071) 56.63ug/L m

response 59982

Ion	Exp%	Act%
63.10	100	100
46.10	191.10	0.00#
0.00	0.00	0.00
0.00	0.00	0.00

> MD
 6/02/20

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060120\
 Data File : VV016403.D
 Acq On : 01 Jun 2020 11:37
 Operator : SY/MD
 Sample : L2826-10DL 10X
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sampled :
 CWKC3DL

Manual Integrations
 APPROVED

MMDadoda
 6/2/2020 4:48:55 PM

Quant Time: Jun 02 02:03:25 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053020WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jun 02 01:13:11 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.63	114	83423	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	71934	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.28	152	21851	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.33	65	28582	3.91	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	78.20%
7) Chloroethane-d5	1.58	69	12016	2.16	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	43.20%#
11) 1,1-Dichloroethene-d2	2.11	63	35628	2.79	ug/L	-0.02
Spiked Amount	5.000	Range	60 - 125	Recovery	=	55.80%#
20) 2-Butanone-d5	3.99	46	58885m	37.37	ug/L	0.05
Spiked Amount	50.000	Range	40 - 130	Recovery	=	74.74%
24) Chloroform-d	4.36	84	48688	3.94	ug/L	-0.01
Spiked Amount	5.000	Range	70 - 125	Recovery	=	78.80%
26) 1,2-Dichloroethane-d4	5.05	65	31550	4.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.00%
32) Benzene-d6	5.05	84	113654	5.56	ug/L	-0.02
Spiked Amount	5.000	Range	70 - 125	Recovery	=	111.20%
36) 1,2-Dichloropropane-d6	6.09	67	33136	5.25	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.00%
41) Toluene-d8	7.33	98	93930	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.60%
45) trans-1,3-Dichloropropene-	7.64	79	10663	4.68	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.60%
48) 2-Hexanone-d5	8.18	63	59982m	56.63	ug/L	0.07
Spiked Amount	50.000	Range	45 - 130	Recovery	=	113.26%
59) 1,1,2,2-Tetrachloroethane-	10.26	84	21199	4.75	ug/L	0.03
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.00%
65) 1,2-Dichlorobenzene-d4	11.66	152	19592	4.83	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.60%

7 M1D
 6/02/20

7 M1D
 6/02/20

Target Compounds

					Ovalue
3) Chloromethane	1.25	50	992	0.119	ug/L 99
5) Vinyl chloride	1.33	62	2809	0.377	ug/L # 21
6) Bromomethane	1.53	94	1626	0.389	ug/L 92
14) Carbon disulfide	2.29	76	3141	0.192	ug/L # 84
16) Methylene chloride	2.50	84	1884	0.328	ug/L # 9
18) trans-1,2-Dichloroethene	2.74	96	2939	0.516	ug/L 85
21) 2-Butanone	4.07	43	25677	16.428	ug/L 85
22) cis-1,2-Dichloroethene	3.92	96	50158	7.974	ug/L 98
25) Chloroform	4.39	83	10628	0.943	ug/L 94
34) Trichloroethene	5.93	95	6260	1.121	ug/L 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed