

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060120\
 Data File : VV016420.D
 Acq On : 01 Jun 2020 18:57
 Operator : SY/MD
 Sample : L2780-07
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Quant Time: Jun 02 04:31:11 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053020WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jun 02 01:13:11 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	83904	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	81923	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	35076	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	25161	3.42	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	68.40%
7) Chloroethane-d5	1.58	69	21310	3.82	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	76.40%
11) 1,1-Dichloroethene-d2	2.12	63	38165	2.97	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	59.40%#
20) 2-Butanone-d5	3.97	46	66797	42.15	ug/L	0.04
Spiked Amount	50.000	Range	40 - 130	Recovery	=	84.30%
24) Chloroform-d	4.37	84	52006	4.18	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.60%
26) 1,2-Dichloroethane-d4	5.06	65	30515	4.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.40%
32) Benzene-d6	5.07	84	105620	4.54	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.80%
36) 1,2-Dichloropropane-d6	6.09	67	32943	4.58	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.60%
41) Toluene-d8	7.33	98	89659	4.21	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.20%
45) trans-1,3-Dichloropropene-	7.64	79	9966	3.84	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.80%
48) 2-Hexanone-d5	8.12	63	60119	49.84	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	99.68%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	23374	4.60	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.00%
65) 1,2-Dichlorobenzene-d4	11.65	152	29816	4.58	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.60%


Target Compounds					Ovalue
25) Chloroform	4.40	83	3315	0.293 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060120\
Data File : VV016420.D
Acq On : 01 Jun 2020 18:57
Operator : SY/MD
Sample : L2780-07
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: Jun 02 04:31:11 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053020WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jun 02 01:13:11 2020
Response via : Initial Calibration

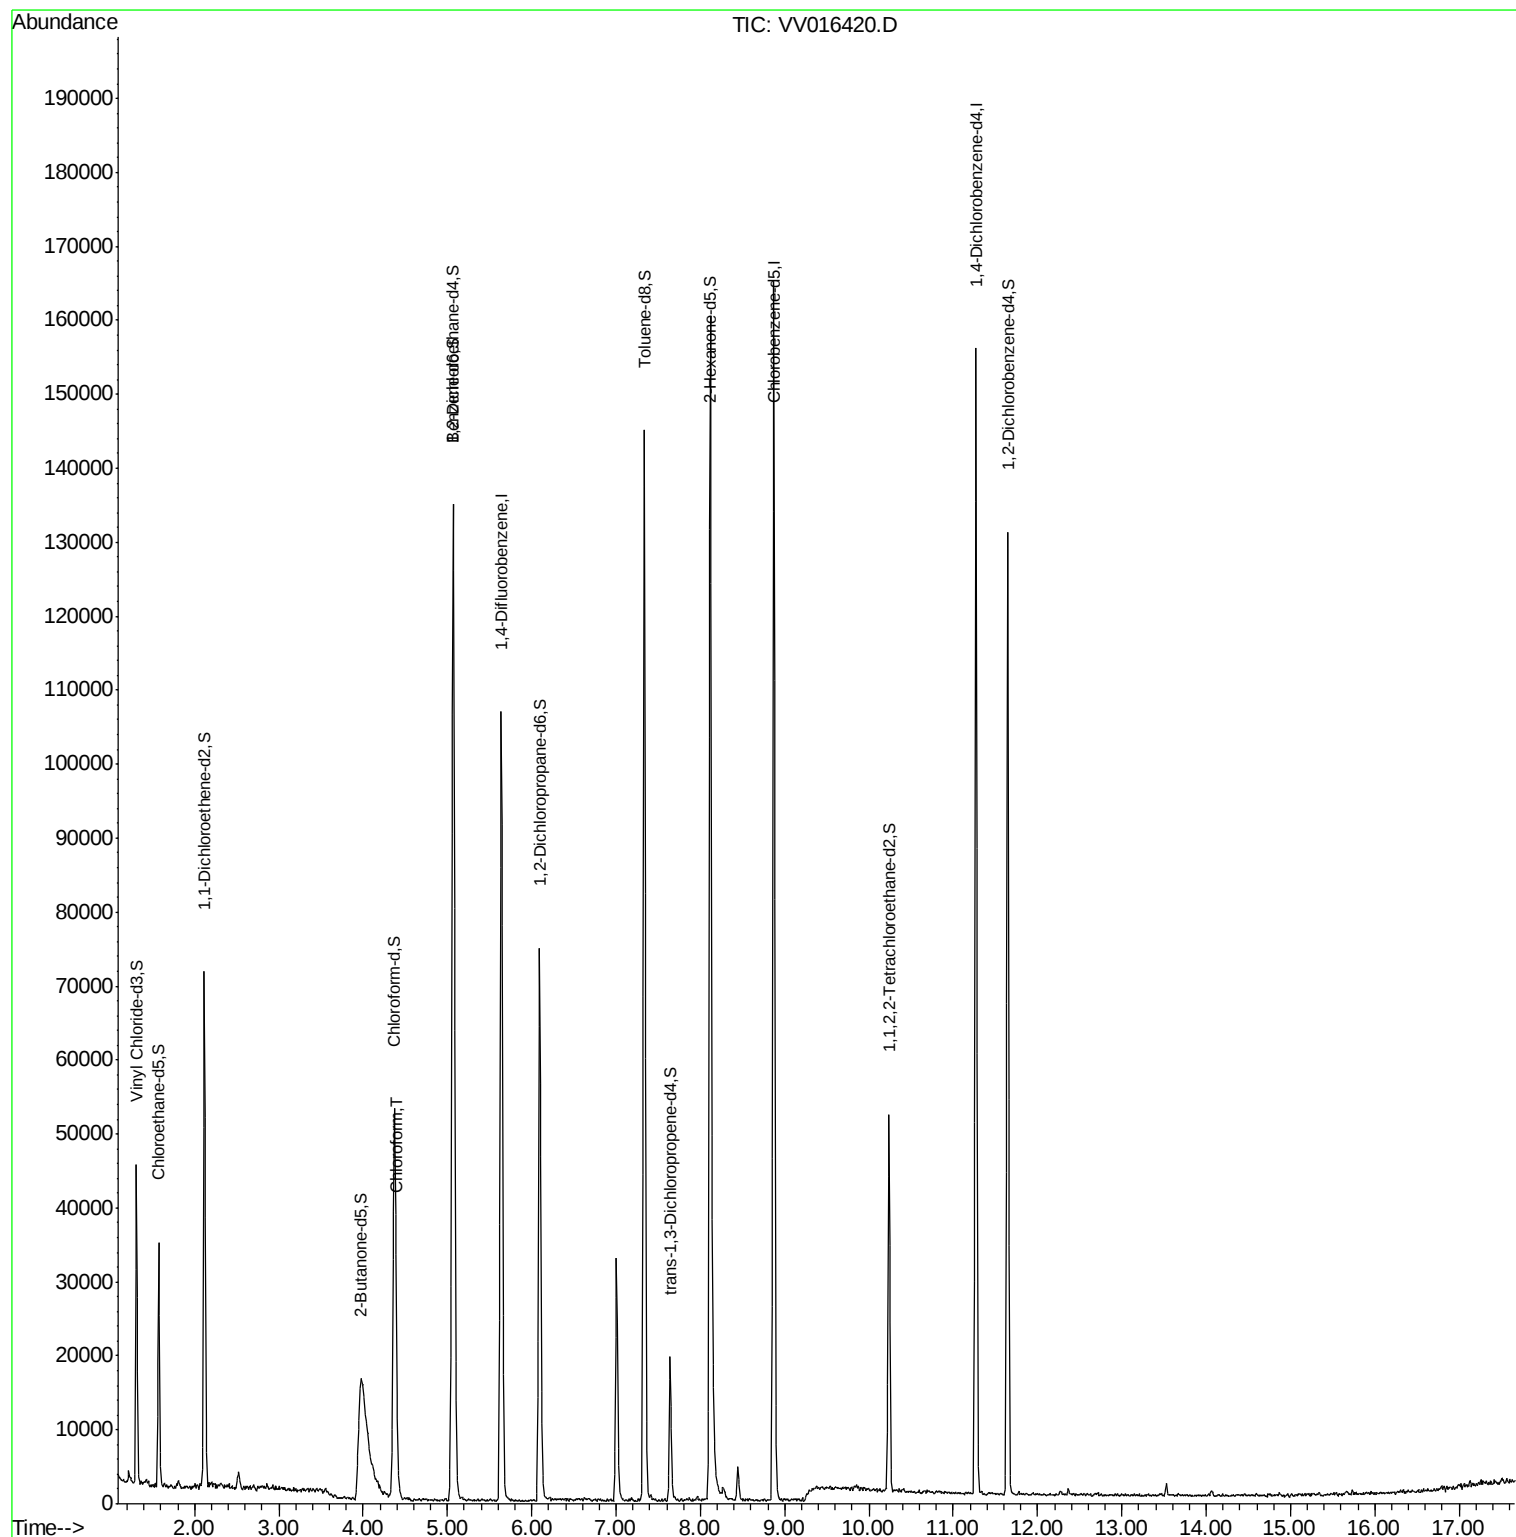

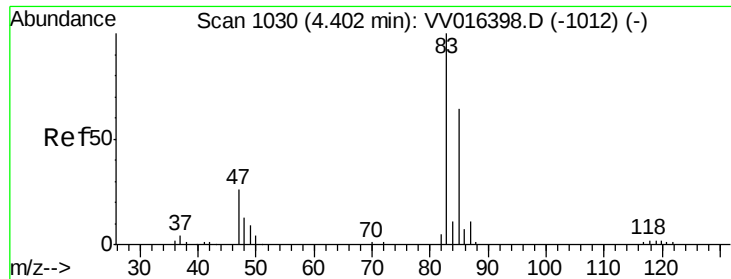

#25
 Chloroform
 Concen: 0.293 ug/L
 RT: 4.40 min Scan# 1029
 Delta R.T. -0.00 min
 Lab File: VV016420.D
 Acq: 01 Jun 2020 18:57

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Tot Ion: 83 Resp: 3315
 Ion Ratio Lower Upper
 83 100
 85 62.6 45.8 85.2

