


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV060120\
 Data File : VV016397.D
 Acq On : 01 Jun 2020 08:51
 Operator : SY/MD
 Sample : BFB37
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB37

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053020WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Jun 02 01:13:11 2020

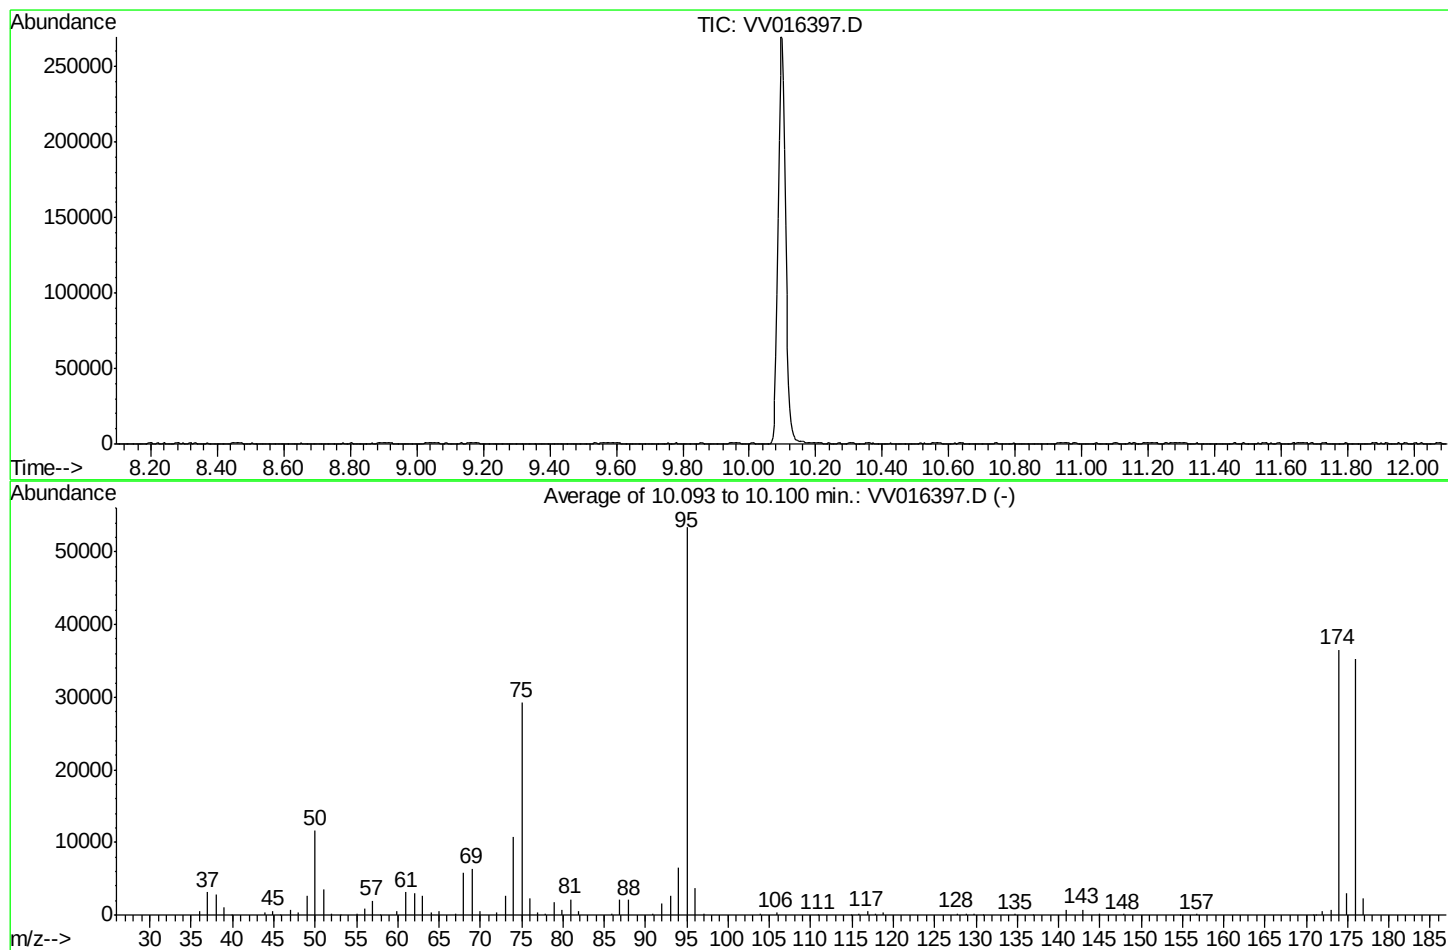

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	11556	PASS
75	95	30	80	54.8	29261	PASS
95	95	100	100	100.0	53394	PASS
96	95	5	9	7.0	3756	PASS
173	174	0.00	2	1.8	642	PASS
174	95	50	120	68.4	36517	PASS
175	174	5	9	8.0	2927	PASS
176	174	95	101	96.7	35304	PASS
177	176	5	9	6.4	2267	PASS

m/z	Abundance
36.00	511.0
37.00	3057.0
38.00	2781.0
39.00	1069.0
39.90	207.0
44.00	473.0
44.90	526.0
47.00	643.0
48.00	332.0
49.00	2543.0
50.00	11166.0
51.00	3552.0
51.90	196.0
55.00	178.0
56.00	911.0
56.90	1782.0
60.00	542.0
61.00	2982.0
62.00	2729.0
63.00	2555.0
64.00	319.0
65.00	492.0
67.00	175.0
68.00	5386.0
69.00	6128.0
70.00	452.0
71.90	331.0
73.00	2449.0
74.00	10052.0
75.00	27696.0
76.00	2257.0
77.00	315.0
77.80	190.0
78.90	1729.0
79.90	629.0
80.90	2096.0
81.90	534.0
85.90	131.0
86.90	2015.0
87.90	1952.0
90.80	222.0
92.00	1514.0
93.00	2388.0
94.00	5968.0
95.00	50216.0
96.00	3730.0
97.00	118.0
103.90	254.0
105.80	290.0
114.90	108.0
115.80	222.0
116.90	388.0
117.80	189.0
118.80	384.0
127.70	214.0
128.90	120.0
129.80	172.0
134.80	102.0
140.90	619.0
142.90	719.0
144.90	129.0
147.90	118.0
156.80	133.0
170.80	106.0
171.90	491.0
173.00	588.0
173.90	33104.0
174.90	2778.0
175.90	32624.0
177.00	2111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB37

m/z	Abundance
36.00	488.0
37.00	3281.0
38.00	3018.0
39.00	1129.0
39.90	211.0
44.00	531.0
44.90	578.0
45.90	121.0
46.90	744.0
48.00	354.0
49.00	2781.0
50.00	11891.0
51.00	3682.0
51.90	168.0
53.10	110.0
55.00	202.0
56.00	986.0
56.90	2056.0
57.80	111.0
59.90	592.0
61.00	3271.0
62.00	3042.0
63.00	2755.0
64.00	348.0
64.90	512.0
67.00	181.0
68.00	5890.0
69.00	6621.0
69.90	542.0
71.90	346.0
73.00	2709.0
74.00	11143.0
75.00	30336.0
76.00	2361.0
77.00	311.0
77.80	177.0
78.90	1864.0
79.90	716.0
80.90	2249.0
81.90	581.0
85.90	134.0
86.90	2100.0
87.90	2158.0
90.80	242.0
92.00	1749.0
93.00	2690.0
94.00	6682.0
95.00	55128.0
96.00	3896.0
97.00	137.0
103.90	277.0
105.80	302.0
110.90	103.0
115.80	240.0
116.80	464.0
117.80	227.0
118.80	423.0
127.70	232.0
128.90	138.0
129.80	195.0
130.80	114.0
134.80	118.0
140.80	638.0
142.90	765.0
144.90	137.0
147.90	126.0
154.70	102.0
156.80	159.0
170.90	109.0
171.90	533.0
173.00	676.0
173.90	37688.0
174.90	3024.0
175.90	36536.0
177.00	2345.0

Instrument :
MSVOA_V
ClientSampleId :
BFB37

m/z	Abundance
35.90	459.0
37.00	3111.0
38.00	2912.0
39.00	1139.0
39.90	244.0
43.90	619.0
44.90	568.0
45.80	115.0
47.00	742.0
47.90	347.0
49.00	2720.0
50.00	11613.0
51.00	3499.0
52.00	135.0
55.00	223.0
56.00	1012.0
56.90	2003.0
59.90	607.0
61.00	3071.0
62.00	3082.0
63.00	2604.0
64.00	375.0
64.90	494.0
66.90	168.0
68.00	5939.0
69.00	6498.0
69.90	582.0
71.90	354.0
73.00	2743.0
74.00	10983.0
75.00	29752.0
76.00	2363.0
76.90	306.0
77.90	195.0
78.90	1973.0
79.90	684.0
80.90	2210.0
81.90	563.0
85.90	147.0
86.90	2020.0
88.00	2210.0
90.80	265.0
92.00	1774.0
93.00	2684.0
94.00	6922.0
95.00	54840.0
96.00	3642.0
97.00	145.0
103.90	270.0
105.90	290.0
115.80	239.0
116.80	493.0
117.80	253.0
118.80	392.0
127.70	224.0
128.80	135.0
129.80	209.0
130.80	122.0
134.80	140.0
136.90	107.0
140.80	666.0
142.90	711.0
144.90	146.0
147.90	109.0
154.80	123.0
156.80	138.0
171.10	116.0
171.90	576.0
173.00	663.0
173.90	38760.0
174.90	2981.0
175.90	36752.0
176.90	2345.0

Instrument :
MSVOA_V
ClientSampleId :
BFB37

Scan 2789 (10.058 min): VV016397.D
BFB37

m/z	Abundance
39.90	159.0
44.00	234.0

Instrument :
MSVOA_V
ClientSampleId :
BFB37