

Quantitation Report (Qedit)



Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060319\
 Data File : VV011197.D
 Acq On : 03 Jun 2019 11:28
 Operator : SY/MD
 Sample : VV0603SBL01
 Misc : 5.00G/10ML/MSVOA_V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK69

Manual Integrations
 APPROVED

MMDadoda
 6/6/2019 8:48:33 AM

Quant Time: Jun 04 01:24:07 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM053019S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jun 04 01:13:38 2019
 Response via : Initial Calibration

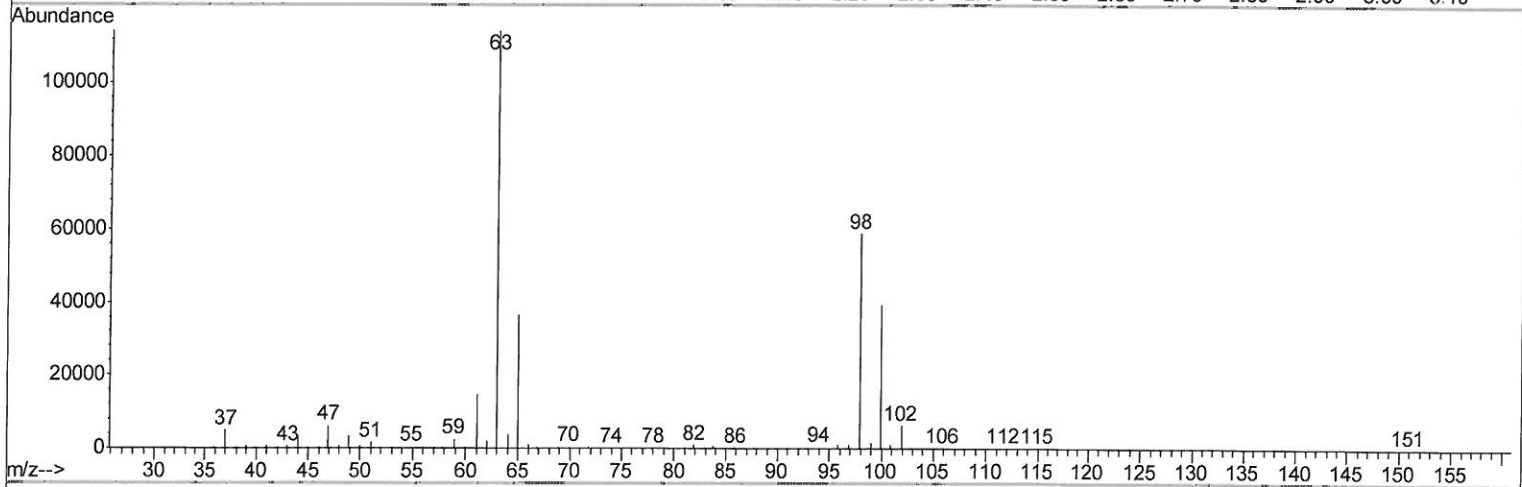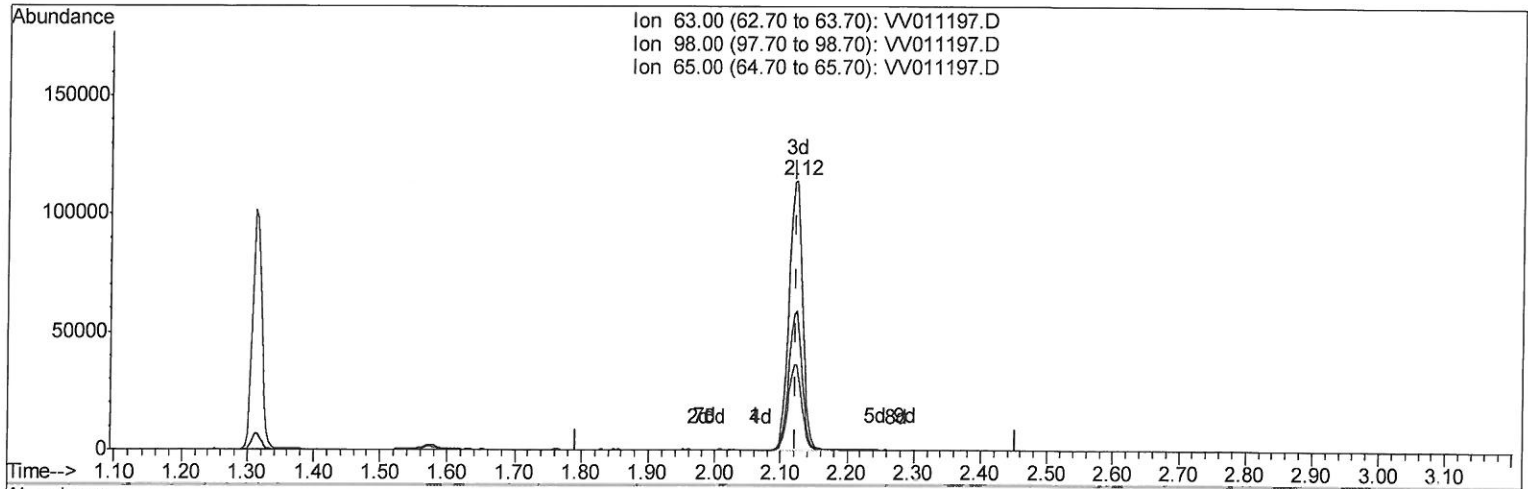

TIC: VV011197.D

(10) 1,1-Dichloroethene-d2 (S)

2.122min (+0.000) 17.34ug/L m

response 162504

Ion	Exp%	Act%
63.00	100	100
98.00	64.20	0.03#
65.00	23.10	0.01#
0.00	0.00	0.00

>06/04/19 SZ

Quantitation Report (Qedit)



Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060319\
Data File : VV011197.D
Acq On : 03 Jun 2019 11:28
Operator : SY/MD
Sample : VV0603SBL01
Misc : 5.00G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK69

Manual Integrations
APPROVED

MMDadoda
6/6/2019 8:48:33 AM

Quant Time: Jun 04 01:24:07 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM053019S.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 04 01:13:38 2019
Response via : Initial Calibration

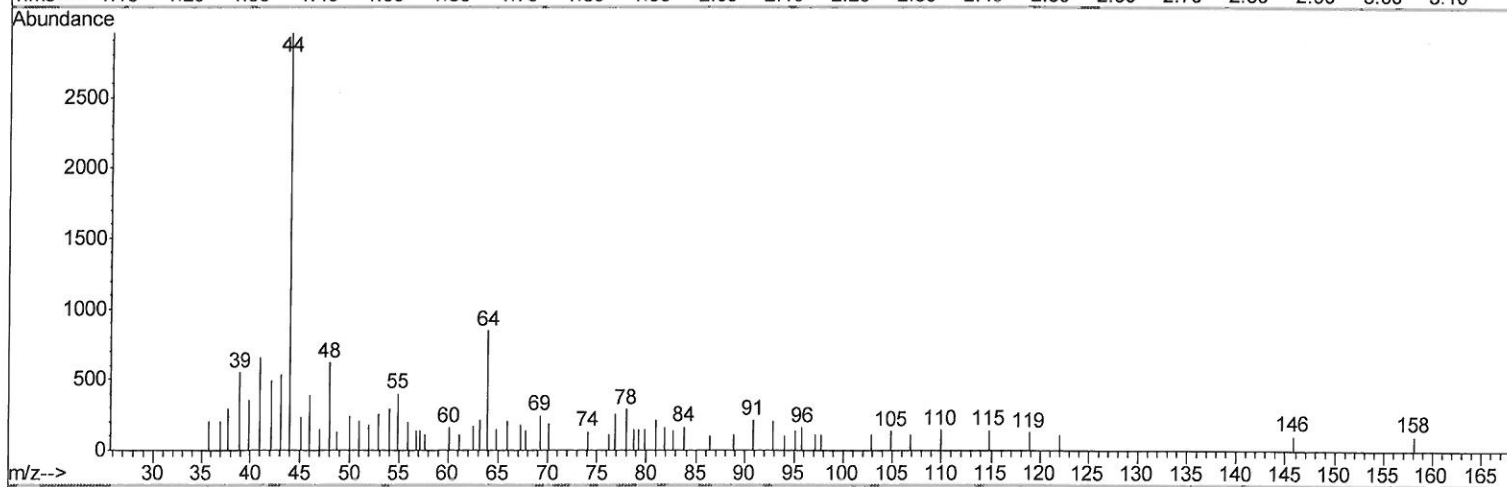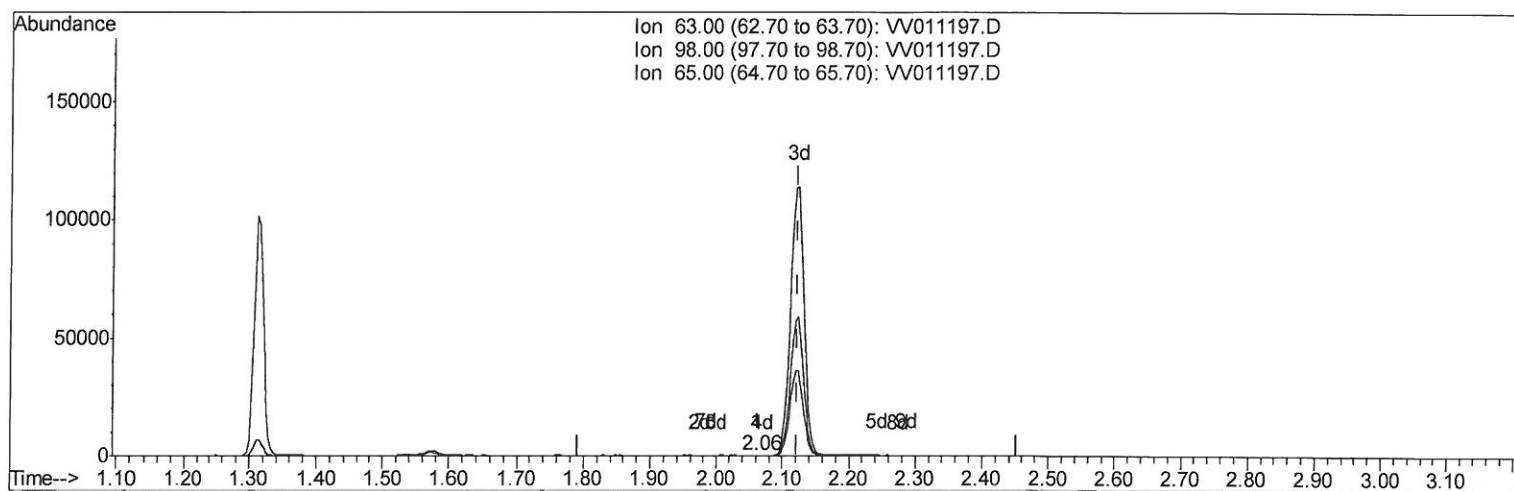

TIC: VV011197.D

(10) 1,1-Dichloroethene-d2 (S)

2.061min (-0.061) 0.01ug/L

response 82

Ion	Exp%	Act%
63.00	100	100
98.00	64.20	52.44
65.00	23.10	19.51
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060319\
 Data File : VV011197.D
 Acq On : 03 Jun 2019 11:28
 Operator : SY/MD
 Sample : VV0603SBL01
 Misc : 5.00G/10ML/MSVOA_V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK69

Manual Integrations
 APPROVED

MMDadoda
 6/6/2019 8:48:33 AM

Quant Time: Jun 04 01:24:36 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM053019S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jun 04 01:13:38 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	337358	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	310055	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	144852	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	98178	21.51	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.04%
7) Chloroethane-d5	1.57	69	90240	25.72	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	102.88%
10) 1,1-Dichloroethene-d2	2.12	63	162504m	17.34	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	69.36%
20) 2-Butanone-d5	3.94	46	66270	39.72	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	79.44%
24) Chloroform-d	4.40	84	161091	19.53	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	78.12%
26) 1,2-Dichloroethane-d4	5.08	65	120955	22.51	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.04%
29) Benzene-d6	5.09	84	409347	24.31	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	97.24%
33) 1,2-Dichloropropane-d6	6.11	67	128290	23.78	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.12%
37) Toluene-d8	7.36	98	375696	23.65	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	94.60%
38) trans-1,3-Dichloropropene-	7.66	79	52079	21.33	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.32%
39) 2-Hexanone-d5	8.13	63	49544	40.40	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	80.80%
48) 1,1,2,2-Tetrachloroethane-	10.26	84	100475	20.66	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	82.64%
61) 1,2-Dichlorobenzene-d4	11.67	152	128171	23.65	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	94.60%

06/04/19 Sy

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060319\
Data File : VV011197.D
Acq On : 03 Jun 2019 11:28
Operator : SY/MD
Sample : VV0603SBL01
Misc : 5.00G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK69

Manual Integrations
APPROVED

MMDadoda
6/6/2019 8:48:33 AM

Quant Time: Jun 04 01:24:36 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM053019S.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 04 01:13:38 2019
Response via : Initial Calibration

