


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060319\
Data File : VV011195.D
Acq On : 03 Jun 2019 09:29
Operator : SY/MD
Sample : BFB68
Misc : 5.00G/10ML/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB68

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM053019S.M
Title : VOC Analysis
Last Update : Tue Jun 04 01:13:38 2019

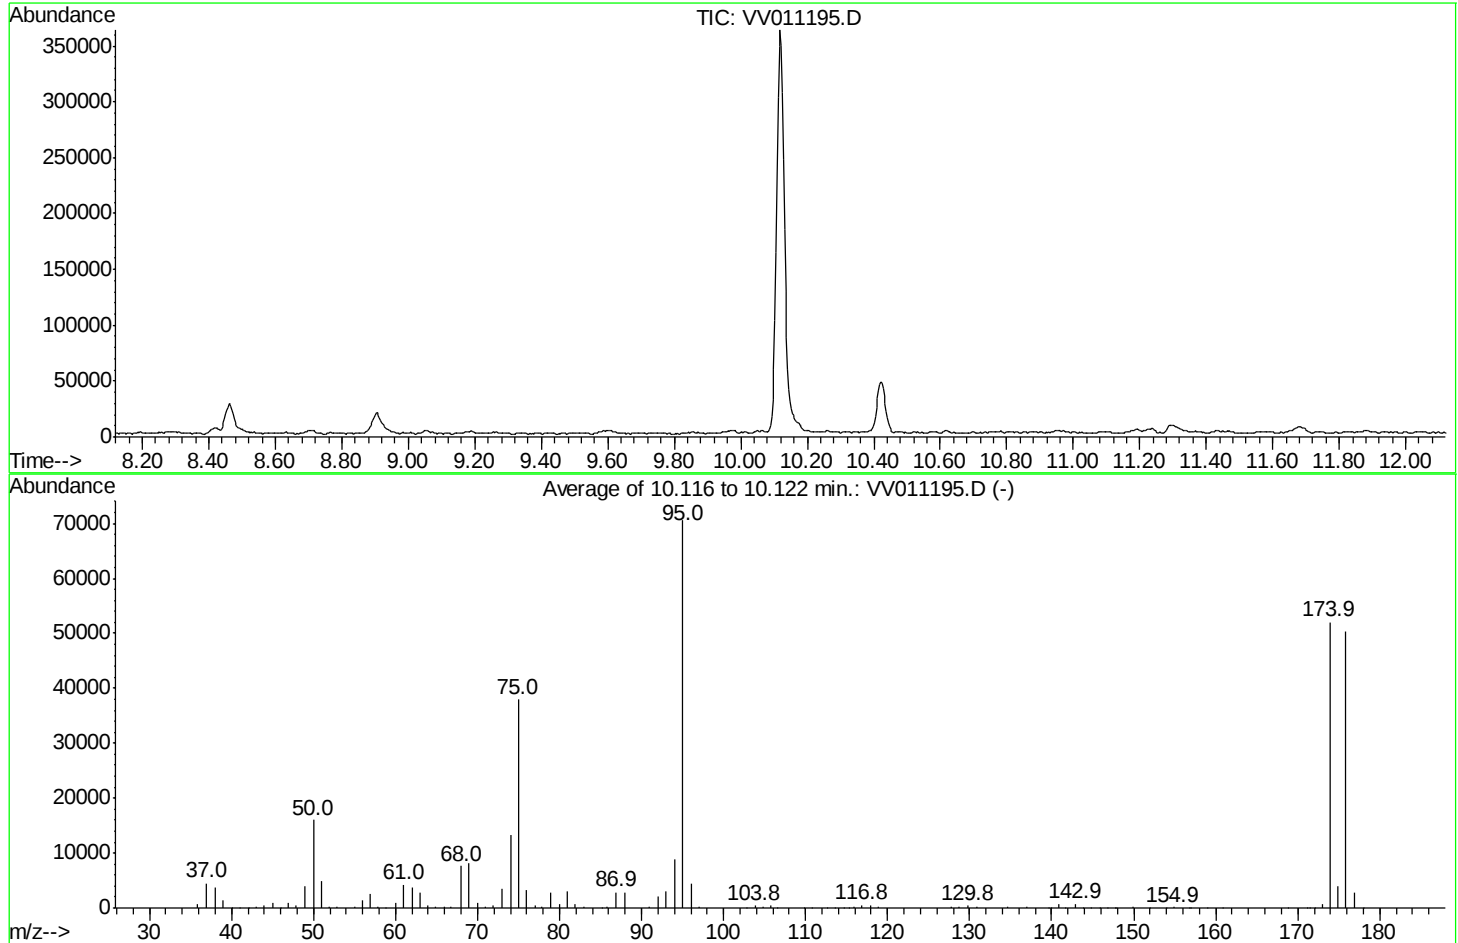

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.6	15981	PASS
75	95	30	80	53.7	37917	PASS
95	95	100	100	100.0	70573	PASS
96	95	5	9	6.3	4441	PASS
173	174	0.00	2	1.6	823	PASS
174	95	50	120	73.7	51981	PASS
175	174	5	9	7.6	3941	PASS
176	174	95	101	96.8	50336	PASS
177	176	5	9	5.7	2881	PASS

m/z	Abundance
35.90	719.0
36.60	164.0
37.90	300.0
39.00	201.0
40.10	229.0
41.00	160.0
42.00	142.0
42.90	109.0
43.90	570.0
44.70	116.0
46.00	107.0
46.80	103.0
48.70	128.0
55.00	179.0
66.80	100.0
68.90	264.0
91.20	140.0
99.70	113.0
118.80	157.0
149.50	123.0
168.80	180.0

Instrument :
MSVOA_V
ClientSampleId :
BFB68

m/z	Abundance
35.90	1277.0
37.00	4646.0
38.00	4009.0
39.00	1632.0
40.00	316.0
41.00	259.0
42.10	127.0
43.00	247.0
43.90	910.0
45.00	826.0
45.90	180.0
47.00	917.0
47.80	505.0
49.00	3720.0
50.00	15813.0
51.00	5134.0
52.00	252.0
52.90	117.0
55.00	361.0
56.00	1500.0
57.00	2468.0
57.90	202.0
58.80	116.0
59.90	1001.0
61.00	4226.0
62.00	3678.0
63.00	2764.0
64.00	474.0
64.80	134.0
65.90	134.0
66.80	293.0
68.00	7696.0
69.00	8508.0
70.00	849.0
71.00	102.0
71.90	395.0
73.00	3645.0
74.00	13103.0
75.00	37760.0
76.00	3394.0
77.10	428.0
77.90	250.0
78.90	2701.0
80.00	806.0
80.90	3034.0
81.90	685.0
82.90	146.0
85.10	108.0
85.80	133.0
86.90	2720.0
87.90	2664.0
90.80	325.0
91.90	2054.0
92.90	3118.0
94.00	8643.0
95.00	70280.0
96.00	4326.0
96.90	127.0
102.80	125.0
103.80	445.0
104.80	135.0
105.80	349.0
106.60	123.0
109.90	110.0
110.80	105.0
112.60	107.0
115.90	301.0
116.90	514.0
117.80	373.0
118.90	441.0
127.80	259.0
128.70	201.0
129.80	359.0
130.90	156.0
134.60	243.0
137.00	179.0
140.00	146.0
140.80	679.0
141.70	100.0
142.90	738.0
144.70	117.0
145.90	102.0
146.80	124.0
147.90	149.0
149.90	143.0
152.00	124.0
154.90	195.0
156.80	133.0
159.00	118.0
169.00	196.0
171.10	181.0
173.00	837.0

Instrument :
MSVOA_V
ClientSampleId :
BFB68

173.90	49928.0
175.00	3943.0
175.90	48040.0
176.90	2743.0
178.00	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB68

m/z	Abundance
35.90	1361.0
37.00	4589.0
38.00	4079.0
39.00	1587.0
40.00	346.0
41.00	279.0
42.00	144.0
43.00	239.0
43.90	945.0
45.00	913.0
45.90	188.0
47.00	986.0
47.80	542.0
49.00	4005.0
50.00	16448.0
51.00	4919.0
52.00	260.0
52.90	131.0
55.00	346.0
56.00	1564.0
57.00	2631.0
57.90	174.0
58.90	124.0
59.90	899.0
61.00	4360.0
62.00	3845.0
63.00	2890.0
64.00	454.0
64.90	163.0
66.00	133.0
66.80	294.0
68.00	7791.0
69.00	8539.0
70.00	837.0
71.00	158.0
71.90	418.0
73.00	3692.0
74.00	13563.0
75.00	38936.0
76.00	3458.0
77.10	403.0
77.80	288.0
78.90	2751.0
79.90	839.0
80.90	3155.0
81.90	719.0
82.90	187.0
85.80	154.0
86.90	2972.0
87.90	2758.0
90.90	281.0
92.00	2058.0
92.90	3091.0
94.00	9033.0
95.00	72488.0
96.00	4581.0
96.90	184.0
102.80	103.0
103.90	437.0
104.80	177.0
105.80	404.0
109.80	128.0
114.70	103.0
116.00	315.0
116.80	543.0
117.80	401.0
118.90	510.0
127.80	251.0
128.70	229.0
129.90	397.0
130.90	166.0
134.60	260.0
137.00	200.0
140.00	148.0
140.80	734.0
141.70	133.0
142.90	787.0
144.70	117.0
146.80	113.0
148.00	167.0
149.90	182.0
152.00	111.0
154.00	120.0
154.90	198.0
156.80	109.0
168.90	208.0
171.10	131.0
173.00	855.0
173.90	53584.0
174.90	4026.0
175.90	51920.0
176.90	2935.0

Instrument :
MSVOA_V
ClientSampleId :
BFB68

m/z	Abundance
35.90	1367.0
37.00	4180.0
38.00	3921.0
39.00	1434.0
39.90	340.0
41.00	283.0
42.00	161.0
43.00	229.0
44.00	977.0
45.00	877.0
45.80	180.0
47.00	957.0
47.80	530.0
49.00	3886.0
50.00	15684.0
51.00	4316.0
51.90	274.0
52.90	138.0
55.00	342.0
56.00	1381.0
56.90	2384.0
57.80	171.0
58.90	114.0
60.00	784.0
61.00	4068.0
62.00	3679.0
63.00	2769.0
64.00	364.0
64.90	176.0
66.00	132.0
66.80	228.0
68.00	7516.0
69.00	7892.0
70.00	791.0
71.00	165.0
72.00	431.0
73.00	3426.0
74.00	12992.0
75.00	37056.0
76.00	3184.0
76.90	409.0
77.80	298.0
78.90	2617.0
79.90	798.0
80.90	3080.0
81.90	666.0
82.90	195.0
85.90	144.0
86.90	2867.0
88.00	2707.0
90.90	253.0
92.00	1973.0
92.90	2899.0
94.00	8672.0
95.00	68952.0
96.00	4417.0
97.00	239.0
103.90	395.0
104.80	185.0
105.80	403.0
109.80	129.0
113.60	103.0
114.70	105.0
115.20	138.0
116.00	284.0
116.80	548.0
117.90	347.0
118.90	553.0
127.80	233.0
128.80	203.0
129.80	348.0
130.80	158.0
134.60	222.0
137.00	209.0
139.60	109.0
140.90	720.0
141.70	137.0
142.90	798.0
143.80	110.0
144.70	119.0
145.80	117.0
146.80	112.0
147.70	191.0
149.90	199.0
154.90	186.0
157.00	112.0
160.90	117.0
168.80	212.0
171.40	143.0
172.10	263.0
173.00	777.0
173.90	52432.0

Instrument :
MSVOA_V
ClientSampleId :
BFB68

174.90	3854.0
175.90	51048.0
176.90	2965.0

Instrument :
MSVOA_V
ClientSampleId :
BFB68