

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060419\
 Data File : VV011214.D
 Acq On : 04 Jun 2019 19:13
 Operator : SY/MD
 Sample : K2888-16
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BP8

Quant Time: Jun 05 02:17:17 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Jun 05 01:41:25 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	167753	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	151721	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	65175	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	58366	4.59	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.80%
7) Chloroethane-d5	1.56	69	47360	4.48	ug/L	-0.02
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.60%
11) 1,1-Dichloroethene-d2	2.12	63	91621	3.61	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.20%
20) 2-Butanone-d5	3.95	46	156093	54.54	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.08%
24) Chloroform-d	4.40	84	106340	4.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.00%
26) 1,2-Dichloroethane-d4	5.08	65	58647	4.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.00%
32) Benzene-d6	5.10	84	222016	4.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.80%
36) 1,2-Dichloropropane-d6	6.12	67	67476	4.83	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.60%
41) Toluene-d8	7.36	98	195361	4.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.80%
43) trans-1,3-Dichloropropene-	7.67	79	24422	4.58	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.60%
46) 2-Hexanone-d5	8.14	63	125370	55.68	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	111.36%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	48271	5.06	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.20%
64) 1,2-Dichlorobenzene-d4	11.67	152	63976	4.97	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.40%


Target Compounds					Ovalue
13) Acetone	2.20	43	10660	5.556 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060419\
Data File : VV011214.D
Acq On : 04 Jun 2019 19:13
Operator : SY/MD
Sample : K2888-16
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BP8

Quant Time: Jun 05 02:17:17 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jun 05 01:41:25 2019
Response via : Initial Calibration

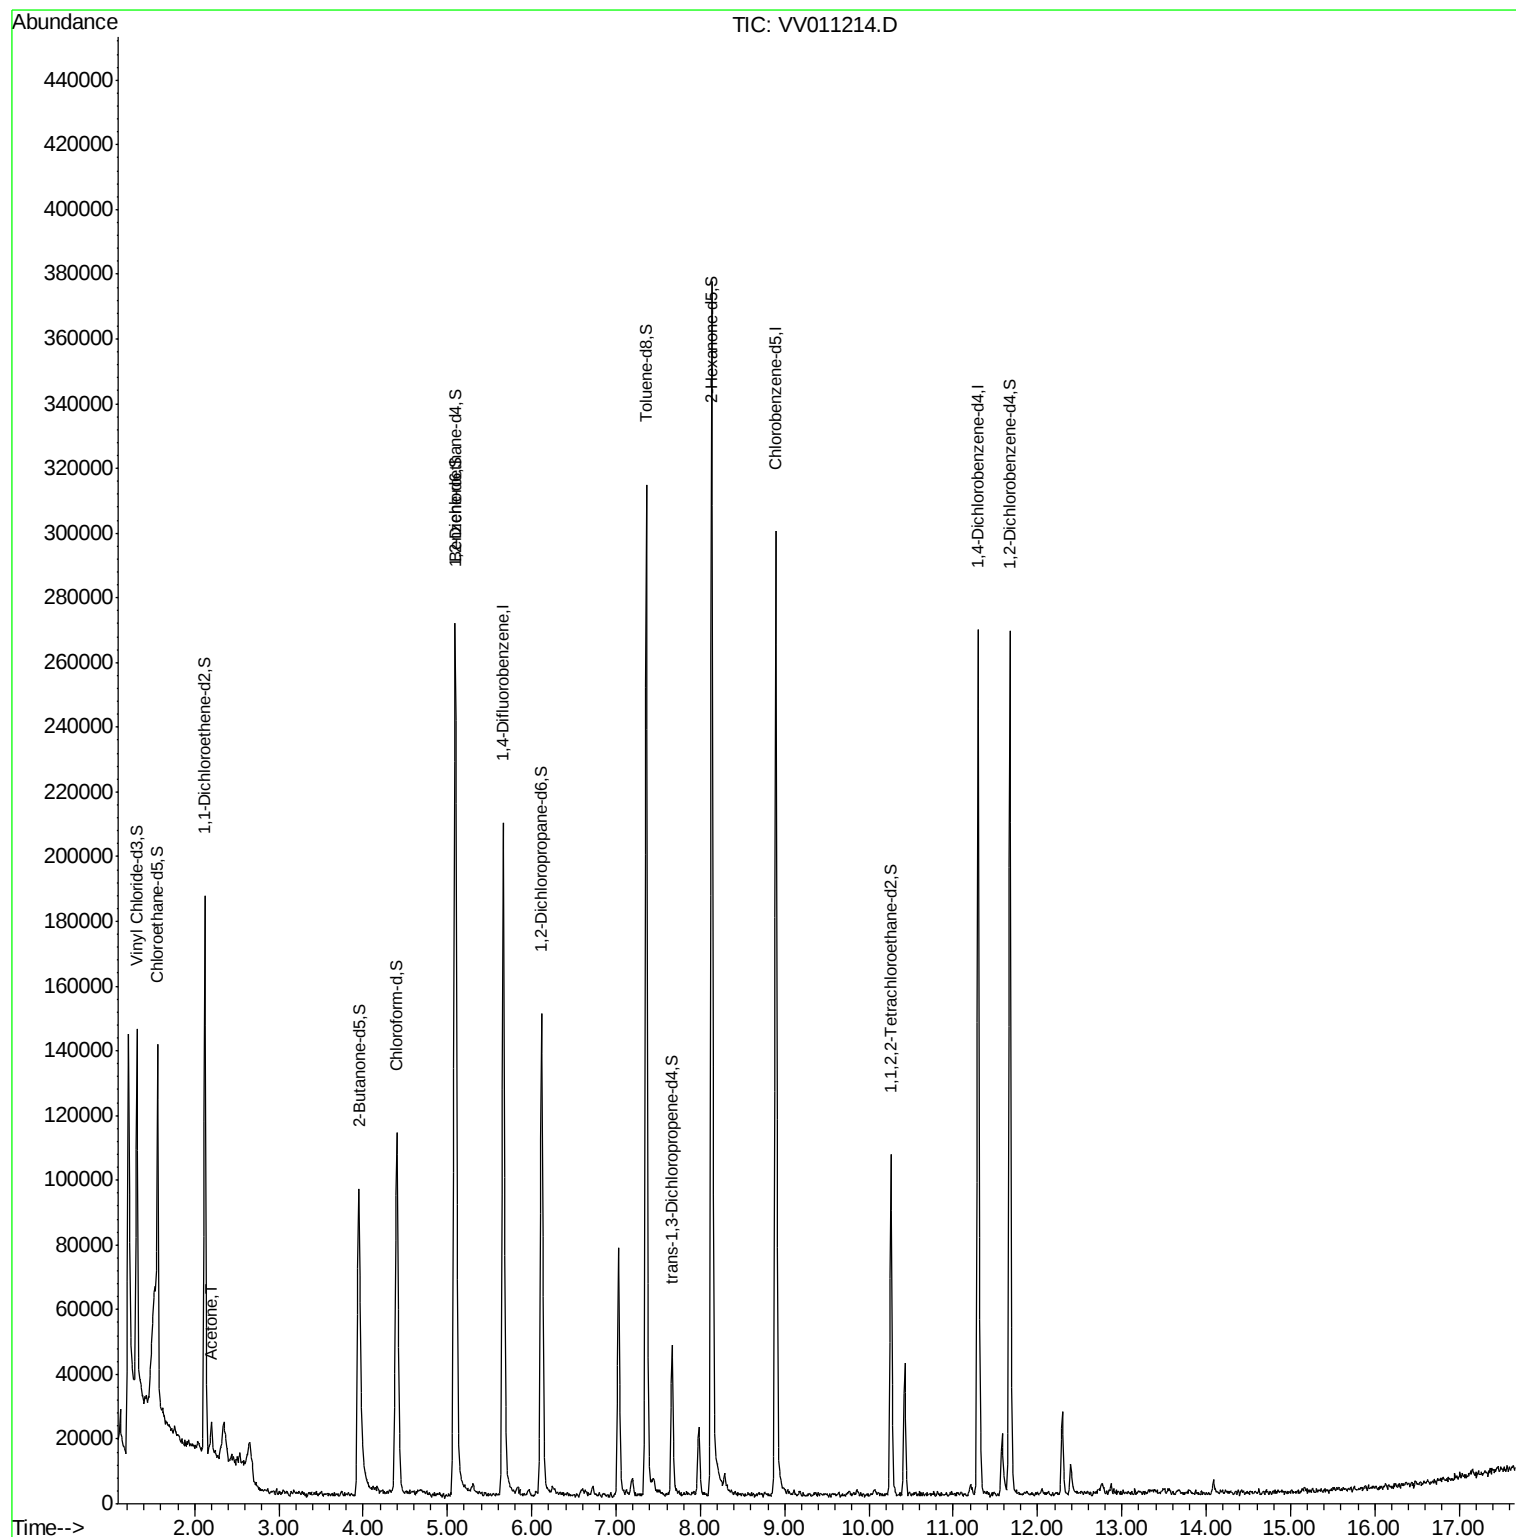

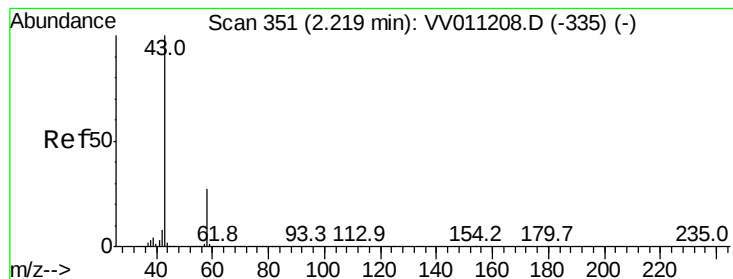

#13

Acetone

Concen: 5.556 ug/L

RT: 2.20 min Scan# 345

Delta R.T. -0.02 min

Lab File: VV011214.D

Acq: 04 Jun 2019 19:13

Instrument :
MSVOA_V
ClientSampleId :
C0BP8

Tot Ion: 43 Resp: 10660

Ion Ratio Lower Upper

43 100

58 25.9 0.0 55.2

