

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060419\
 Data File : VV011216.D
 Acq On : 04 Jun 2019 20:04
 Operator : SY/MD
 Sample : K2889-15
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BN2

Quant Time: Jun 05 02:28:27 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Jun 05 01:41:25 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	174652	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	159642	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	69467	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	60644	4.58	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.60%
7) Chloroethane-d5	1.56	69	46898	4.26	ug/L	-0.02
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.20%
11) 1,1-Dichloroethene-d2	2.12	63	90599	3.43	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.60%
20) 2-Butanone-d5	3.94	46	162765	54.63	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.26%
24) Chloroform-d	4.40	84	106901	4.59	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.80%
26) 1,2-Dichloroethane-d4	5.08	65	60735	4.82	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.40%
32) Benzene-d6	5.09	84	223875	4.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.80%
36) 1,2-Dichloropropane-d6	6.12	67	69521	4.73	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.60%
41) Toluene-d8	7.36	98	202587	4.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.40%
43) trans-1,3-Dichloropropene-	7.66	79	24701	4.40	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.00%
46) 2-Hexanone-d5	8.13	63	136134	57.46	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	114.92%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	51381	5.12	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.40%
64) 1,2-Dichlorobenzene-d4	11.67	152	67079	4.89	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.80%


Target Compounds					Ovalue
13) Acetone	2.19	43	20139	10.081 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060419\
Data File : VV011216.D
Acq On : 04 Jun 2019 20:04
Operator : SY/MD
Sample : K2889-15
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BN2

Quant Time: Jun 05 02:28:27 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jun 05 01:41:25 2019
Response via : Initial Calibration

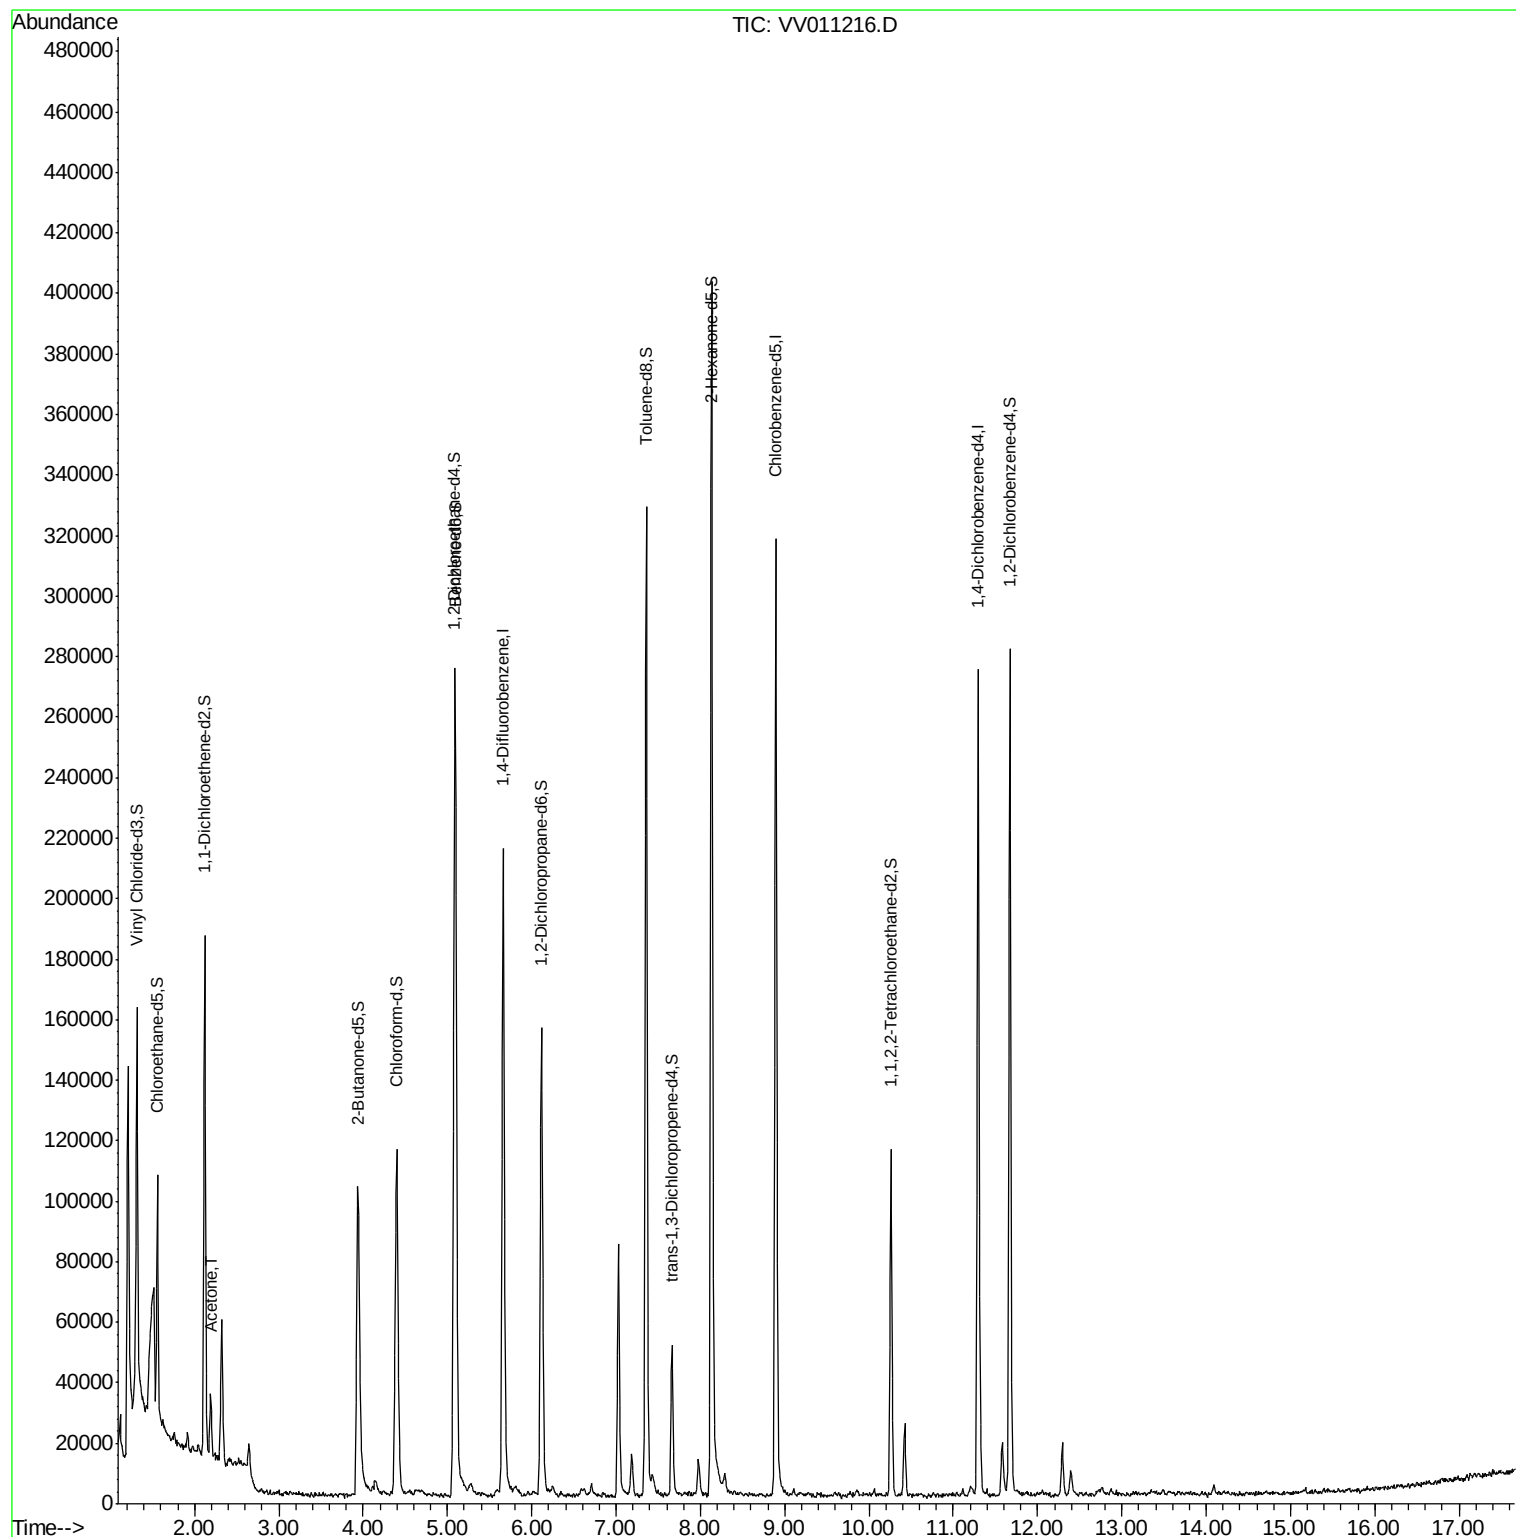

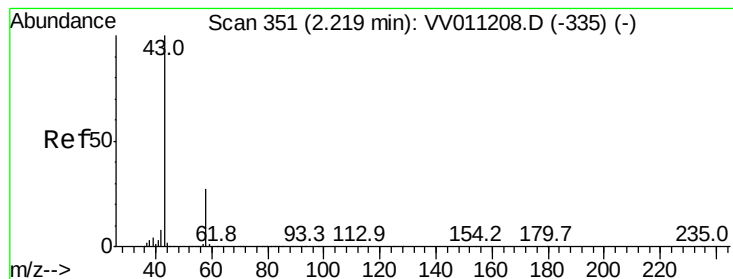

#13

Acetone

Concen: 10.081 ug/L

RT: 2.19 min Scan# 343

Delta R.T. -0.03 min

Lab File: VV011216.D

Acq: 04 Jun 2019 20:04

Instrument :
MSVOA_V
ClientSampleId :
C0BN2

Tot Ion: 43 Resp: 20139

Ion Ratio Lower Upper

43 100

58 27.9 0.0 55.2

