


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV060419\
 Data File : VV011201.D
 Acq On : 04 Jun 2019 11:59
 Operator : SY/MD
 Sample : BFB42
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB42

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Jun 05 05:12:22 2019

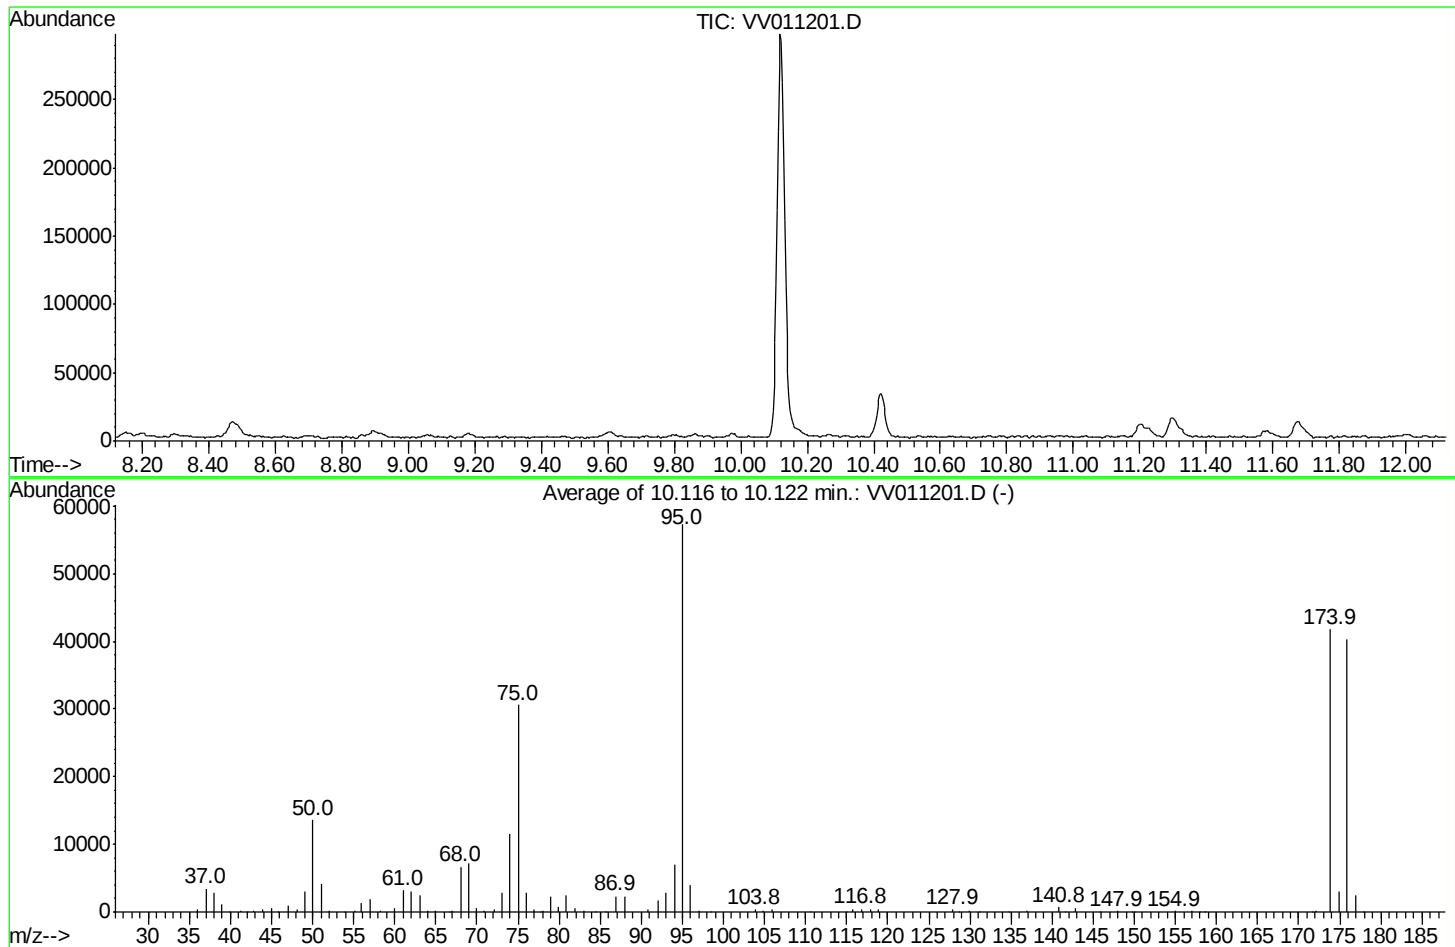

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.6	13541	PASS
75	95	30	80	53.5	30648	PASS
95	95	100	100	100.0	57298	PASS
96	95	5	9	6.9	3958	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.9	41792	PASS
175	174	5	9	7.3	3060	PASS
176	174	95	101	96.4	40304	PASS
177	176	5	9	6.3	2536	PASS

m/z	Abundance
35.60	111.0
36.00	119.0
38.00	150.0
39.10	123.0
39.90	315.0
40.90	242.0
41.80	206.0
43.90	619.0
45.00	118.0
47.50	117.0
49.50	124.0
55.10	132.0
56.70	109.0
57.80	153.0
66.90	114.0
68.90	105.0
78.90	123.0
169.10	155.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42

m/z	Abundance
36.00	619.0
37.00	3312.0
38.00	2876.0
39.00	1187.0
39.90	356.0
40.90	166.0
41.20	166.0
41.70	145.0
42.10	147.0
42.80	139.0
43.90	1001.0
45.00	585.0
47.00	804.0
48.00	438.0
49.00	2928.0
50.00	13242.0
51.00	4052.0
52.10	281.0
55.10	310.0
56.00	1186.0
57.00	1924.0
58.20	130.0
59.90	547.0
61.00	3060.0
62.00	2970.0
63.00	2258.0
63.90	314.0
64.90	106.0
66.60	166.0
67.10	215.0
68.00	6472.0
69.00	6859.0
69.90	577.0
70.90	134.0
72.10	365.0
73.00	2684.0
74.00	11144.0
75.00	29312.0
76.00	2866.0
76.90	487.0
77.70	223.0
78.90	2317.0
80.00	685.0
80.90	2388.0
81.90	504.0
83.10	121.0
85.60	111.0
86.90	2293.0
88.00	2310.0
90.90	284.0
92.00	1580.0
93.00	2811.0
94.00	6859.0
95.00	54400.0
96.00	3932.0
96.90	151.0
103.90	376.0
104.80	181.0
105.90	336.0
110.60	121.0
115.80	261.0
116.80	414.0
117.80	310.0
118.90	358.0
127.90	253.0
129.90	189.0
134.70	109.0
136.80	140.0
140.80	683.0
141.60	108.0
142.90	566.0
148.10	177.0
150.00	102.0
154.90	190.0
156.90	155.0
168.90	114.0
172.10	150.0
173.90	38928.0
175.00	2948.0
175.90	37096.0
176.90	2389.0
177.80	124.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42

m/z	Abundance
36.00	595.0
37.00	3545.0
38.00	3142.0
39.00	1223.0
39.80	327.0
41.20	193.0
41.80	160.0
42.70	142.0
43.90	990.0
44.90	645.0
45.80	117.0
47.00	996.0
48.00	469.0
49.00	3075.0
50.00	14038.0
51.00	4414.0
52.00	260.0
53.90	102.0
55.10	324.0
55.90	1286.0
57.00	1943.0
58.20	134.0
60.00	606.0
61.00	3269.0
62.00	3147.0
63.00	2520.0
64.00	277.0
64.90	138.0
67.10	259.0
68.00	6993.0
69.00	7561.0
69.90	626.0
70.90	150.0
72.10	442.0
73.00	2830.0
74.00	12002.0
75.00	31392.0
76.00	3027.0
76.90	473.0
77.90	253.0
78.90	2523.0
79.90	741.0
80.90	2561.0
81.90	578.0
83.00	136.0
84.40	123.0
85.60	103.0
86.90	2423.0
88.00	2358.0
90.80	348.0
92.00	1768.0
93.00	2947.0
94.00	7222.0
95.00	59064.0
96.00	4087.0
97.00	144.0
98.40	105.0
103.90	347.0
104.80	183.0
105.90	305.0
110.60	103.0
114.90	128.0
115.80	304.0
116.80	423.0
117.80	307.0
118.90	368.0
127.90	328.0
128.60	104.0
129.80	218.0
134.80	106.0
136.90	195.0
140.90	726.0
141.60	109.0
142.90	682.0
145.80	117.0
147.90	168.0
149.70	105.0
155.00	181.0
157.00	150.0
168.90	126.0
171.60	106.0
172.10	189.0
173.90	43224.0
174.90	3161.0
175.90	41632.0
176.90	2588.0
177.90	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42

m/z	Abundance
36.00	565.0
37.00	3485.0
38.00	3135.0
39.00	1198.0
39.80	304.0
41.20	193.0
41.80	152.0
42.70	140.0
43.90	950.0
44.90	641.0
45.80	116.0
47.00	1031.0
48.10	444.0
49.00	2967.0
50.00	13343.0
51.00	4003.0
52.00	238.0
55.00	321.0
55.90	1243.0
57.00	1857.0
58.20	110.0
60.00	594.0
61.00	3180.0
62.00	3147.0
63.00	2473.0
64.00	245.0
64.90	149.0
67.10	249.0
68.00	6687.0
69.00	7299.0
69.90	572.0
70.90	123.0
72.10	494.0
73.00	2803.0
74.00	11441.0
75.00	31240.0
76.00	2821.0
77.00	465.0
78.00	295.0
78.90	2479.0
79.90	686.0
80.90	2449.0
81.80	601.0
83.00	124.0
84.40	128.0
86.90	2318.0
88.00	2196.0
90.80	308.0
92.00	1767.0
92.90	2848.0
94.00	6945.0
95.00	58432.0
96.00	3856.0
97.10	154.0
98.40	125.0
103.80	294.0
104.80	152.0
105.90	292.0
114.90	141.0
115.70	342.0
116.80	389.0
117.90	325.0
118.90	365.0
127.90	361.0
128.60	104.0
129.80	277.0
131.20	119.0
136.90	231.0
140.90	707.0
142.80	760.0
145.70	136.0
147.80	176.0
149.60	122.0
155.00	161.0
157.00	113.0
157.90	116.0
158.50	113.0
168.90	135.0
171.60	103.0
173.90	43224.0
174.90	3072.0
175.90	42184.0
176.90	2632.0

Instrument :
MSVOA_V
ClientSampleId :
BFB42