


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV060519\
Data File : VV011222.D
Acq On : 05 Jun 2019 09:35
Operator : SY/MD
Sample : BFB43
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB43

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Jun 07 08:11:19 2019

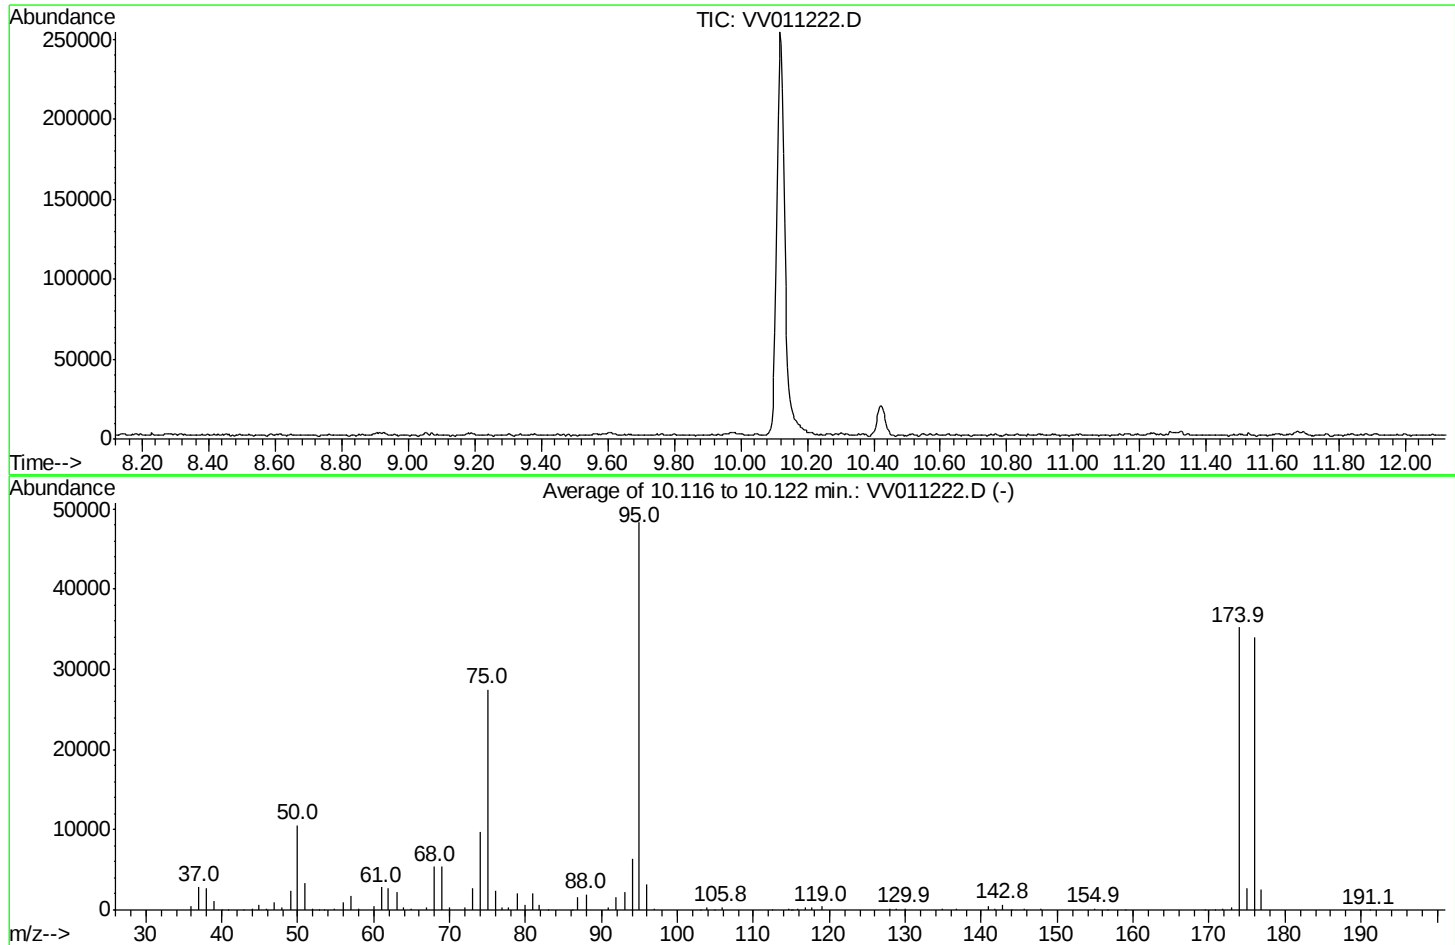

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	10612	PASS
75	95	30	80	56.9	27520	PASS
95	95	100	100	100.0	48336	PASS
96	95	5	9	6.7	3237	PASS
173	174	0.00	2	0.9	324	PASS
174	95	50	120	72.9	35240	PASS
175	174	5	9	7.7	2730	PASS
176	174	95	101	96.4	33962	PASS
177	176	5	9	7.5	2542	PASS

Scan 2794 (10.074 min): VV011222.D
BFB43

m/z	Abundance
36.10	115.0
36.60	120.0
37.20	104.0
37.80	109.0
39.90	295.0
41.00	170.0
41.70	129.0
42.80	152.0
43.90	692.0
47.20	105.0
50.00	106.0
58.90	126.0
64.30	103.0
69.90	107.0
156.40	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB43

m/z	Abundance
36.00	633.0
37.00	2859.0
38.00	2800.0
39.00	1045.0
39.90	375.0
41.20	156.0
42.80	161.0
44.00	876.0
44.90	611.0
45.90	182.0
47.00	957.0
47.80	367.0
49.00	2295.0
50.00	10421.0
51.00	3235.0
52.00	179.0
52.80	103.0
54.90	224.0
55.90	1037.0
57.00	1667.0
58.00	147.0
60.00	513.0
61.00	2766.0
61.90	2699.0
63.00	2216.0
63.90	280.0
65.00	166.0
66.90	224.0
68.00	5188.0
69.00	5337.0
70.00	473.0
72.00	308.0
73.00	2824.0
74.00	9291.0
75.00	27376.0
76.00	2380.0
77.00	345.0
77.70	325.0
78.80	1994.0
79.90	565.0
80.90	2075.0
81.90	592.0
86.90	1621.0
88.00	1772.0
90.80	288.0
92.00	1547.0
93.00	2218.0
94.00	6355.0
95.00	47120.0
96.00	3217.0
97.00	148.0
103.00	105.0
103.90	300.0
105.80	305.0
114.70	161.0
115.90	201.0
116.80	343.0
117.70	222.0
118.90	406.0
127.90	205.0
128.90	174.0
130.00	214.0
134.90	145.0
136.80	135.0
140.80	532.0
141.80	168.0
142.90	642.0
145.60	107.0
147.80	139.0
154.90	152.0
156.60	138.0
158.90	108.0
170.80	126.0
171.70	222.0
173.90	33448.0
174.90	2596.0
175.90	31848.0
176.90	2386.0

Instrument :
MSVOA_V
ClientSampleId :
BFB43

m/z	Abundance
36.00	617.0
37.00	3104.0
38.00	2816.0
39.00	1084.0
39.90	320.0
41.20	149.0
41.90	109.0
42.90	169.0
44.00	868.0
45.00	601.0
45.90	150.0
46.90	995.0
47.80	403.0
49.00	2511.0
50.00	11063.0
51.00	3475.0
51.90	180.0
53.50	108.0
54.80	216.0
56.00	1003.0
57.00	1733.0
58.10	156.0
60.00	568.0
61.00	2919.0
62.00	2808.0
63.00	2263.0
63.90	300.0
65.00	136.0
66.90	261.0
68.00	5497.0
69.00	5618.0
70.00	477.0
72.00	357.0
73.00	2928.0
74.00	9965.0
75.00	28392.0
76.00	2593.0
77.00	343.0
77.80	300.0
78.90	2168.0
79.90	644.0
80.90	2216.0
81.80	644.0
86.90	1683.0
87.90	2028.0
90.80	281.0
91.90	1707.0
93.00	2300.0
94.00	6636.0
95.00	49952.0
96.00	3267.0
97.00	125.0
102.90	102.0
103.90	331.0
104.90	110.0
105.80	345.0
114.70	144.0
114.90	126.0
115.80	213.0
116.80	372.0
117.80	266.0
119.00	506.0
127.90	201.0
128.80	193.0
130.00	231.0
134.90	176.0
136.80	134.0
140.80	515.0
141.70	188.0
142.90	721.0
144.00	108.0
145.60	108.0
147.90	181.0
154.90	181.0
156.70	112.0
171.70	223.0
172.90	487.0
173.90	36320.0
174.90	2813.0
175.90	35096.0
176.90	2665.0
191.10	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB43

m/z	Abundance
36.00	596.0
37.00	3079.0
38.00	2770.0
39.00	1017.0
39.90	285.0
40.80	138.0
41.10	137.0
41.90	139.0
42.90	144.0
44.00	901.0
45.00	567.0
45.90	127.0
46.90	835.0
47.90	428.0
49.00	2573.0
50.00	10672.0
51.00	3426.0
51.90	179.0
53.50	117.0
54.70	216.0
56.00	894.0
57.00	1704.0
57.90	141.0
60.00	601.0
61.00	2737.0
62.00	2644.0
63.00	2176.0
64.00	300.0
65.00	104.0
66.90	267.0
68.00	5379.0
69.00	5452.0
69.90	482.0
72.00	336.0
73.00	2600.0
74.00	9813.0
75.00	26792.0
76.00	2452.0
76.90	337.0
77.80	228.0
78.90	2107.0
79.90	690.0
80.90	2156.0
81.80	603.0
82.90	142.0
86.10	140.0
86.90	1693.0
87.90	1982.0
90.80	278.0
91.90	1683.0
93.00	2194.0
94.00	6318.0
95.00	47936.0
96.00	3228.0
96.90	109.0
103.80	303.0
104.90	122.0
105.80	324.0
112.50	101.0
114.70	107.0
115.10	118.0
115.80	248.0
116.80	358.0
117.80	296.0
119.00	487.0
127.90	185.0
128.80	167.0
129.90	208.0
134.90	167.0
136.80	118.0
140.90	421.0
141.60	171.0
142.80	709.0
144.00	119.0
145.60	105.0
147.90	201.0
154.90	190.0
169.40	109.0
171.80	197.0
172.90	487.0
173.90	35952.0
174.90	2781.0
175.90	34944.0
176.90	2575.0
191.10	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB43