

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060624\
 Data File : VV035980.D
 Acq On : 06 Jun 2024 12:11
 Operator : SY/MD
 Sample : VV0606SBL01
 Misc : 5.00g/10.0mL/MSVOA_V/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK315

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 06/07/2024
 Supervised By :Semsettin Yesilyurt 06/07/2024

Quant Time: Jun 07 02:17:41 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 07 02:16:44 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	429904	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	401007	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	164089	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	185246	23.438	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	93.760%		
7) Chloroethane-d5	1.526	69	153502	24.357	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	97.440%		
11) 1,1-Dichloroethene-d2	2.053	65	81915	23.281	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	93.120%		
21) 2-Butanone-d5	3.809	46	49480m	27.285	ug/L	-0.03
Spiked Amount 50.000	Range 20 - 135		Recovery =	54.580%		
24) Chloroform-d	4.239	84	306085	22.395	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	89.560%		
26) 1,2-Dichloroethane-d4	4.934	65	140089	19.549	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	78.200%		
32) Benzene-d6	4.950	84	605080	25.384	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	101.520%		
36) 1,2-Dichloropropane-d6	5.982	67	184639	24.597	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	98.400%		
41) Toluene-d8	7.239	98	508361	24.171	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	96.680%		
43) trans-1,3-Dichloroprop...	7.551	79	59177	19.227	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	76.920%		
47) 2-Hexanone-d5	8.030	63	28011	27.542	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	55.080%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	108304	19.308	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	77.240%		
66) 1,2-Dichlorobenzene-d4	11.558	152	153131	25.448	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	101.800%		
Target Compounds						Qvalue
16) Methylene chloride	2.442	84	30510	3.136	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060624\
Data File : VV035980.D
Acq On : 06 Jun 2024 12:11
Operator : SY/MD
Sample : VV0606SBL01
Misc : 5.00g/10.0mL/MSVOA_V/SOIL
ALS Vial : 5 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
VBLK315

Quant Time: Jun 07 02:17:41 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 07 02:16:44 2024
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 06/07/2024
Supervised By :Semsettin Yesilyurt 06/07/2024

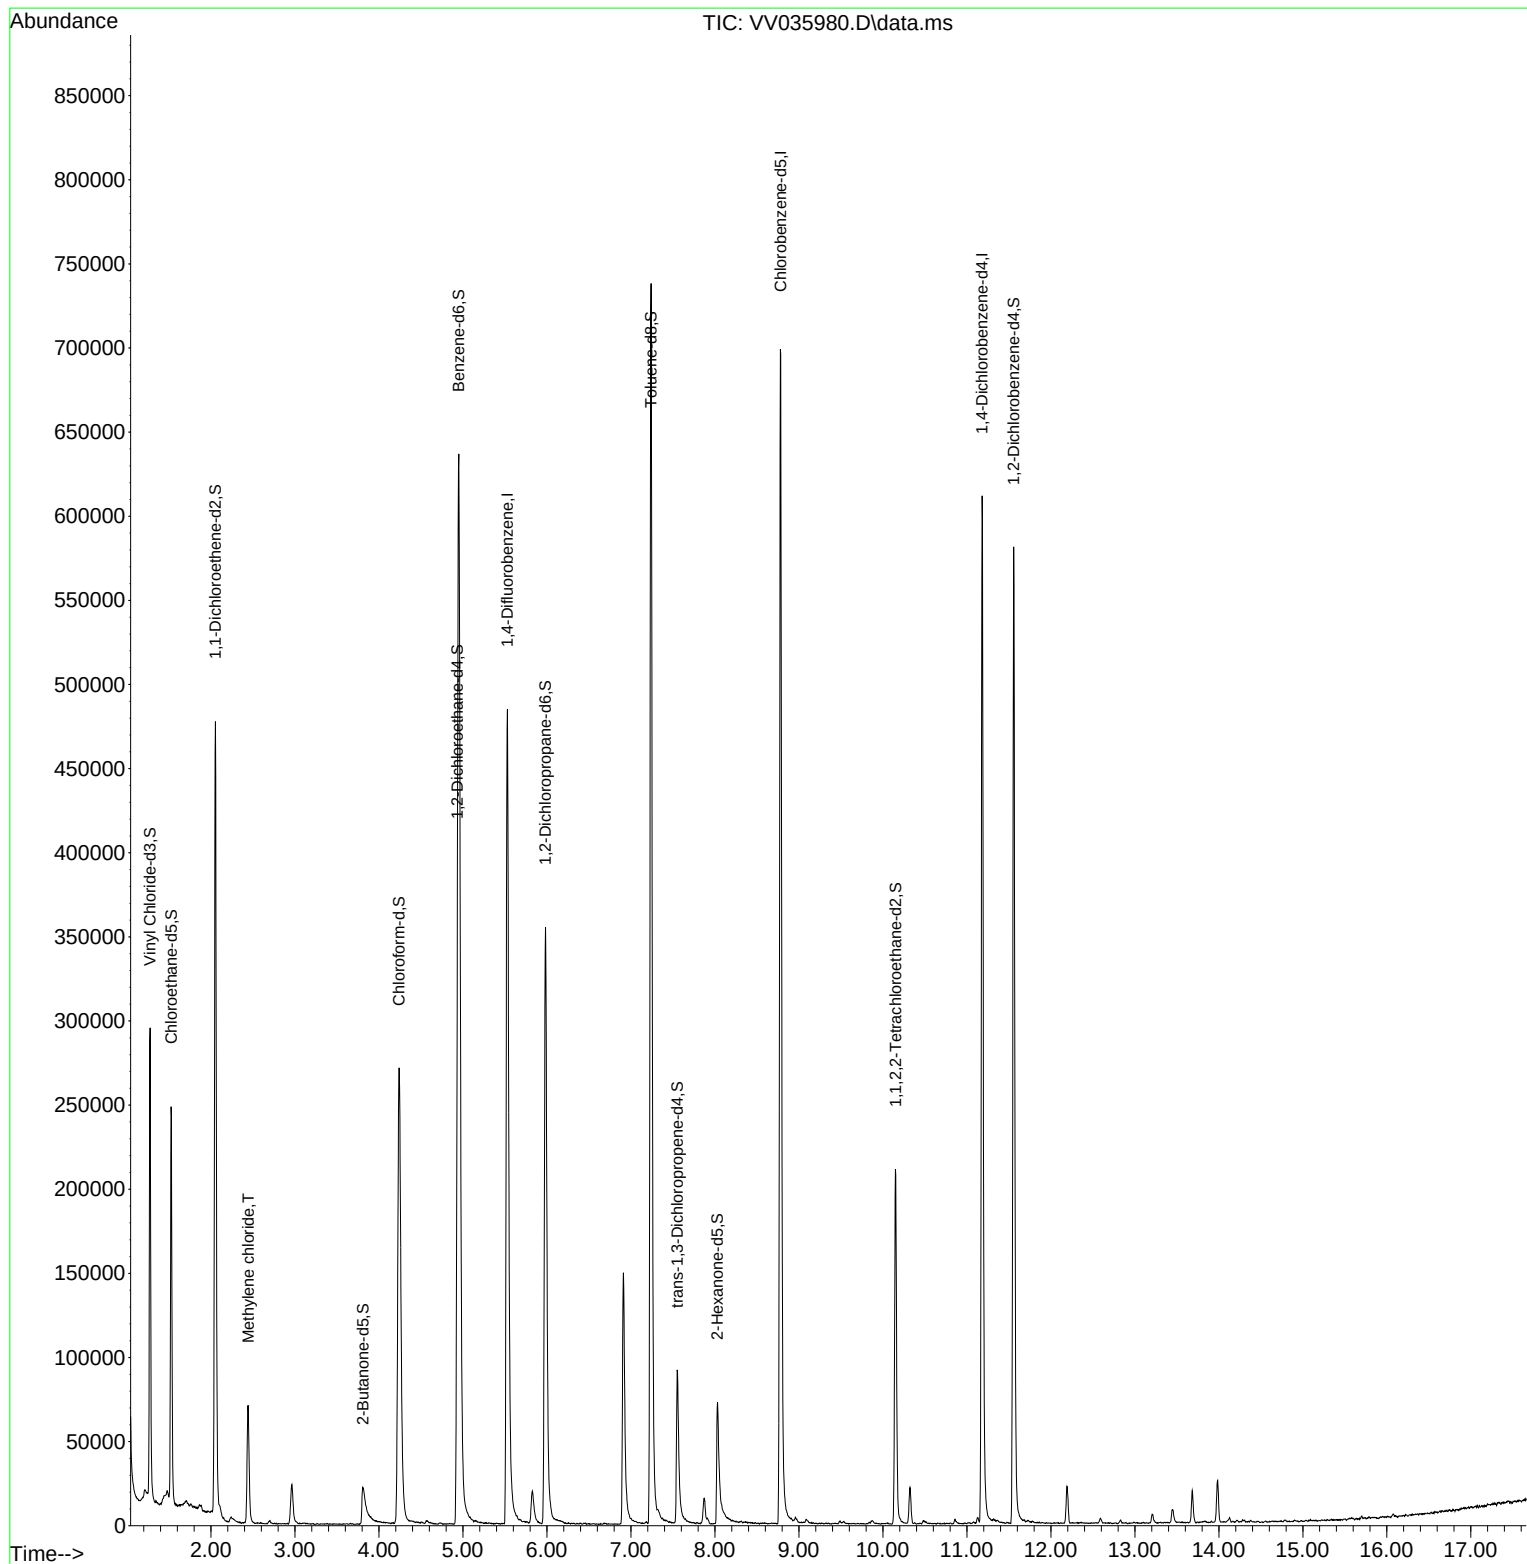

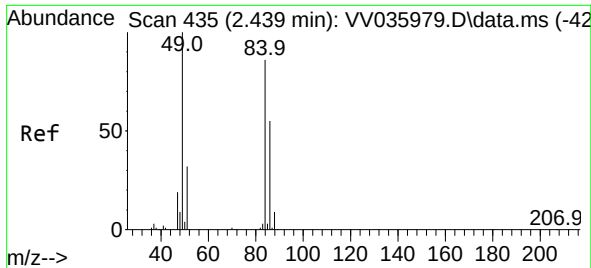

#16
Methylene chloride
Concen: 3.136 ug/L
RT: 2.442 min Scan# 41
Delta R.T. 0.003 min
Lab File: VV035980.D
Acq: 06 Jun 2024 12:11

Instrument :
MSVOA_V
ClientSampleId :
VBLK315

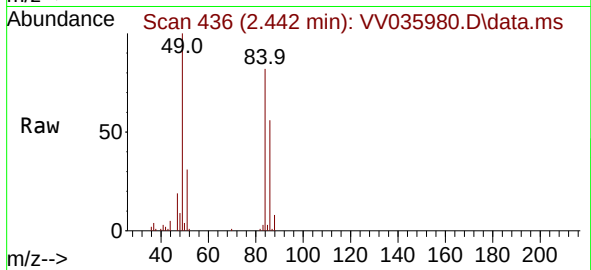

Tgt Ion: 84 Resp: 30510
Ion Ratio Lower Upper
84 100
86 68.5 44.6 82.8
49 122.2 81.1 150.5

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 06/07/2024
Supervised By :Semsettin Yesilyurt 06/07/2024

