

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060724\
 Data File : VV036008.D
 Acq On : 07 Jun 2024 14:16
 Operator : SY/MD
 Sample : P2754-03
 Misc : 4.34g/10.0mL/MSVOA_V/SOIL/B
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jun 08 00:32:17 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 08 00:30:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	420716	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	265934	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	56128	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	114152	14.758	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	59.040%
7) Chloroethane-d5	1.738	69	115	0.019	ug/L	0.21
Spiked Amount	25.000	Range	30 - 150	Recovery	=	0.080%#
11) 1,1-Dichloroethene-d2	2.056	65	48587	14.110	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	56.440%
21) 2-Butanone-d5	3.838	46	12286	6.923	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	13.840%#
24) Chloroform-d	4.246	84	207432	15.508	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	62.040%
26) 1,2-Dichloroethane-d4	4.944	65	87252	12.442	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	49.760%#
32) Benzene-d6	4.957	84	371295	23.488	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.960%
36) 1,2-Dichloropropane-d6	5.989	67	121360	24.379	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.520%
41) Toluene-d8	7.243	98	237016	16.993	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	67.960%
43) trans-1,3-Dichloroprop...	7.564	79	22836	11.188	ug/L	0.01
Spiked Amount	25.000	Range	30 - 135	Recovery	=	44.760%
47) 2-Hexanone-d5	8.043	63	8337	12.361	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	24.720%
56) 1,1,2,2-Tetrachloroeth...	10.152	84	51886	13.948	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	55.800%
66) 1,2-Dichlorobenzene-d4	11.561	152	31489	15.299	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	61.200%#
Target Compounds						Qvalue
25) Chloroform	4.275	83	8279	0.591	ug/L	98
35) Methylcyclohexane	5.989	83	27370	3.713	ug/L #	19


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060724\
Data File : VV036008.D
Acq On : 07 Jun 2024 14:16
Operator : SY/MD
Sample : P2754-03
Misc : 4.34g/10.0mL/MSVOA_V/SOIL/B
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Jun 08 00:32:17 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 08 00:30:25 2024
Response via : Initial Calibration

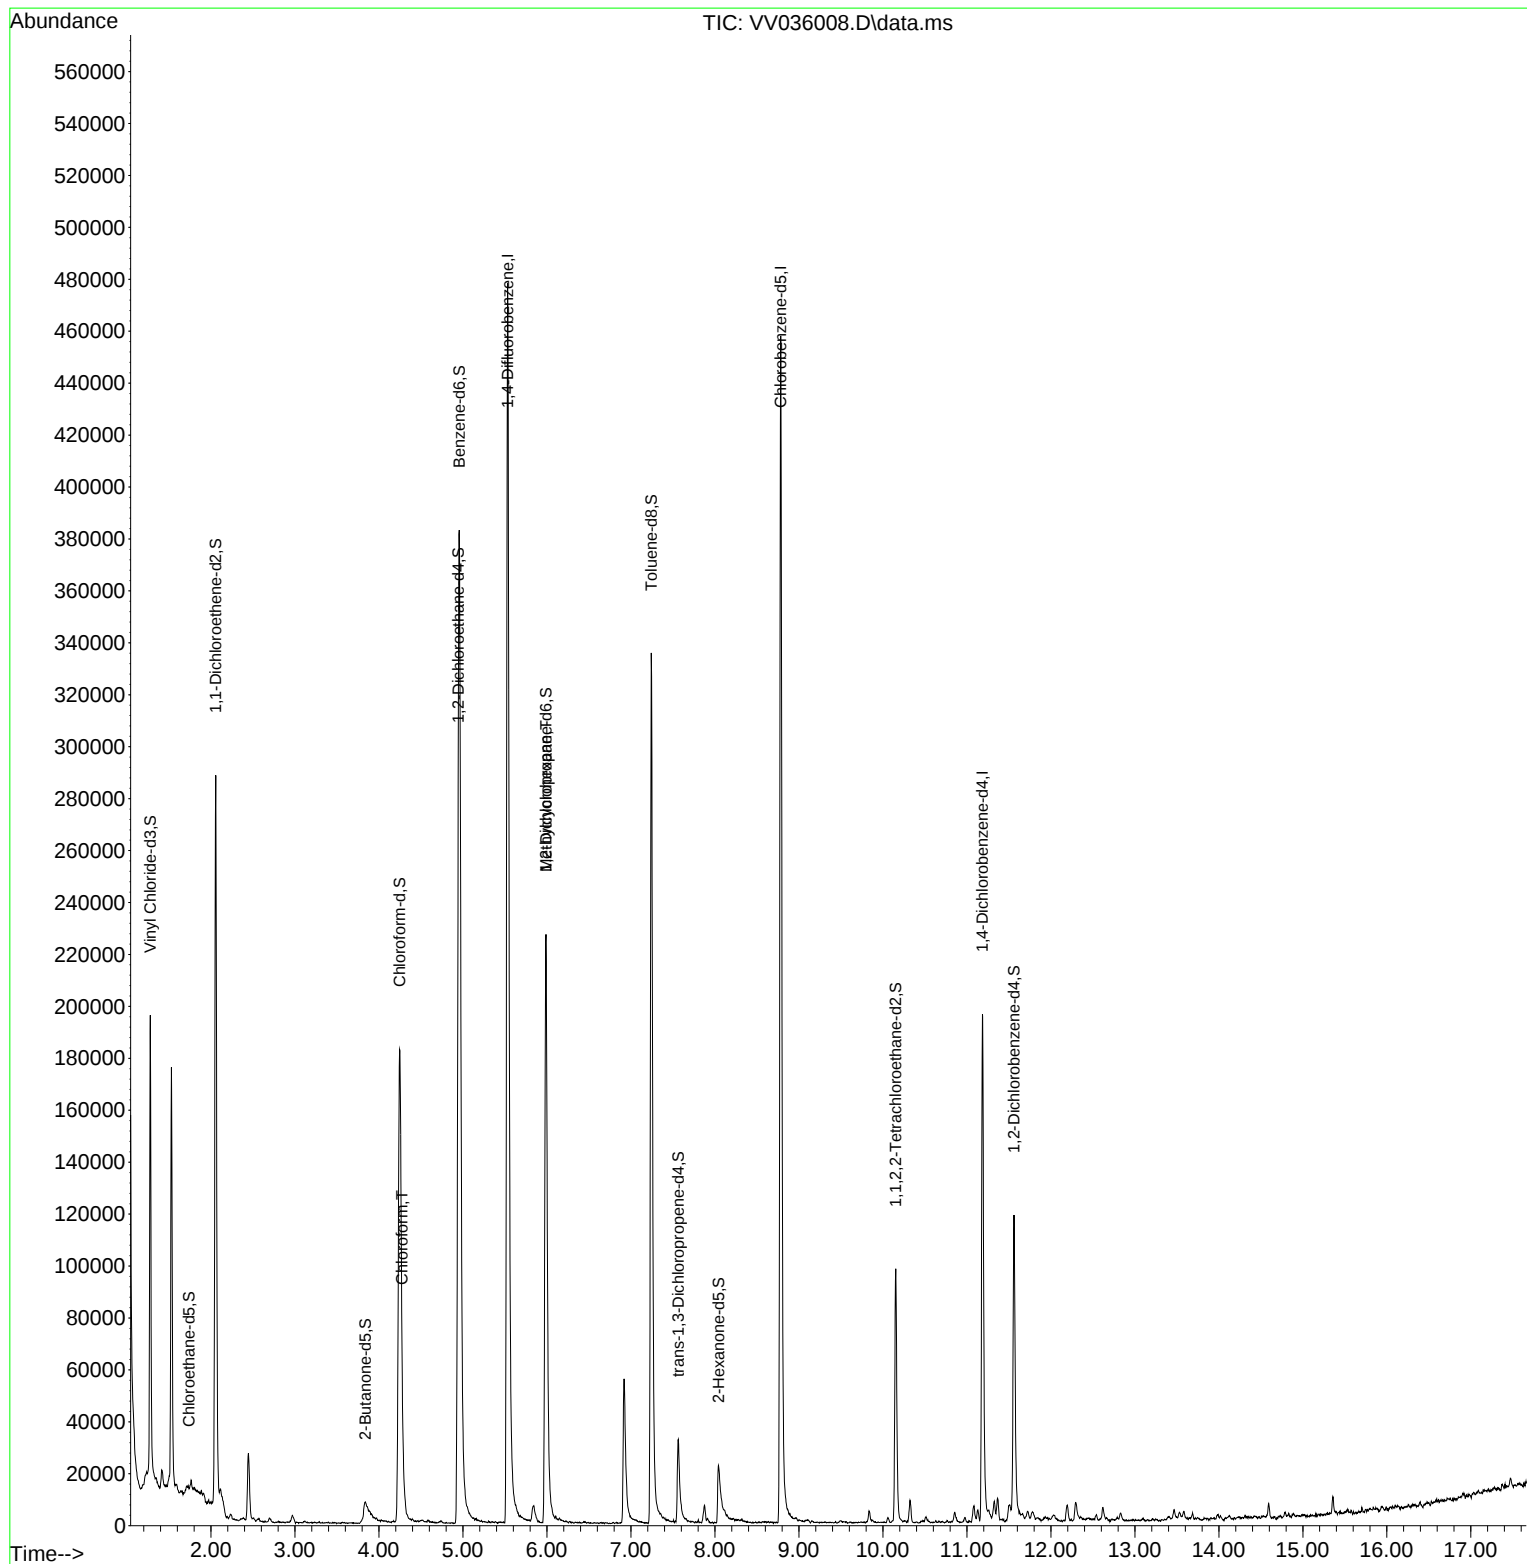

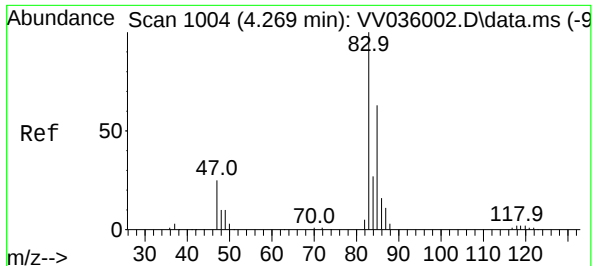

#25

Chloroform

Concen: 0.591 ug/L

RT: 4.275 min Scan# 1

Delta R.T. 0.006 min

Lab File: VV036008.D

Acq: 07 Jun 2024 14:16

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 83 Resp: 8279

Ion Ratio Lower Upper

83 100

85 66.1 45.2 84.0

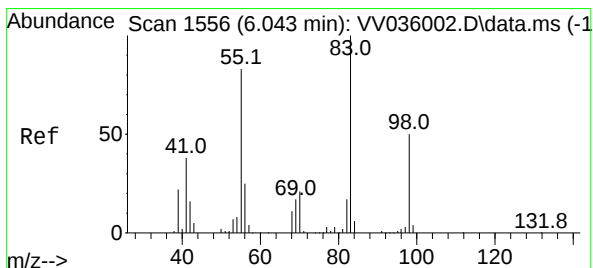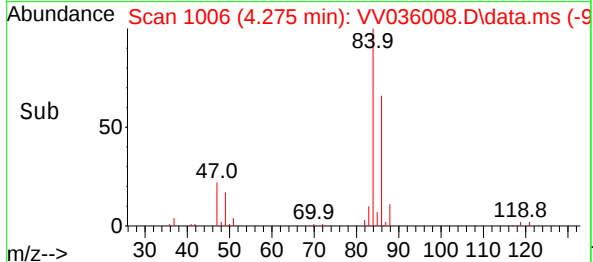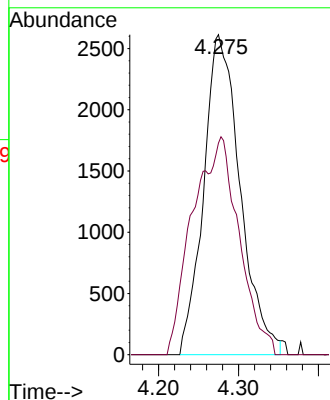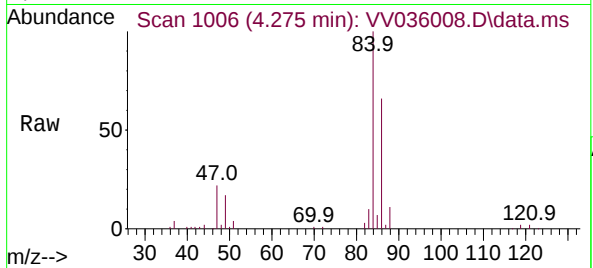

#35

Methylcyclohexane

Concen: 3.713 ug/L

RT: 5.989 min Scan# 1539

Delta R.T. -0.055 min

Lab File: VV036008.D

Acq: 07 Jun 2024 14:16

Tgt Ion: 83 Resp: 27370

Ion Ratio Lower Upper

83 100

55 0.0 60.7 91.1#

98 1.1 38.7 58.1#

