


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060724\
Data File : VV036001.D
Acq On : 07 Jun 2024 10:23
Operator : SY/MD
Sample : BFB317
Misc : 5.00g/10.0mL/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB317

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Title : VOC Analysis
Last Update : Tue Jun 11 05:03:54 2024

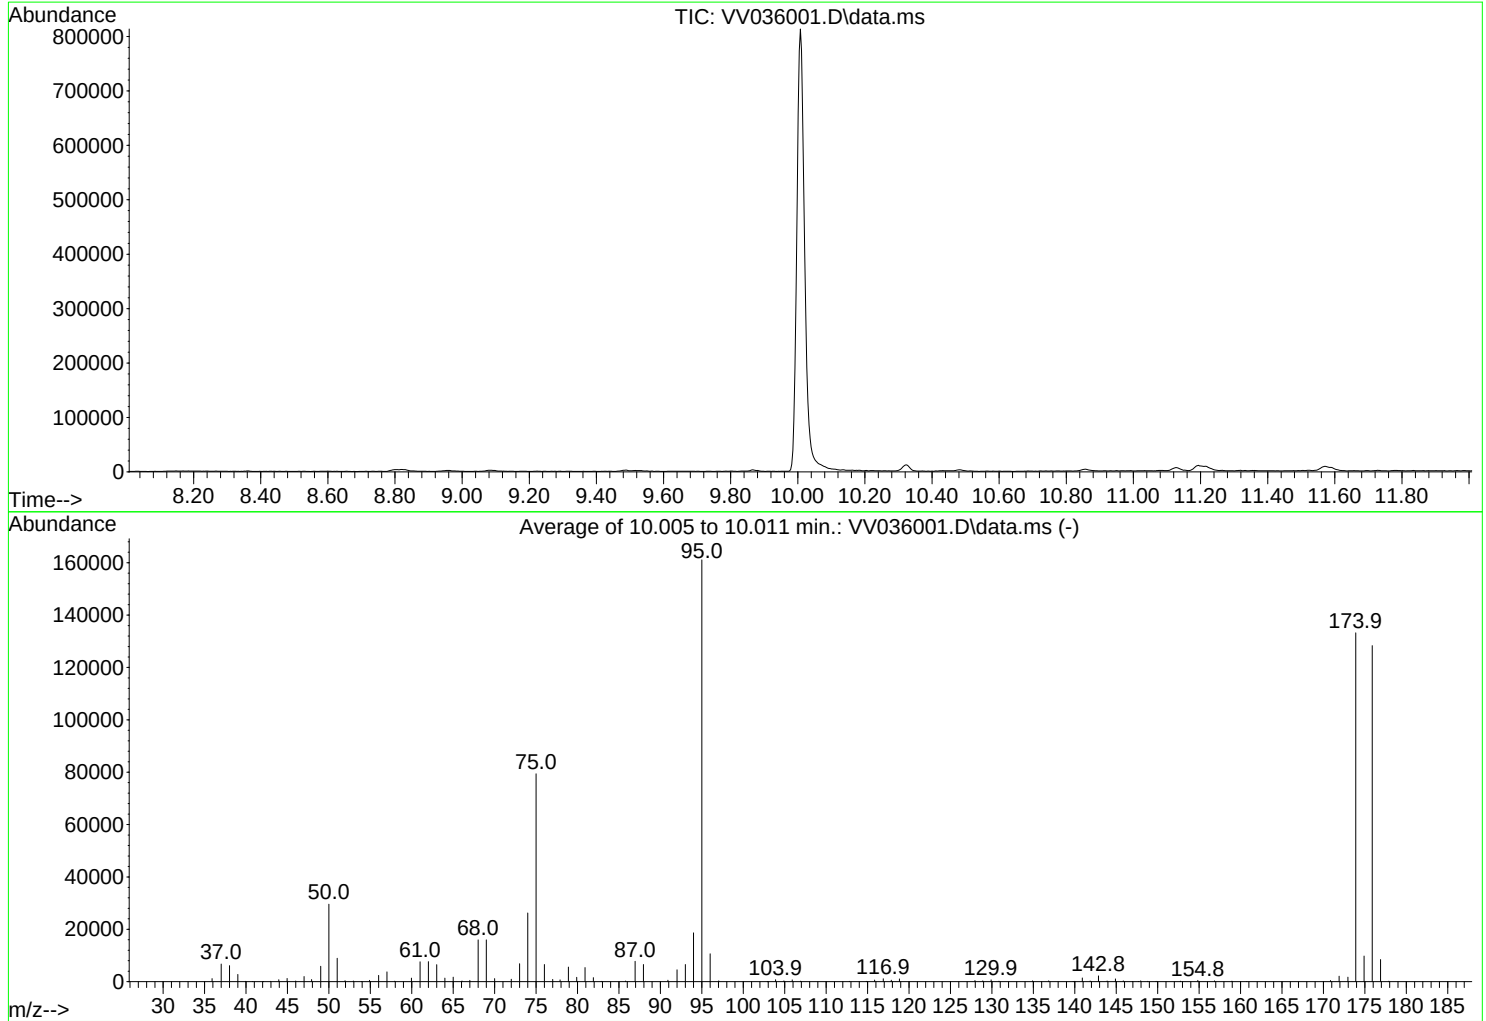

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	29571	PASS
75	95	30	80	49.3	79416	PASS
95	95	100	100	100.0	161109	PASS
96	95	5	9	6.6	10653	PASS
173	174	0.00	2	1.3	1693	PASS
174	95	50	120	82.7	133237	PASS
175	174	5	9	7.4	9801	PASS
176	174	95	101	96.3	128347	PASS
177	176	5	9	6.6	8461	PASS

Scan 2777 (9.969 min): VV036001.D\data.ms
BFB317

m/z	Abundance
39.90	297.0
43.90	637.0
77.00	152.0

Instrument :
MSVOA_V
ClientSampleId :
BFB317

m/z	Abundance
35.90	1119.0
37.00	6653.0
38.00	6221.0
39.00	2785.0
40.00	421.0
40.80	135.0
43.00	110.0
44.00	1334.0
45.00	1270.0
46.00	309.0
47.00	1964.0
47.90	811.0
49.00	5924.0
50.00	29432.0
51.00	9160.0
52.00	361.0
52.90	263.0
53.90	113.0
54.90	452.0
56.00	2265.0
57.00	3717.0
58.00	170.0
59.90	1395.0
61.00	7556.0
62.00	7562.0
63.00	6475.0
64.00	1370.0
65.00	1663.0
66.00	272.0
67.00	480.0
68.00	15874.0
69.00	15694.0
70.00	1223.0
72.00	958.0
73.00	6942.0
74.00	26312.0
75.00	79248.0
76.00	6640.0
77.00	1012.0
77.90	628.0
78.90	5572.0
79.90	1705.0
80.90	5293.0
81.90	1406.0
82.80	120.0
85.80	237.0
86.90	7697.0
87.90	6529.0
90.90	516.0
92.00	4314.0
93.00	6442.0
94.00	18464.0
95.00	158016.0
96.00	10910.0
97.00	284.0
102.90	108.0
103.90	660.0
104.90	314.0
105.90	673.0
106.90	253.0
112.80	162.0
114.80	132.0
115.80	615.0
116.90	1092.0
117.90	582.0
118.80	1027.0
127.90	436.0
128.90	305.0
129.90	676.0
130.90	220.0
134.90	283.0
136.80	351.0
139.80	132.0
140.90	1402.0
141.90	218.0
142.90	2137.0
143.90	237.0
144.90	1076.0
145.80	271.0
147.70	249.0
148.00	259.0
148.80	125.0
149.80	149.0
152.70	196.0
154.90	492.0
156.80	284.0
158.90	188.0
170.80	473.0
171.90	1882.0
172.90	1672.0
173.90	128544.0
174.90	9615.0

Instrument :
MSVOA_V
ClientSampleId :
BFB317

175.90	123504.0
176.90	8520.0
177.90	200.0

Instrument :
MSVOA_V
ClientSampleId :
BFB317

m/z	Abundance
35.90	1211.0
37.00	7001.0
38.00	6330.0
39.00	2845.0
40.00	406.0
42.10	102.0
42.90	115.0
44.00	1358.0
44.90	1244.0
46.00	254.0
47.00	2048.0
47.90	812.0
49.00	6003.0
50.00	30640.0
51.00	9134.0
52.00	405.0
52.90	253.0
54.00	108.0
54.90	507.0
56.00	2492.0
57.00	3804.0
58.00	169.0
60.00	1393.0
61.00	7771.0
62.00	7972.0
63.00	6692.0
64.00	1406.0
65.00	1725.0
66.10	236.0
67.00	512.0
68.00	16488.0
69.00	16456.0
70.00	1232.0
72.00	925.0
73.00	7006.0
74.00	27048.0
75.00	82088.0
76.00	6720.0
77.00	1048.0
77.90	722.0
78.90	5748.0
79.90	1665.0
80.90	5465.0
81.90	1627.0
82.90	141.0
85.80	240.0
86.90	8123.0
88.00	6721.0
90.90	569.0
92.00	4720.0
93.00	6701.0
94.00	19336.0
95.00	166848.0
96.00	10999.0
97.10	342.0
103.90	781.0
104.90	309.0
105.90	680.0
106.90	214.0
112.80	157.0
114.90	155.0
115.90	664.0
116.90	1151.0
117.80	557.0
118.90	1039.0
128.00	461.0
128.90	290.0
129.90	713.0
130.90	208.0
134.90	322.0
136.90	338.0
140.00	150.0
140.90	1462.0
141.80	251.0
142.80	2252.0
143.90	250.0
144.90	1060.0
145.90	317.0
147.00	133.0
147.90	294.0
148.80	129.0
149.80	170.0
152.70	175.0
154.90	494.0
156.90	292.0
159.00	218.0
160.70	103.0
170.90	434.0
171.90	2145.0
172.90	1735.0
173.90	137664.0
174.90	10101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB317

175.90	132864.0
176.90	8846.0
177.90	207.0

Instrument :
MSVOA_V
ClientSampleId :
BFB317

m/z	Abundance
35.90	1120.0
37.00	6441.0
38.00	5825.0
39.00	2637.0
40.00	369.0
42.10	114.0
42.90	122.0
44.00	1393.0
44.90	1150.0
46.00	178.0
47.00	1929.0
47.90	744.0
49.00	5684.0
50.00	28640.0
51.00	8548.0
51.90	421.0
53.00	221.0
54.90	484.0
56.00	2456.0
57.00	3761.0
57.90	157.0
60.00	1308.0
61.00	7334.0
62.00	7457.0
63.00	6317.0
64.00	1258.0
65.00	1725.0
66.00	202.0
67.00	437.0
68.00	15501.0
69.00	15657.0
70.00	1126.0
72.00	821.0
73.00	6599.0
74.00	25288.0
75.00	76912.0
76.00	6336.0
77.00	1044.0
77.90	727.0
78.90	5356.0
79.90	1503.0
80.90	5317.0
81.90	1639.0
82.90	144.0
85.80	300.0
87.00	7432.0
88.00	6301.0
90.90	589.0
92.00	4546.0
93.00	6429.0
94.00	18088.0
95.00	158464.0
96.00	10051.0
97.10	370.0
103.90	742.0
104.90	247.0
105.90	632.0
106.90	146.0
112.80	121.0
114.90	179.0
115.90	648.0
116.90	1134.0
117.80	493.0
118.90	1024.0
127.90	478.0
128.90	258.0
129.90	700.0
130.80	171.0
134.90	288.0
136.90	303.0
140.00	159.0
140.90	1372.0
141.80	210.0
142.90	2162.0
143.90	203.0
144.90	950.0
145.90	332.0
146.90	144.0
147.90	334.0
148.80	138.0
149.80	139.0
152.80	125.0
154.80	429.0
156.90	264.0
159.00	217.0
160.80	120.0
170.90	350.0
171.90	2174.0
173.00	1671.0
173.90	133504.0
174.90	9688.0
175.90	128672.0

Instrument :
MSVOA_V
ClientSampleId :
BFB317

176.908018.0

177.90188.0

Instrument :
MSVOA_V
ClientSampleId :
BFB317