




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061124\
Data File : VV036032.D
Acq On : 11 Jun 2024 13:51
Operator : SY/MD
Sample : P2798-02
Misc : 5.35g/10.1mL/MSVOA_V/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB13

Manual IntegrationsAPPROVED

Quant Time: Jun 12 02:07:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 12 02:05:45 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/12/2024
Supervised By :Semsettin Yesilyurt 06/12/2024

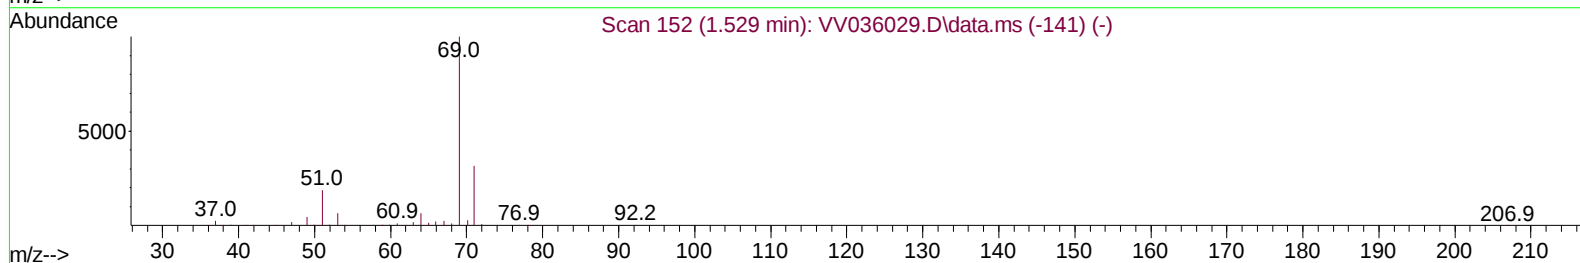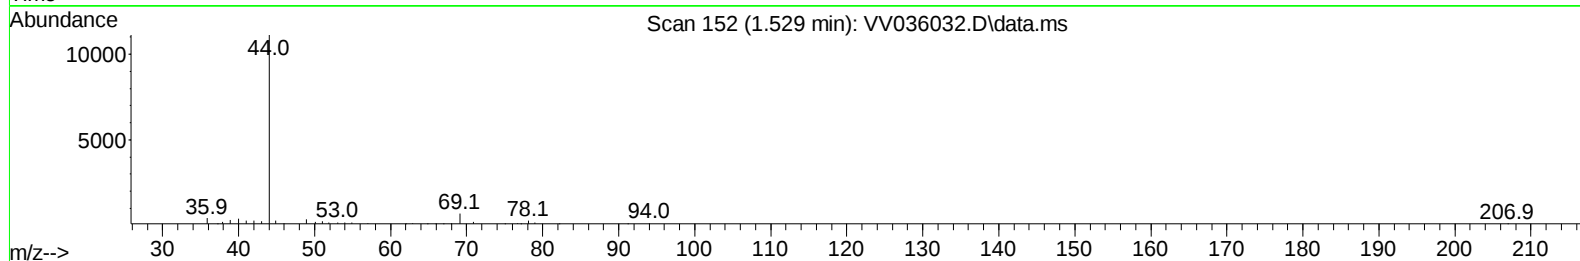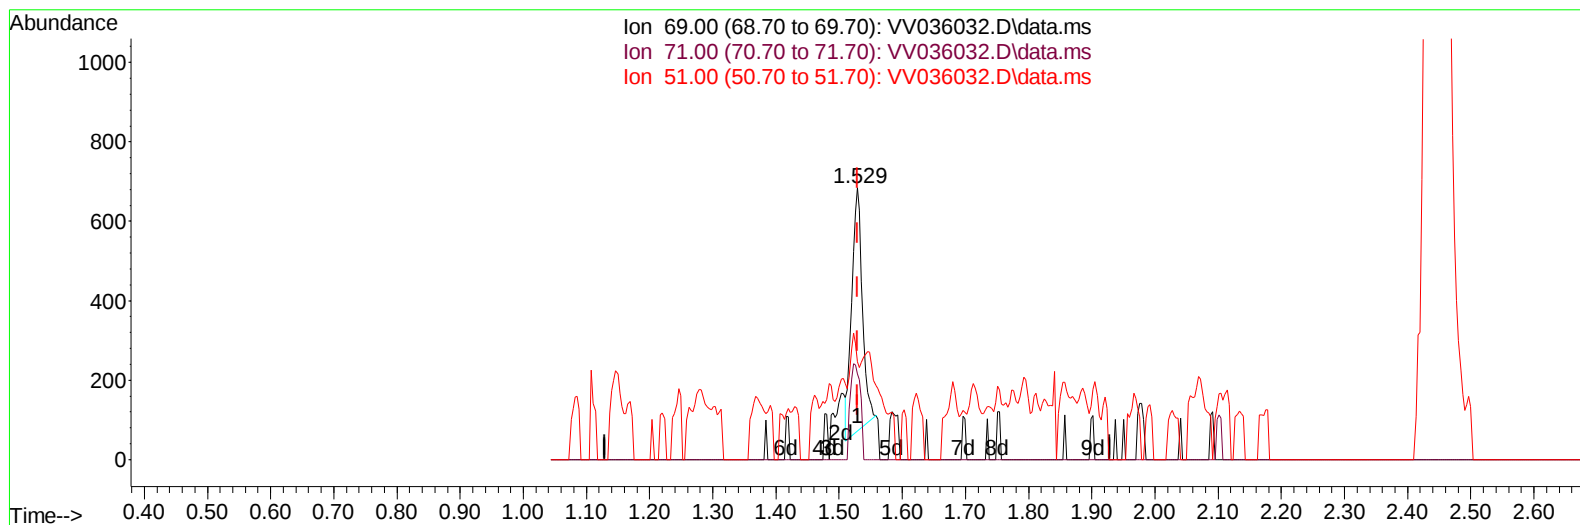

TIC: VV036032.D\data.ms

(7) Chloroethane-d5 (S)

1.529min (+ 0.000) 0.10 ug/L

response 724

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.90	36.74
51.00	26.70	13.67#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061124\
Data File : VV036032.D
Acq On : 11 Jun 2024 13:51
Operator : SY/MD
Sample : P2798-02
Misc : 5.35g/10.1mL/MSVOA_V/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB13

Manual IntegrationsAPPROVED

Quant Time: Jun 12 02:07:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 12 02:05:45 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/12/2024
Supervised By :Semsettin Yesilyurt 06/12/2024

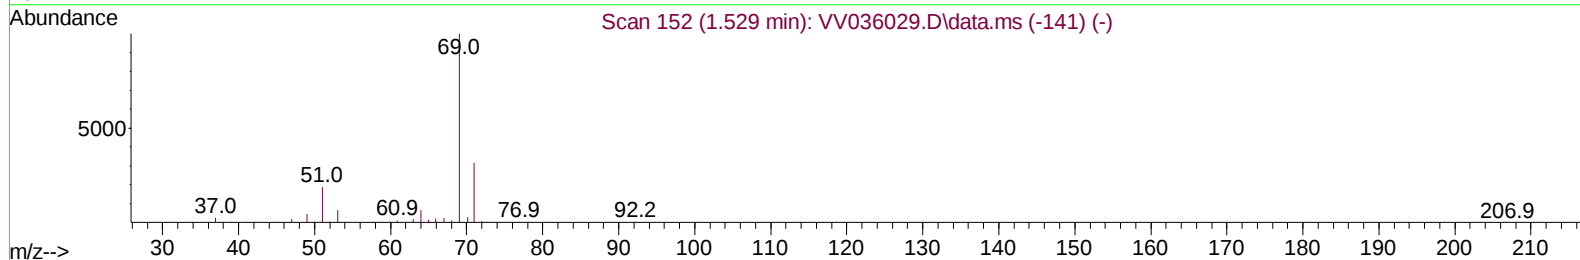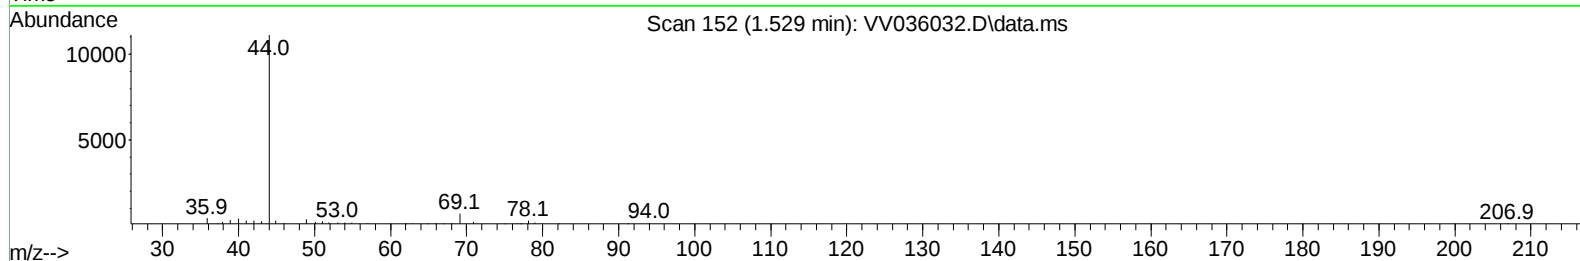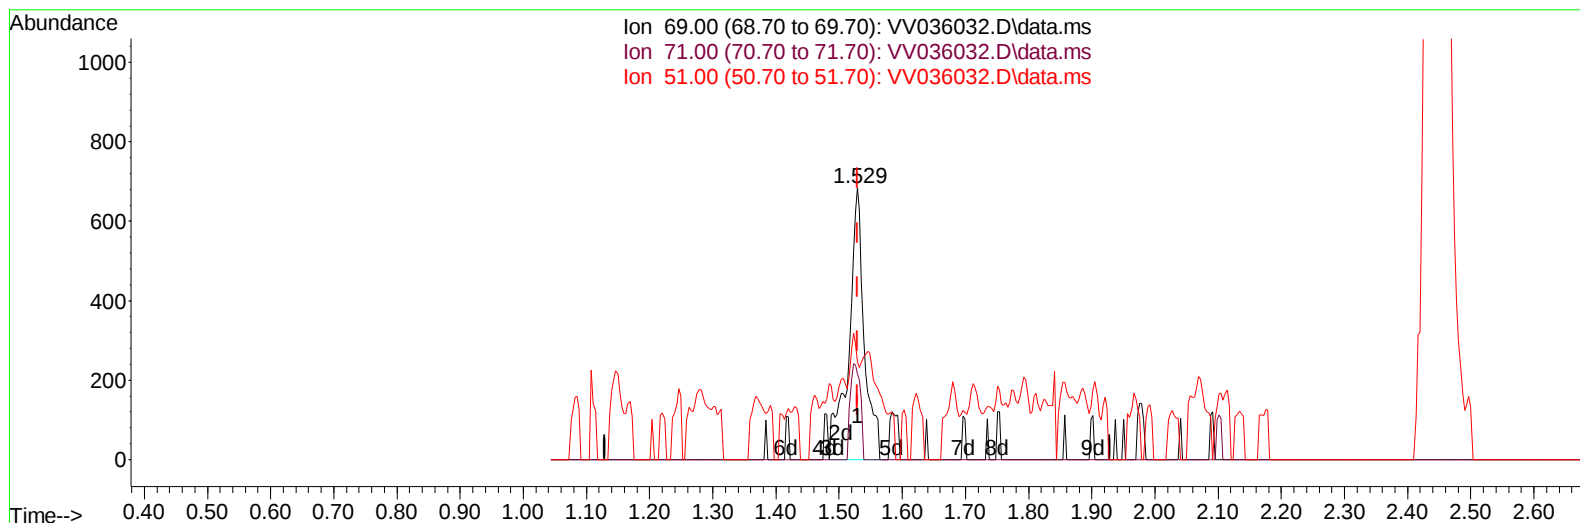

TIC: VV036032.D\data.ms

(7) Chloroethane-d5 (S)

1.529min (+ 0.000) 0.16 ug/L m

response 1181

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.90	22.52
51.00	26.70	8.38#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061124\
Data File : VV036032.D
Acq On : 11 Jun 2024 13:51
Operator : SY/MD
Sample : P2798-02
Misc : 5.35g/10.1mL/MSVOA_V/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB13

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 06/12/2024
Supervised By :Semsettin Yesilyurt 06/12/2024

Quant Time: Jun 12 02:07:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 12 02:05:45 2024
Response via : Initial Calibration

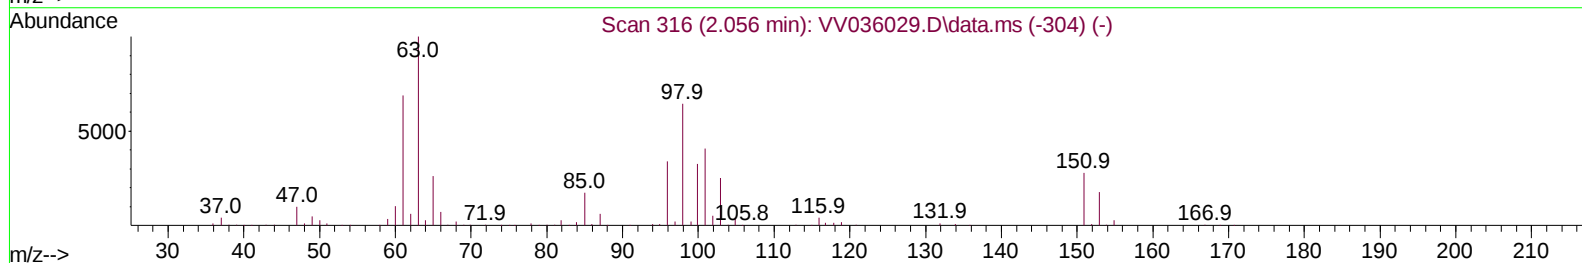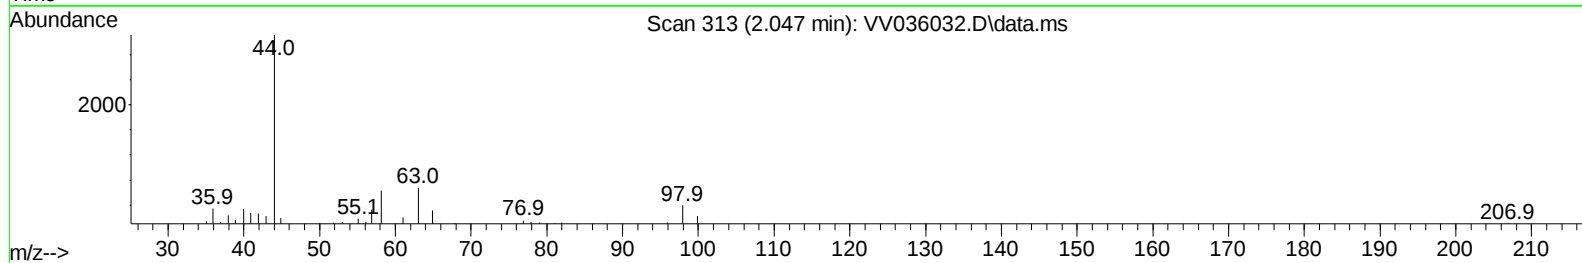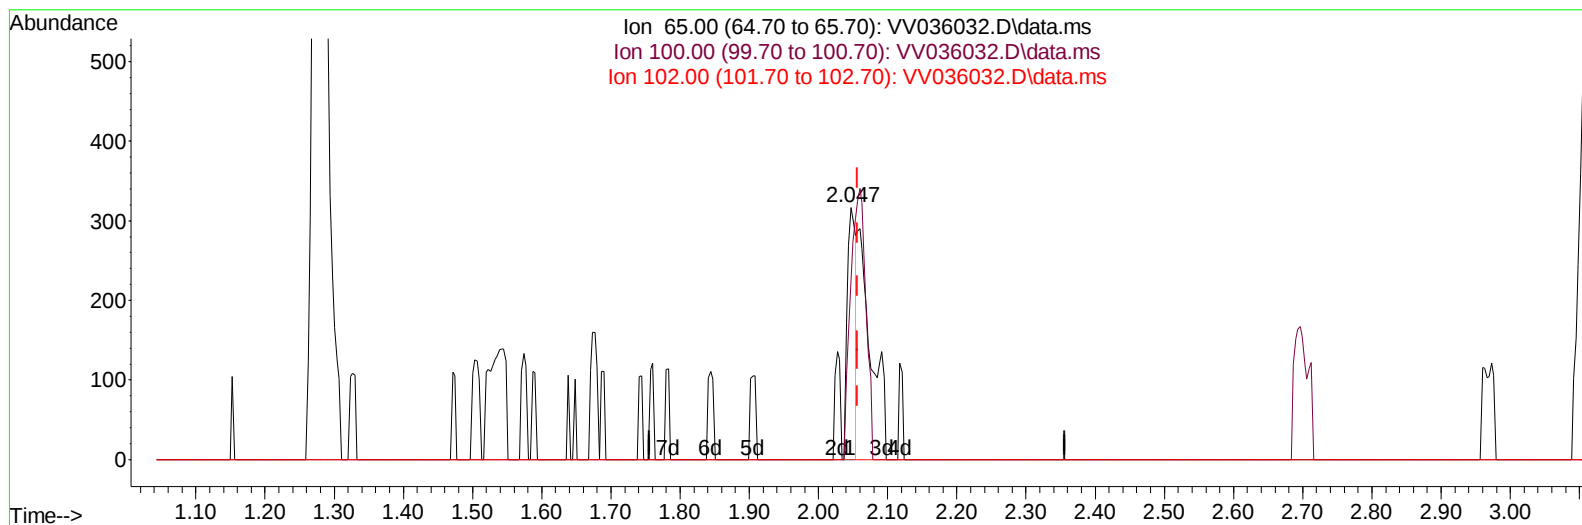

TIC: VV036032.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.047min (-0.010) 0.06 ug/L

response 259

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	132.50	203.47#
102.00	20.40	0.00#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061124\
Data File : VV036032.D
Acq On : 11 Jun 2024 13:51
Operator : SY/MD
Sample : P2798-02
Misc : 5.35g/10.1mL/MSVOA_V/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB13

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 06/12/2024
Supervised By :Semsettin Yesilyurt 06/12/2024

Quant Time: Jun 12 02:07:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 12 02:05:45 2024
Response via : Initial Calibration

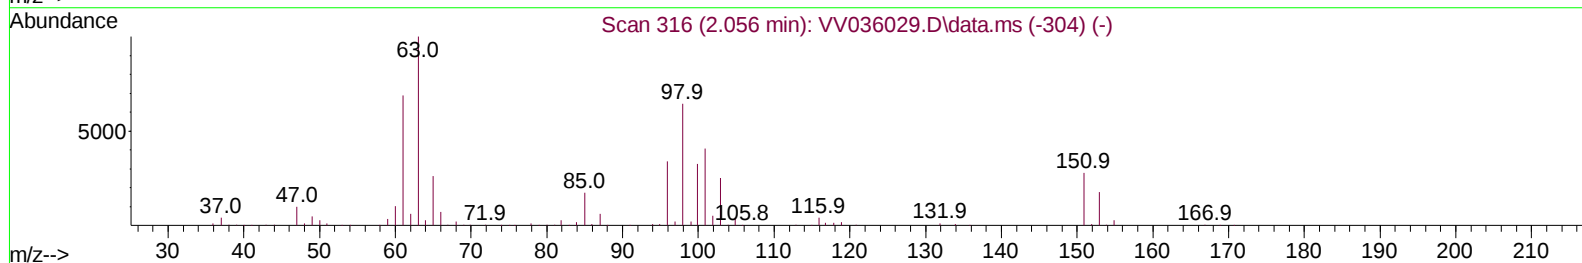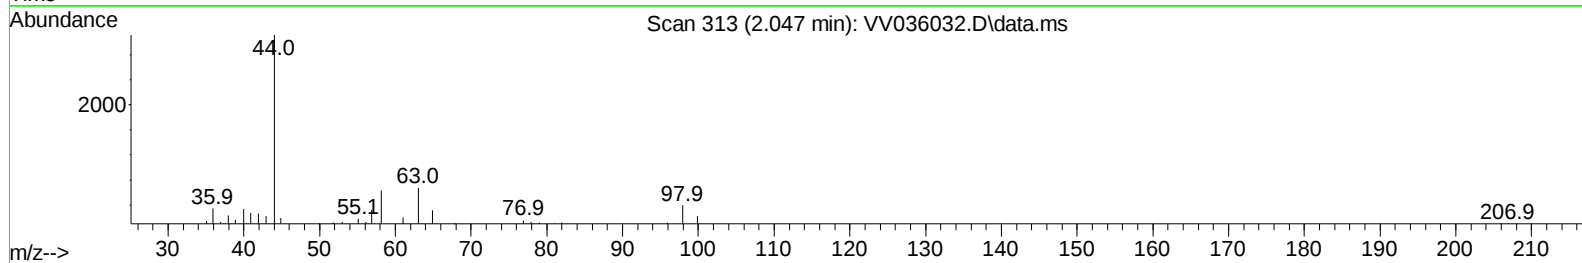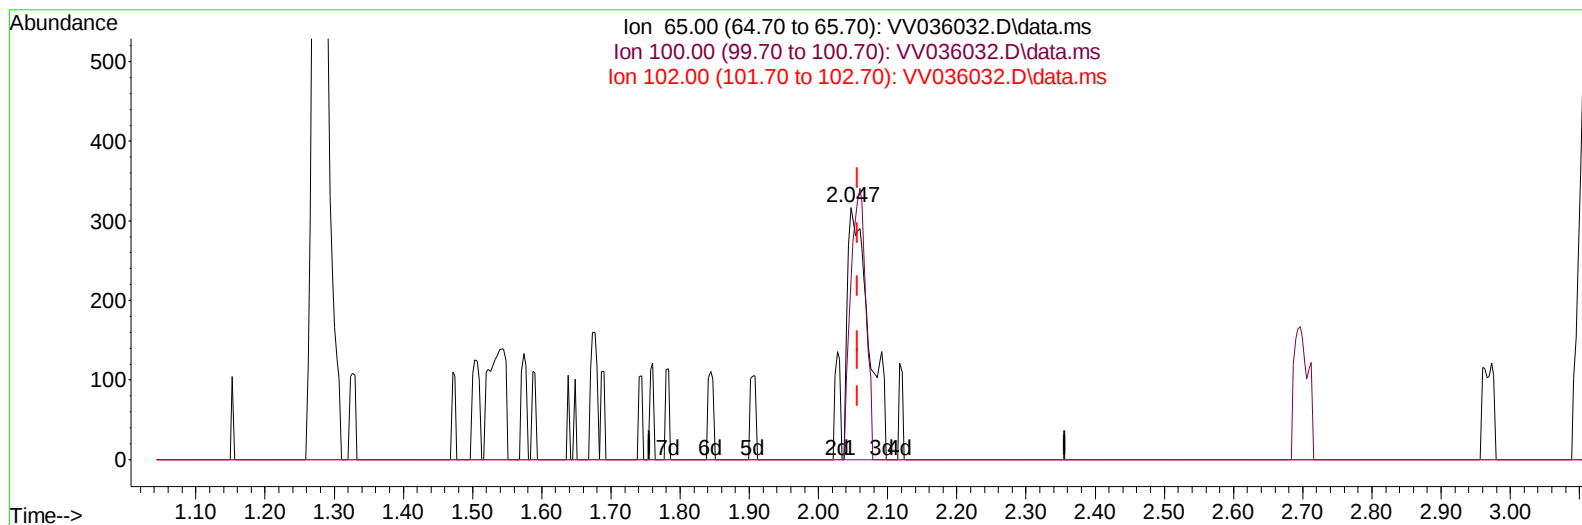

TIC: VV036032.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.047min (-0.010) 0.17 ug/L m

response 683

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	132.50	77.16#
102.00	20.40	0.00#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061124\
Data File : VV036032.D
Acq On : 11 Jun 2024 13:51
Operator : SY/MD
Sample : P2798-02
Misc : 5.35g/10.1mL/MSVOA_V/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB13

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 06/12/2024
Supervised By :Semsettin Yesilyurt 06/12/2024

Quant Time: Jun 12 02:07:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 12 02:05:45 2024
Response via : Initial Calibration

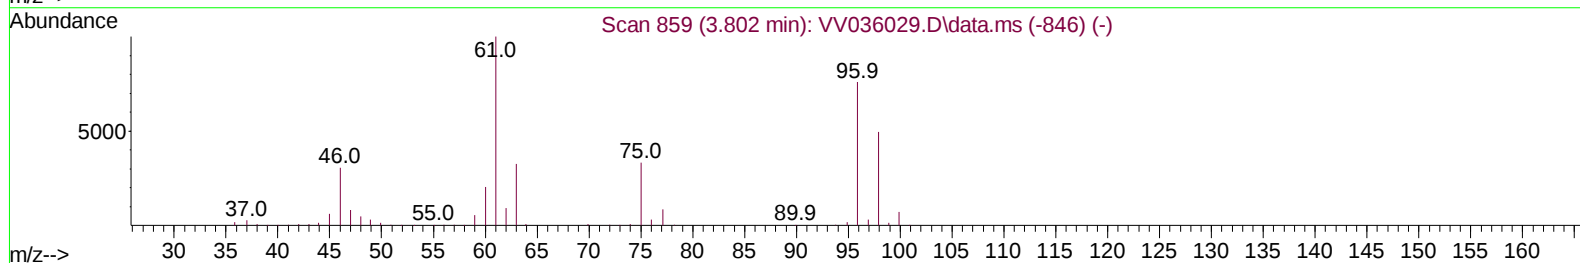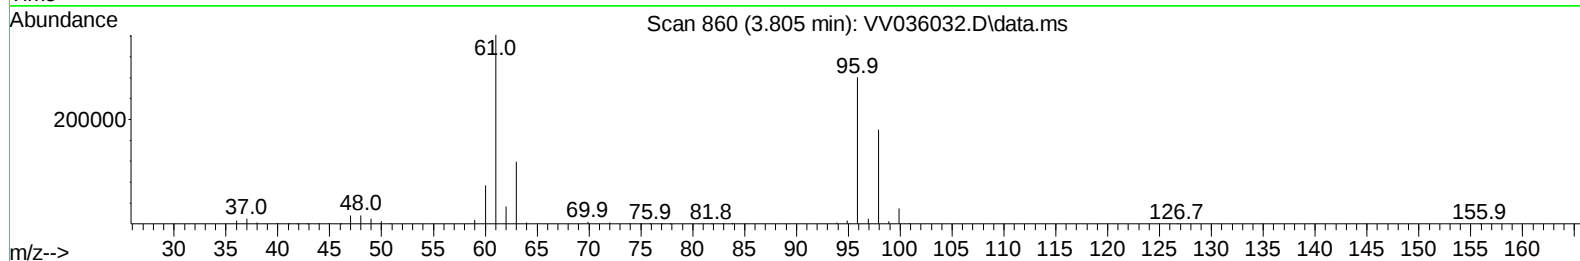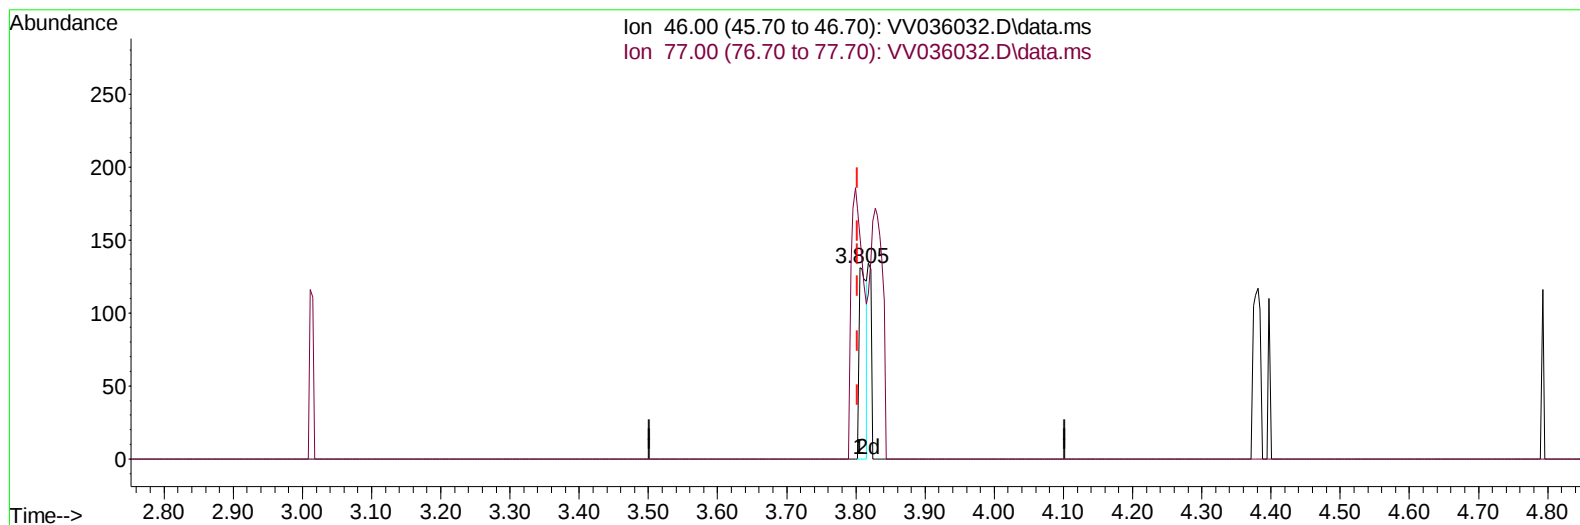

TIC: VV036032.D\data.ms

(21) 2-Butanone-d5 (S)

3.805min (+ 0.003) 0.05 ug/L

response 98

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	11.90	231.63#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061124\
Data File : VV036032.D
Acq On : 11 Jun 2024 13:51
Operator : SY/MD
Sample : P2798-02
Misc : 5.35g/10.1mL/MSVOA_V/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB13

Manual IntegrationsAPPROVED

Quant Time: Jun 12 02:07:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 12 02:05:45 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/12/2024
Supervised By :Semsettin Yesilyurt 06/12/2024

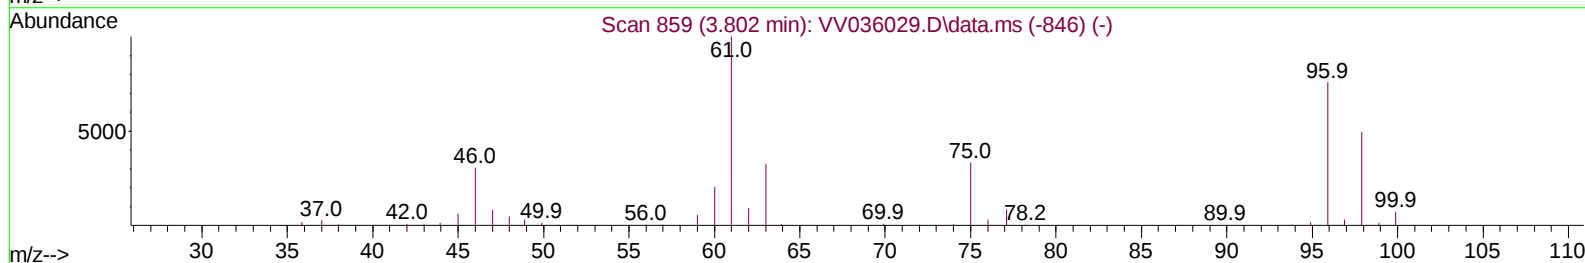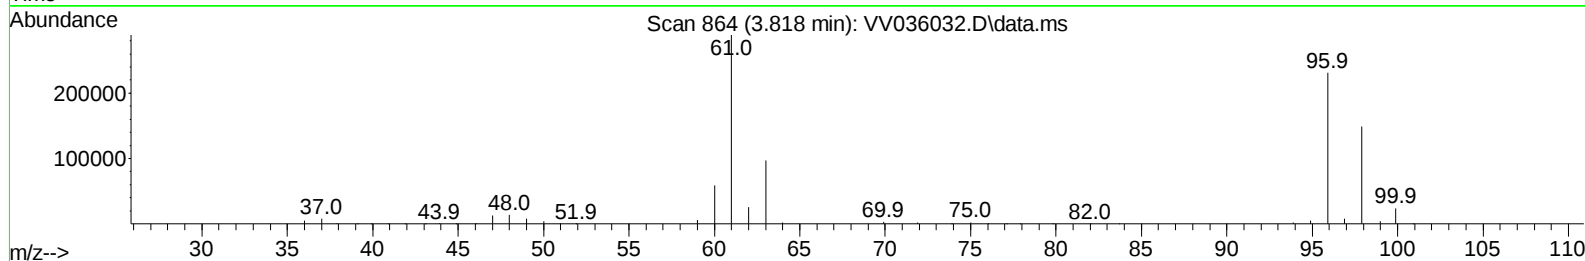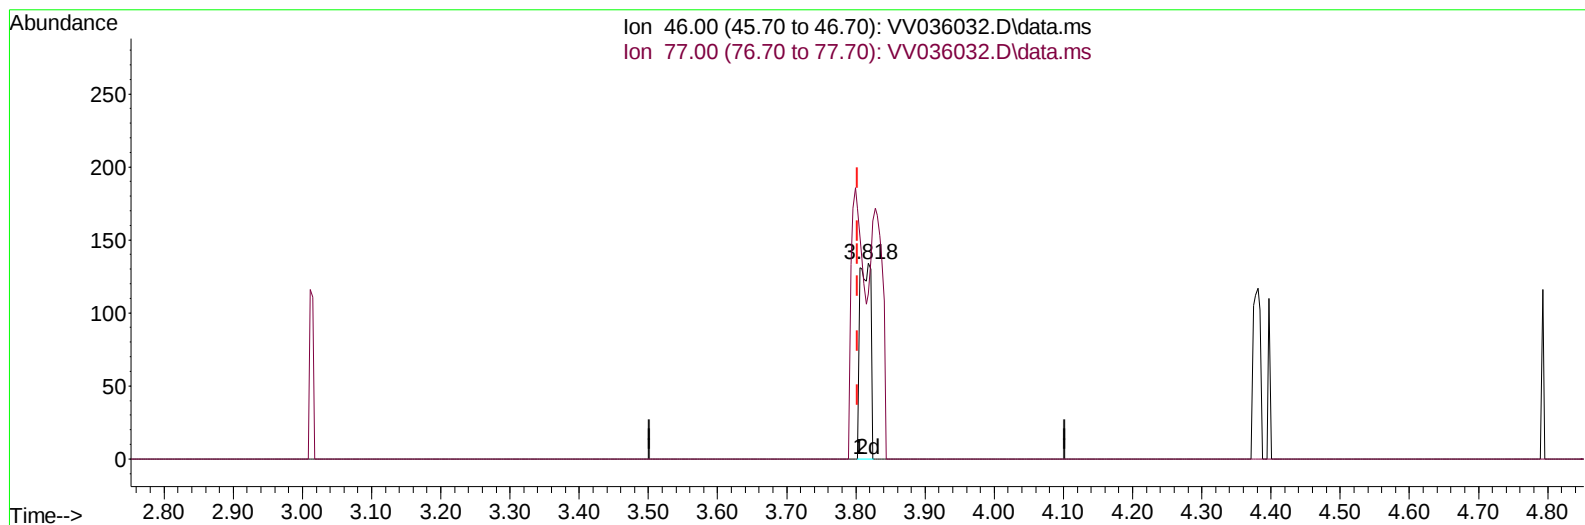

TIC: VV036032.D\data.ms

(21) 2-Butanone-d5 (S)

3.818min (+ 0.016) 0.07 ug/L m

response 149

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	11.90	152.35#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061124\
Data File : VV036032.D
Acq On : 11 Jun 2024 13:51
Operator : SY/MD
Sample : P2798-02
Misc : 5.35g/10.1mL/MSVOA_V/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB13

Manual IntegrationsAPPROVED

Quant Time: Jun 12 02:07:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 12 02:05:45 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/12/2024
Supervised By :Semsettin Yesilyurt 06/12/2024

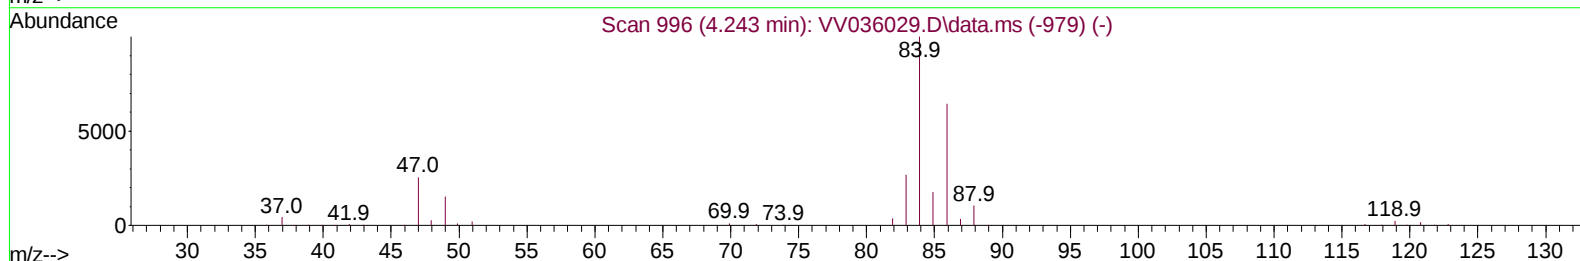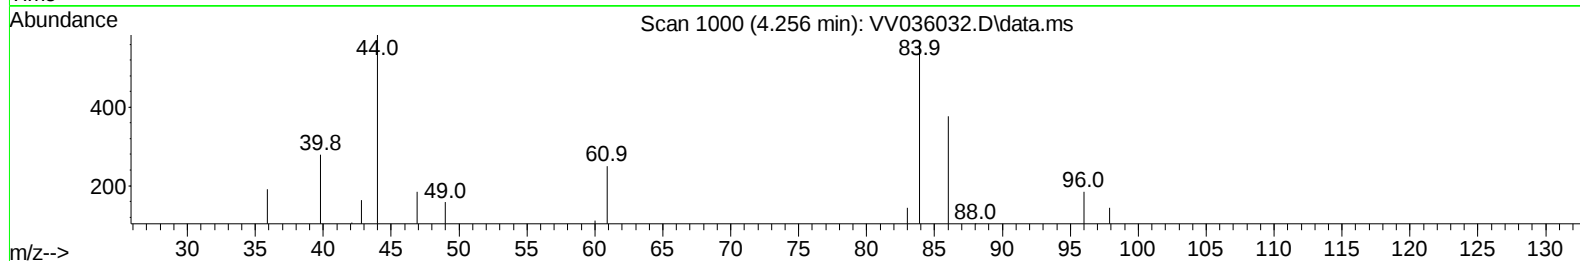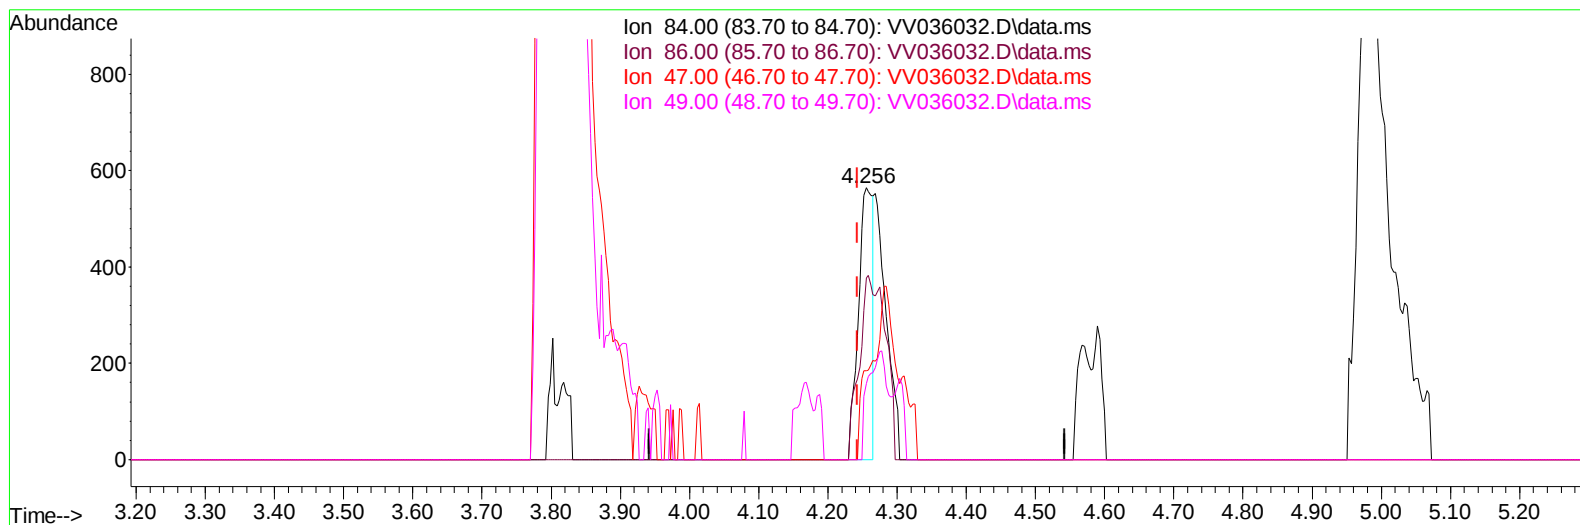

TIC: VV036032.D\data.ms

(24) Chloroform-d (S)

4.256min (+ 0.013) 0.05 ug/L

response 829

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.70	72.26
47.00	44.00	15.44#
49.00	25.60	11.10#




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061124\
Data File : VV036032.D
Acq On : 11 Jun 2024 13:51
Operator : SY/MD
Sample : P2798-02
Misc : 5.35g/10.1mL/MSVOA_V/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB13

Manual IntegrationsAPPROVED

Quant Time: Jun 12 02:07:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 12 02:05:45 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/12/2024
Supervised By :Semsettin Yesilyurt 06/12/2024

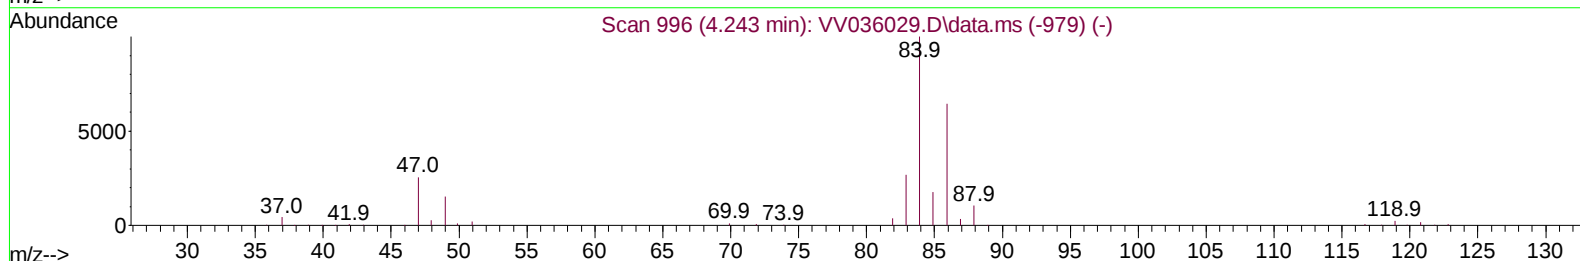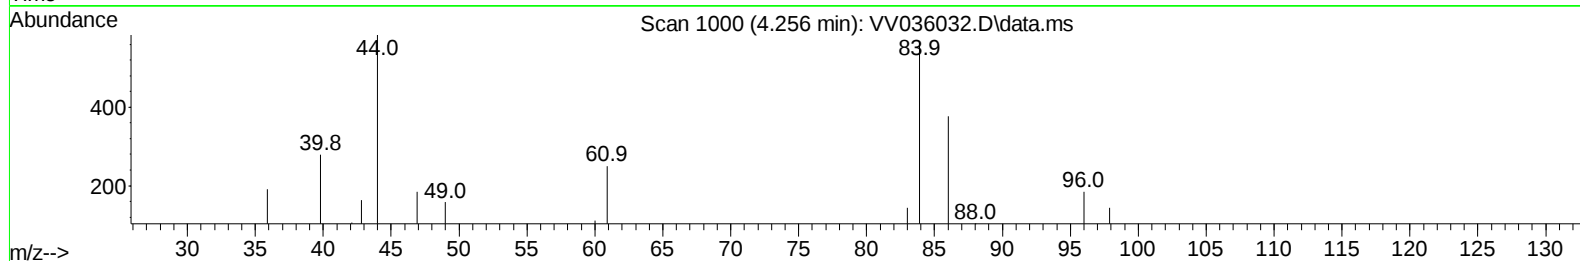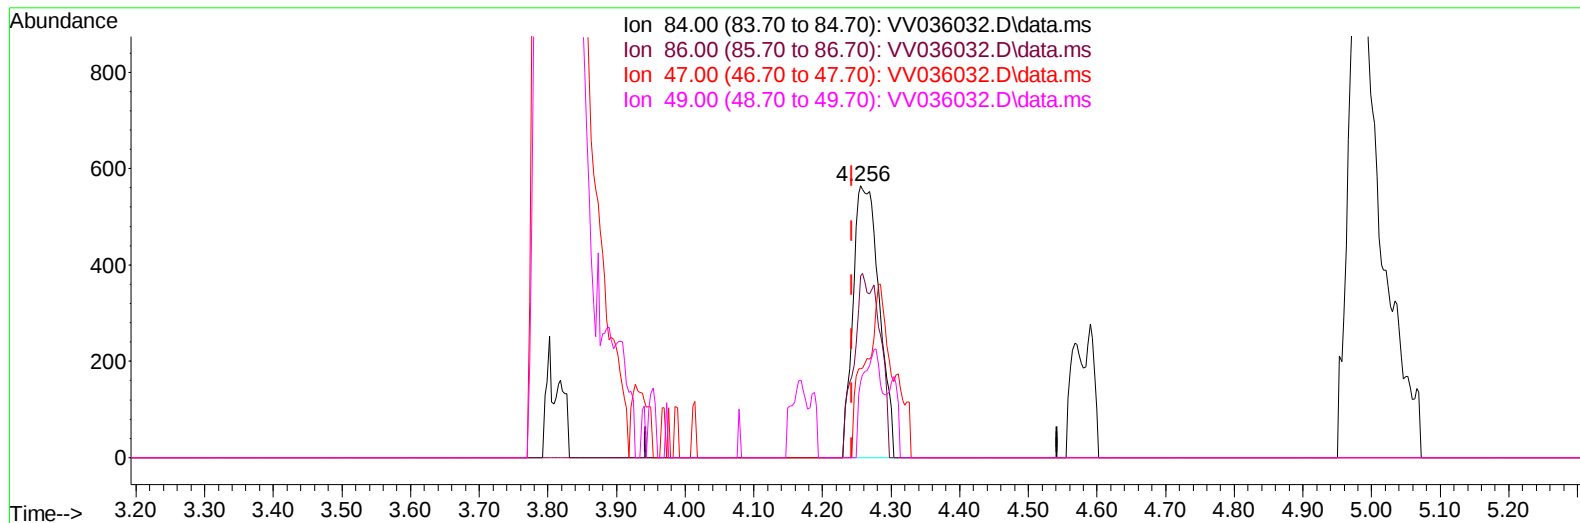

TIC: VV036032.D\data.ms

(24) Chloroform-d (S)

4.256min (+ 0.013) 0.10 ug/L m

response 1492

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.70	40.15#
47.00	44.00	8.58#
49.00	25.60	6.17#




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061124\
Data File : VV036032.D
Acq On : 11 Jun 2024 13:51
Operator : SY/MD
Sample : P2798-02
Misc : 5.35g/10.1mL/MSVOA_V/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB13

Manual IntegrationsAPPROVED

Quant Time: Jun 12 02:07:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 12 02:05:45 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/12/2024
Supervised By :Semsettin Yesilyurt 06/12/2024

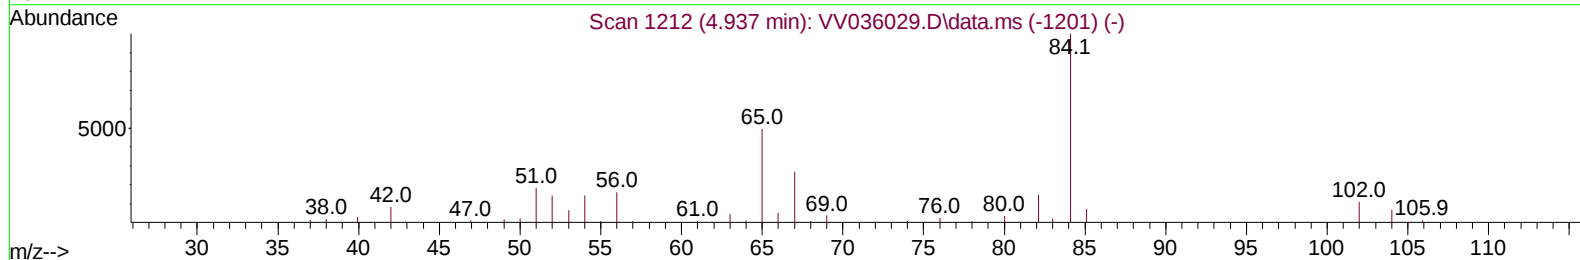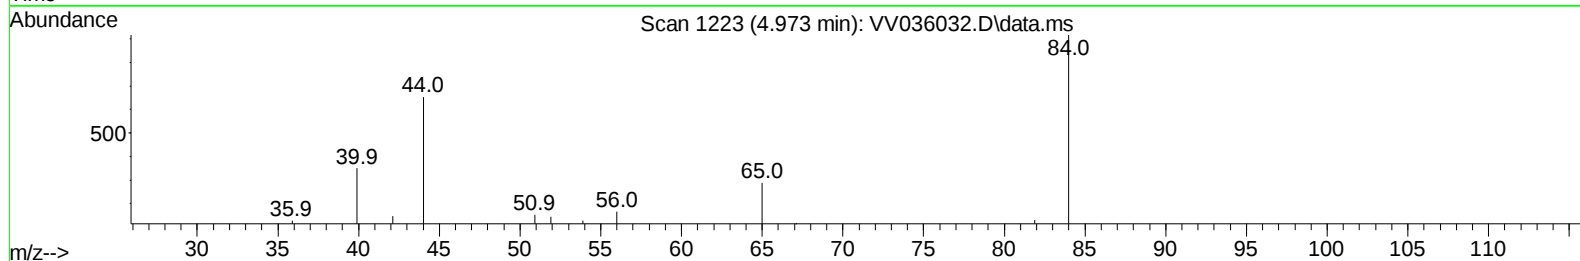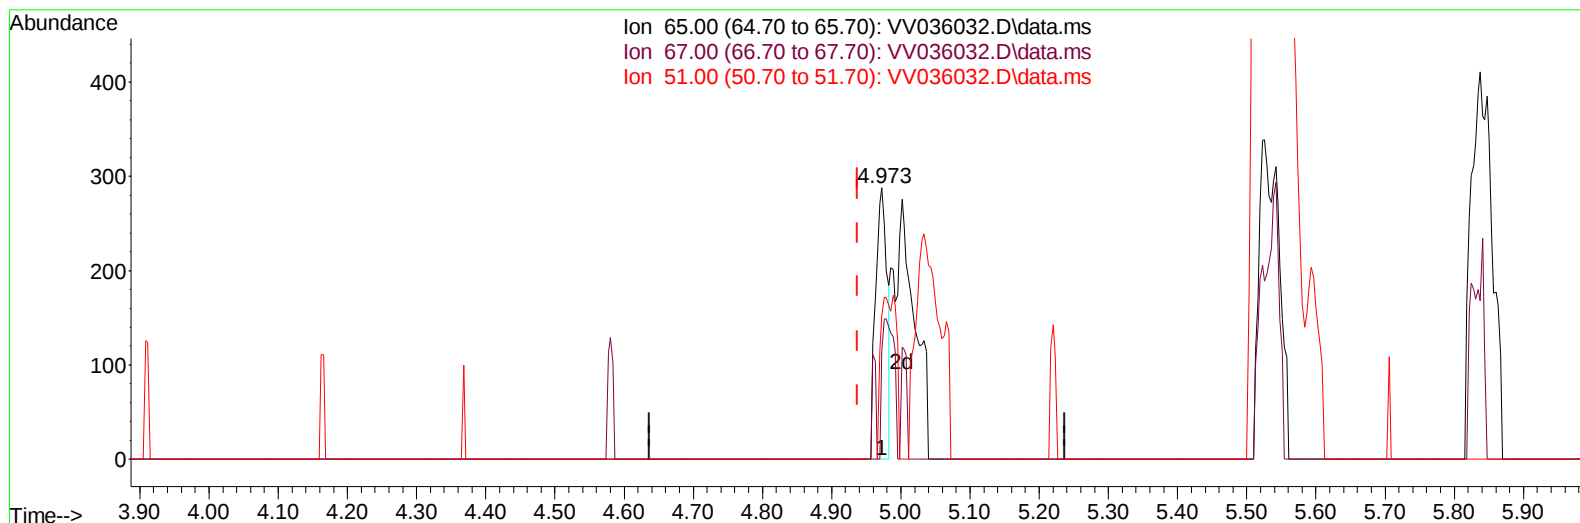

TIC: VV036032.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

4.973min (+ 0.035) 0.04 ug/L

response 327

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	54.30	54.74
51.00	34.20	54.74#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061124\
Data File : VV036032.D
Acq On : 11 Jun 2024 13:51
Operator : SY/MD
Sample : P2798-02
Misc : 5.35g/10.1mL/MSVOA_V/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB13

Manual IntegrationsAPPROVED

Quant Time: Jun 12 02:07:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 12 02:05:45 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/12/2024
Supervised By :Semsettin Yesilyurt 06/12/2024

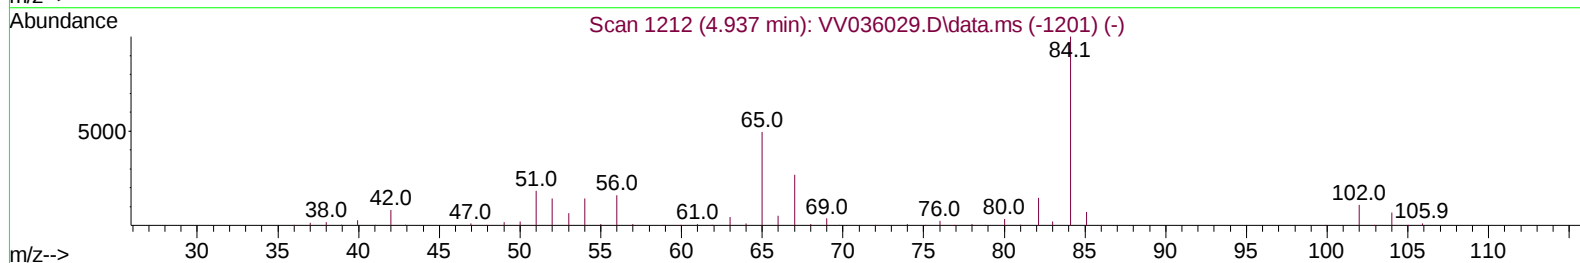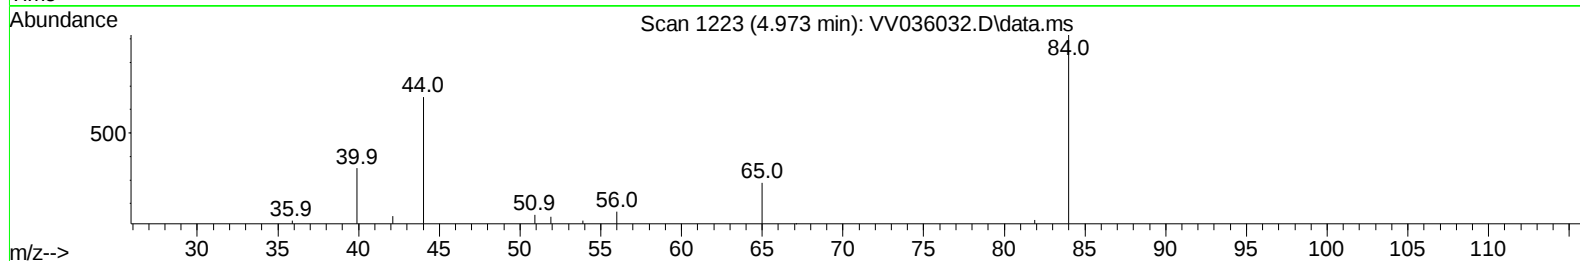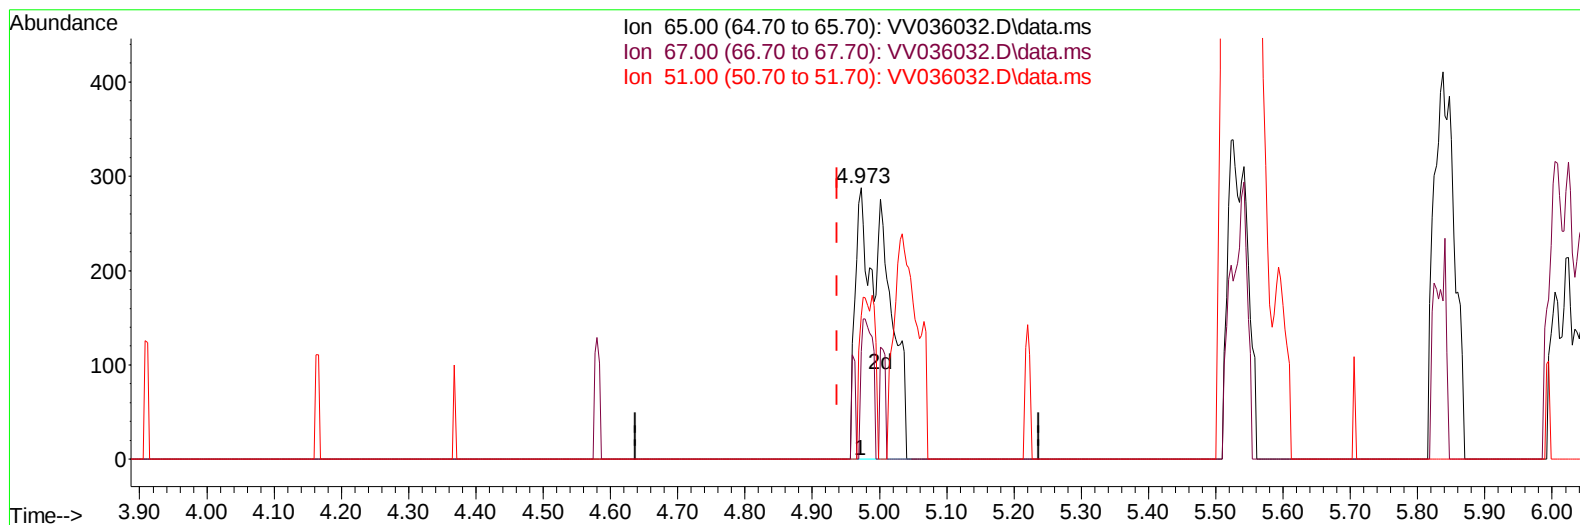

TIC: VV036032.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

4.973min (+ 0.035) 0.11 ug/L m

response 903

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	54.30	19.82#
51.00	34.20	19.82#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061124\
Data File : VV036032.D
Acq On : 11 Jun 2024 13:51
Operator : SY/MD
Sample : P2798-02
Misc : 5.35g/10.1mL/MSVOA_V/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB13

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 06/12/2024
Supervised By :Semsettin Yesilyurt 06/12/2024

Quant Time: Jun 12 02:07:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 12 02:05:45 2024
Response via : Initial Calibration

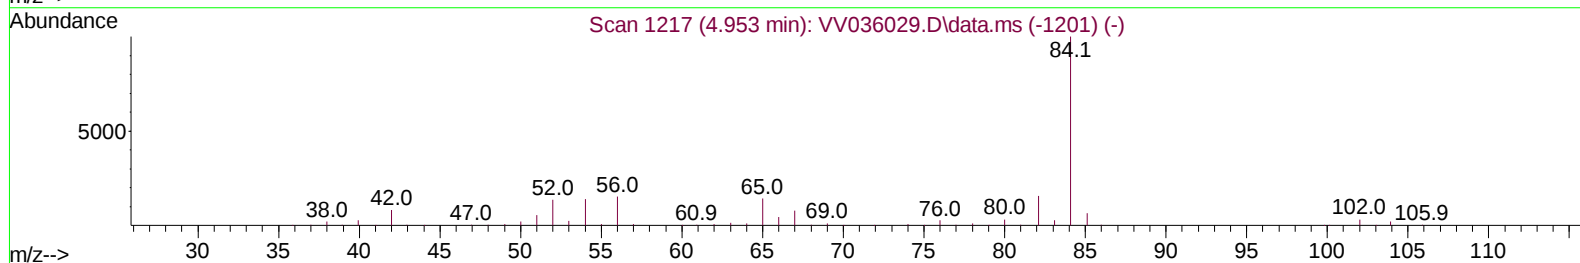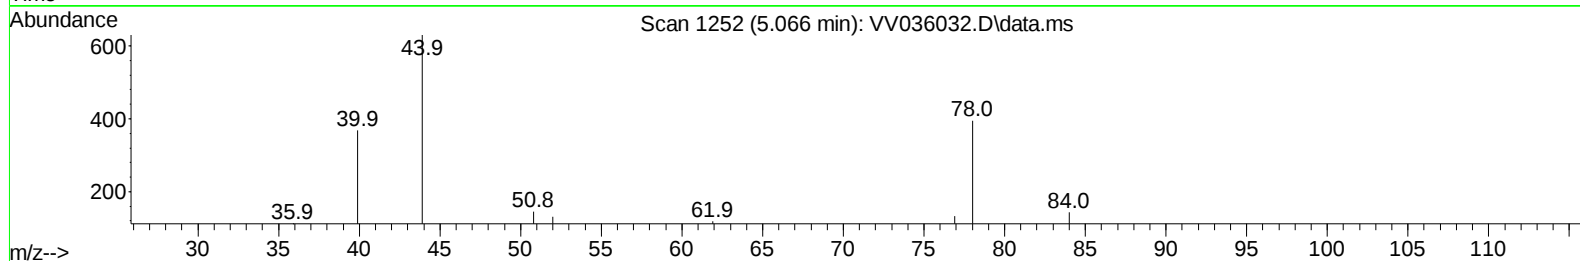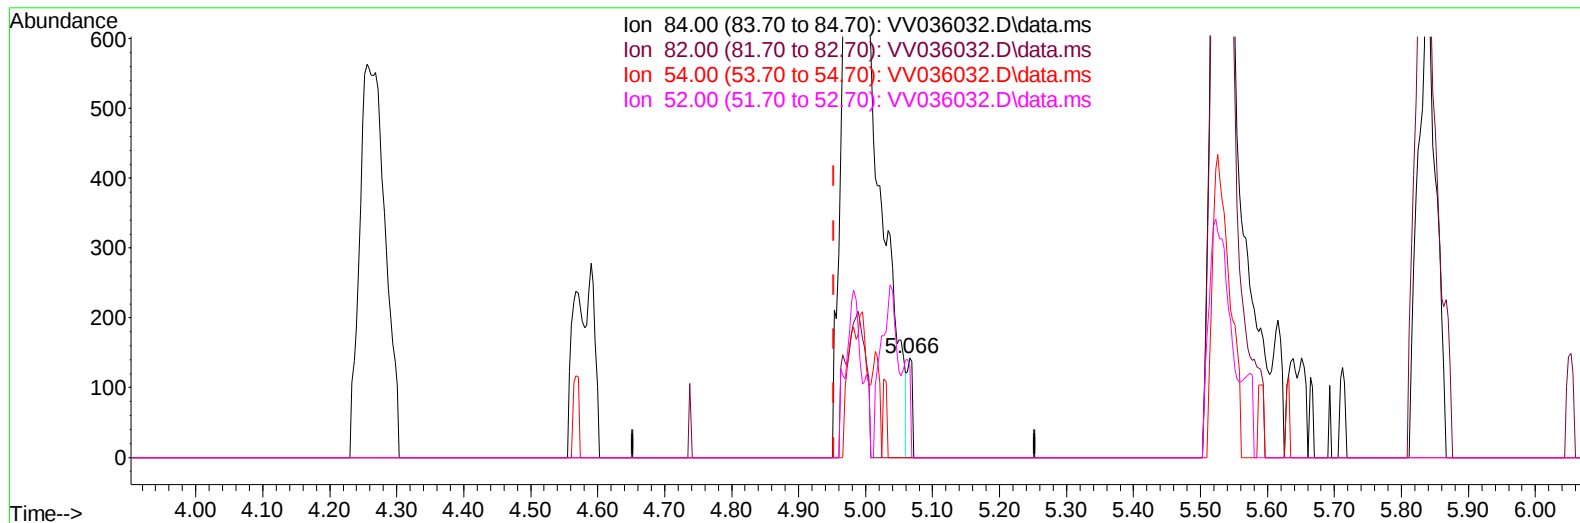

TIC: VV036032.D\data.ms

(32) Benzene-d6 (S)

5.066min (+ 0.113) 0.00 ug/L

response 78

Ion	Exp%	Act%
84.00	100.00	100.00
82.00	15.60	0.00#
54.00	14.30	0.00#
52.00	12.70	133.33#




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061124\
Data File : VV036032.D
Acq On : 11 Jun 2024 13:51
Operator : SY/MD
Sample : P2798-02
Misc : 5.35g/10.1mL/MSVOA_V/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB13

Manual IntegrationsAPPROVED

Quant Time: Jun 12 02:07:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 12 02:05:45 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/12/2024
Supervised By :Semsettin Yesilyurt 06/12/2024

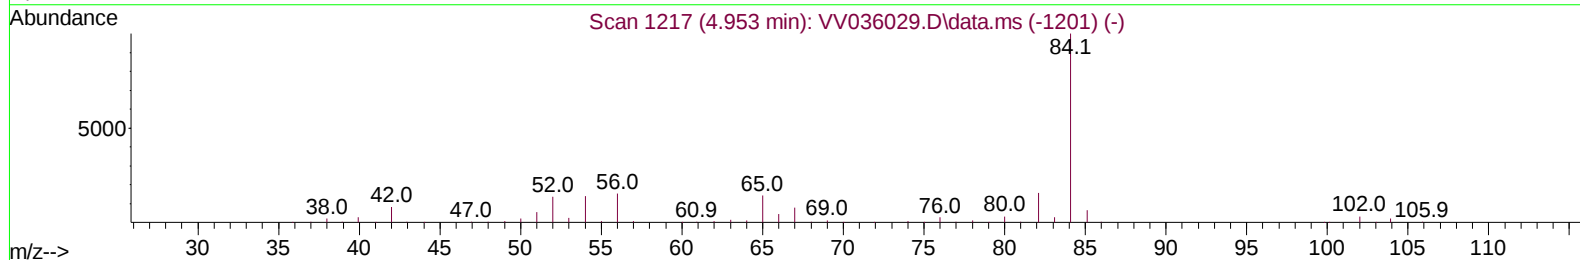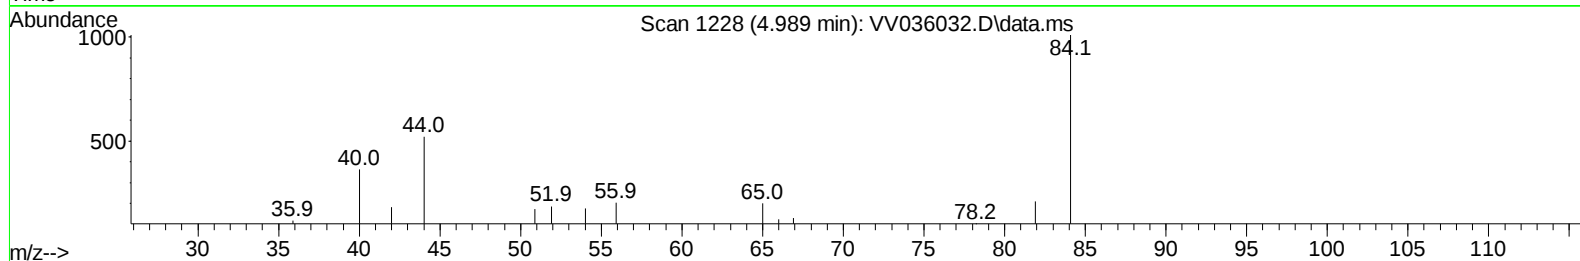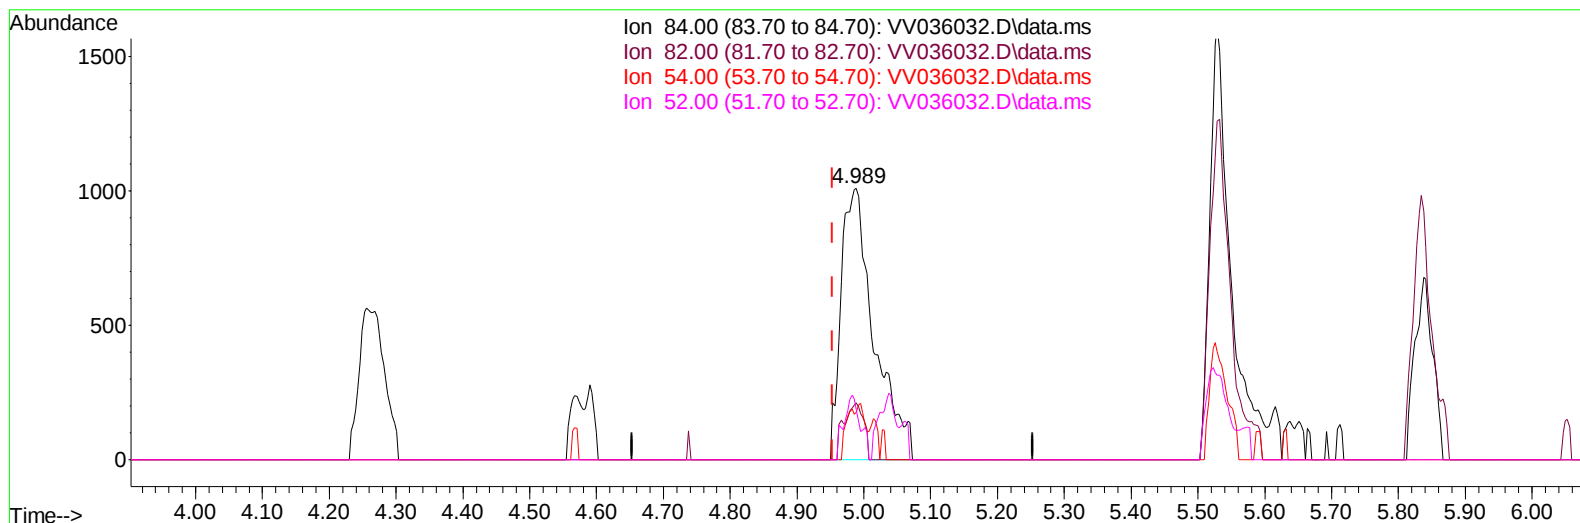

TIC: VV036032.D\data.ms

(32) Benzene-d6 (S)

4.989min (+ 0.035) 0.12 ug/L m

response 3450

Ion	Exp%	Act%
84.00	100.00	100.00
82.00	15.60	0.00#
54.00	14.30	0.00#
52.00	12.70	3.01#




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061124\
Data File : VV036032.D
Acq On : 11 Jun 2024 13:51
Operator : SY/MD
Sample : P2798-02
Misc : 5.35g/10.1mL/MSVOA_V/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB13

Manual IntegrationsAPPROVED

Quant Time: Jun 12 02:07:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 12 02:05:45 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/12/2024
Supervised By :Semsettin Yesilyurt 06/12/2024

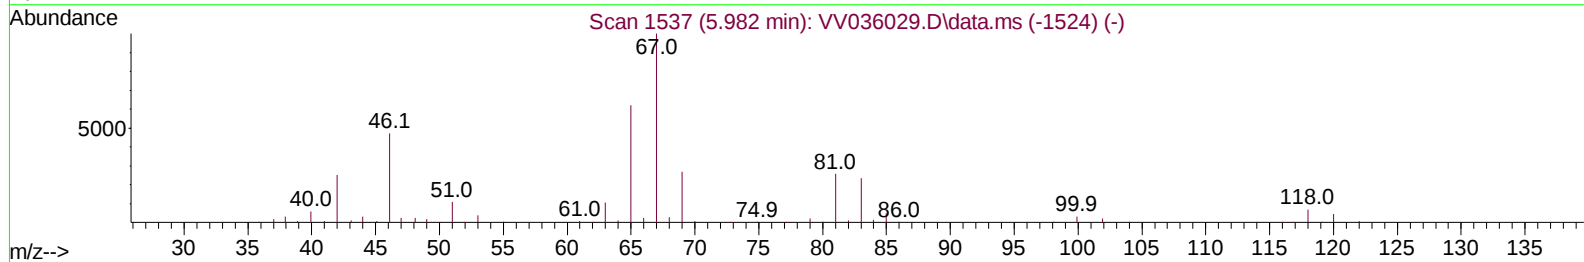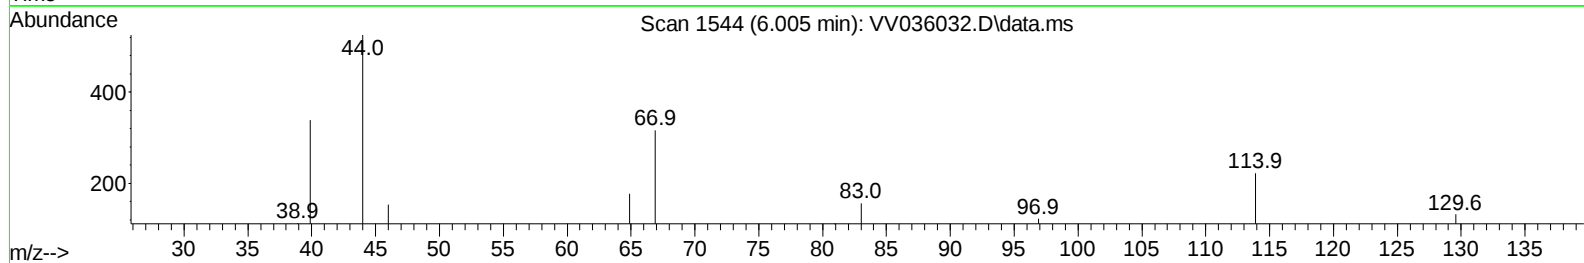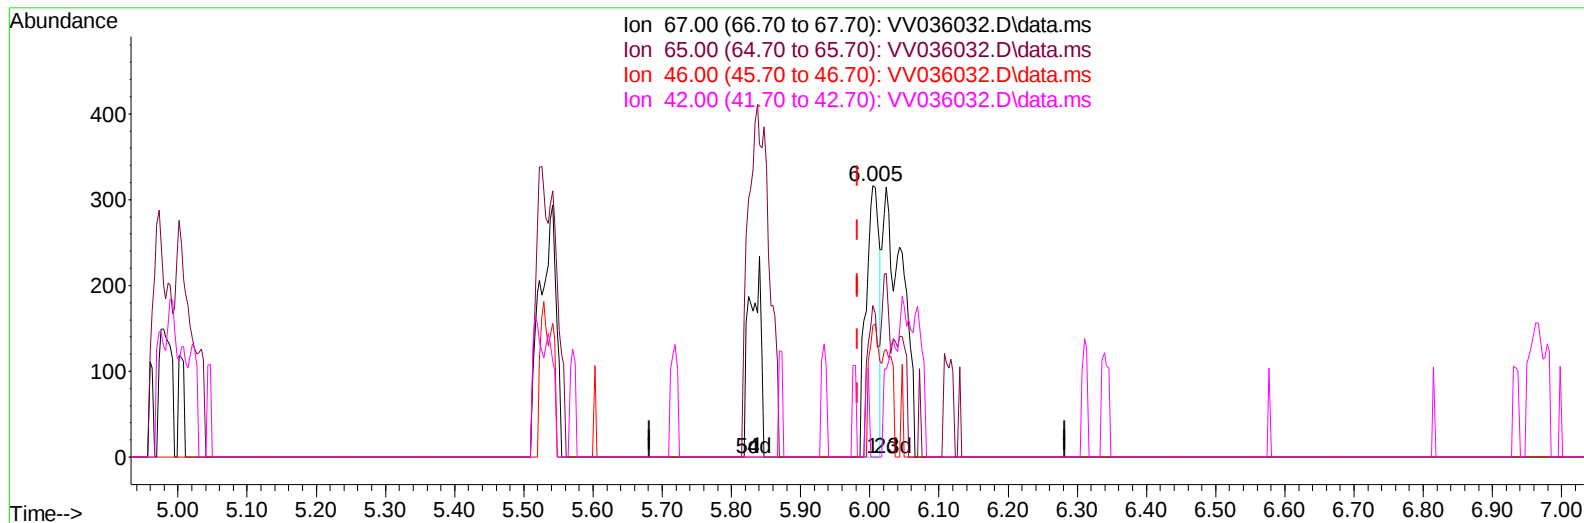

TIC: VV036032.D\data.ms

(36) 1,2-Dichloropropane-d6 (S)

6.005min (+ 0.023) 0.05 ug/L

response 413

Ion	Exp%	Act%
67.00	100.00	100.00
65.00	64.20	40.68#
46.00	47.00	42.37
42.00	25.30	9.69#




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061124\
Data File : VV036032.D
Acq On : 11 Jun 2024 13:51
Operator : SY/MD
Sample : P2798-02
Misc : 5.35g/10.1mL/MSVOA_V/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB13

Manual IntegrationsAPPROVED

Quant Time: Jun 12 02:07:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 12 02:05:45 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/12/2024
Supervised By :Semsettin Yesilyurt 06/12/2024

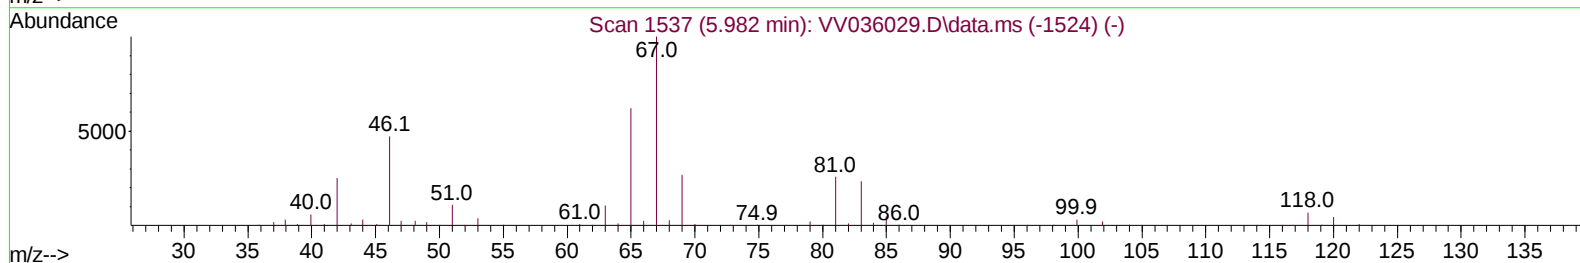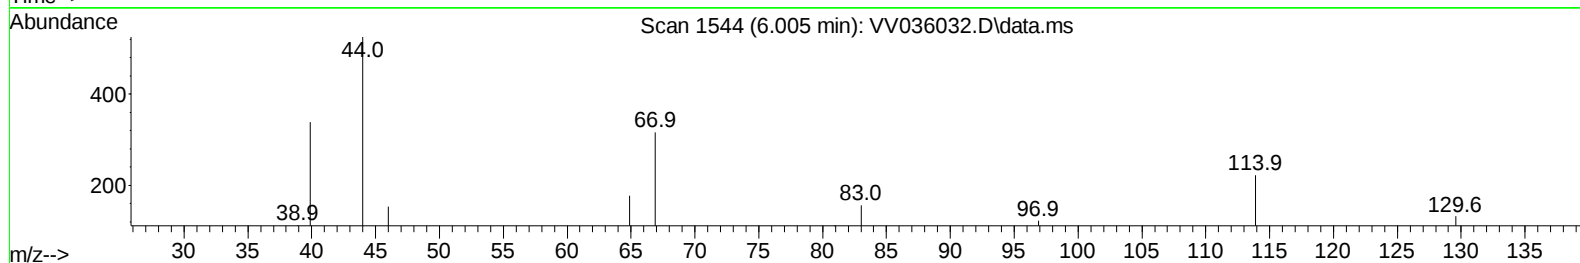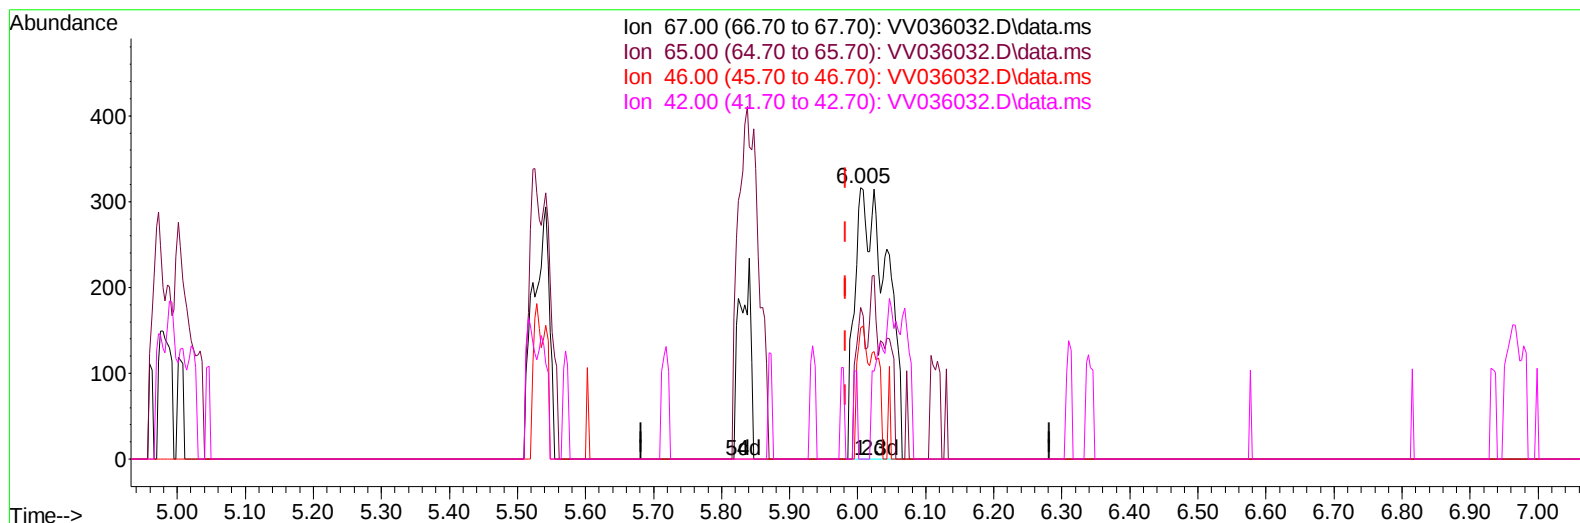

TIC: VV036032.D\data.ms

(36) 1,2-Dichloropropane-d6 (S)

6.005min (+ 0.023) 0.12 ug/L m

response 1041

Ion	Exp%	Act%
67.00	100.00	100.00
65.00	64.20	16.14#
46.00	47.00	16.81#
42.00	25.30	3.84#




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061124\
Data File : VV036032.D
Acq On : 11 Jun 2024 13:51
Operator : SY/MD
Sample : P2798-02
Misc : 5.35g/10.1mL/MSVOA_V/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB13

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 06/12/2024
Supervised By :Semsettin Yesilyurt 06/12/2024

Quant Time: Jun 12 02:07:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 12 02:05:45 2024
Response via : Initial Calibration

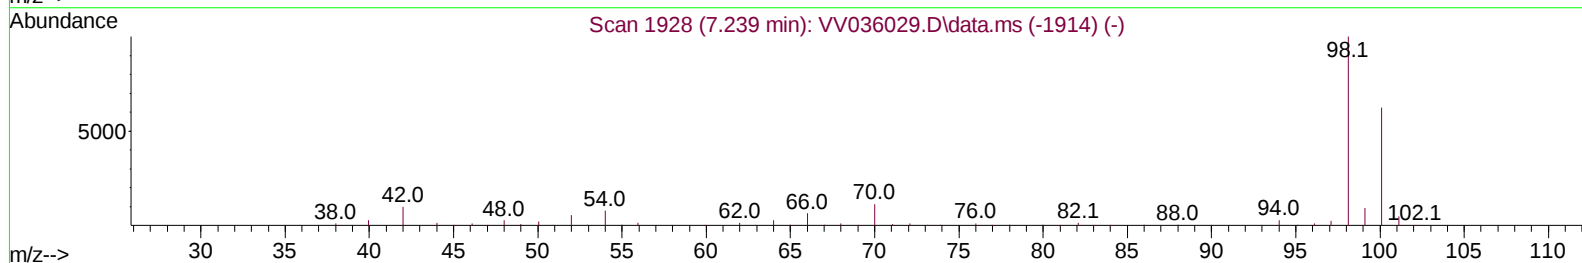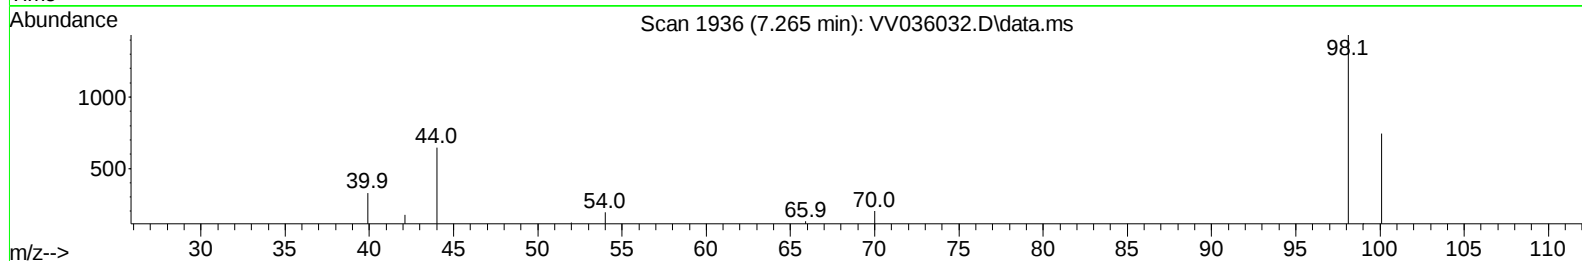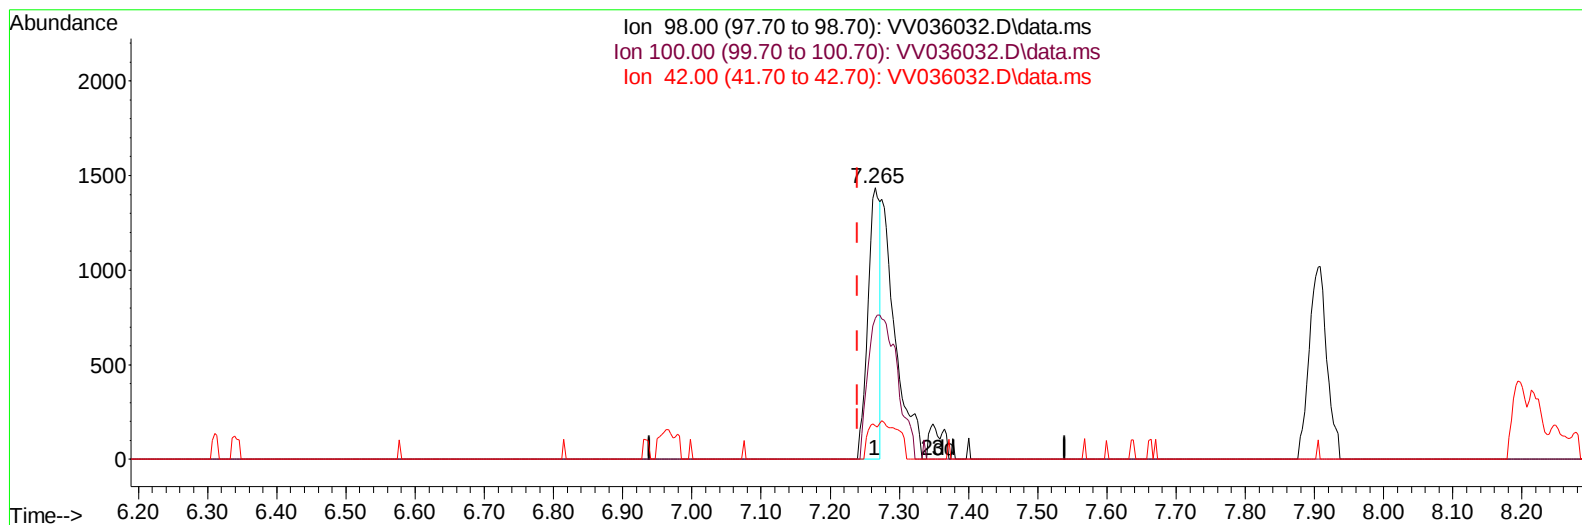

TIC: VV036032.D\data.ms

(41) Toluene-d8 (S)

7.265min (+ 0.026) 0.07 ug/L

response 1711

Ion	Exp%	Act%
98.00	100.00	100.00
100.00	64.70	93.69#
42.00	9.90	11.10
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061124\
Data File : VV036032.D
Acq On : 11 Jun 2024 13:51
Operator : SY/MD
Sample : P2798-02
Misc : 5.35g/10.1mL/MSVOA_V/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB13

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 06/12/2024
Supervised By :Semsettin Yesilyurt 06/12/2024

Quant Time: Jun 12 02:07:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 12 02:05:45 2024
Response via : Initial Calibration

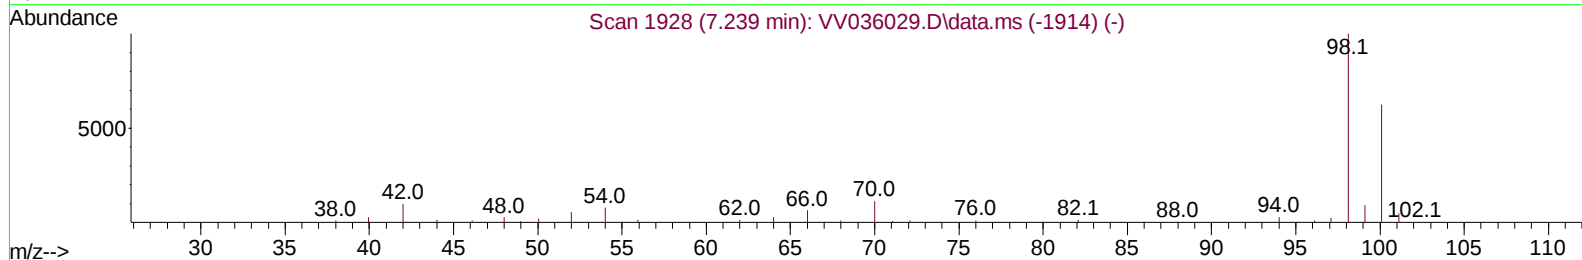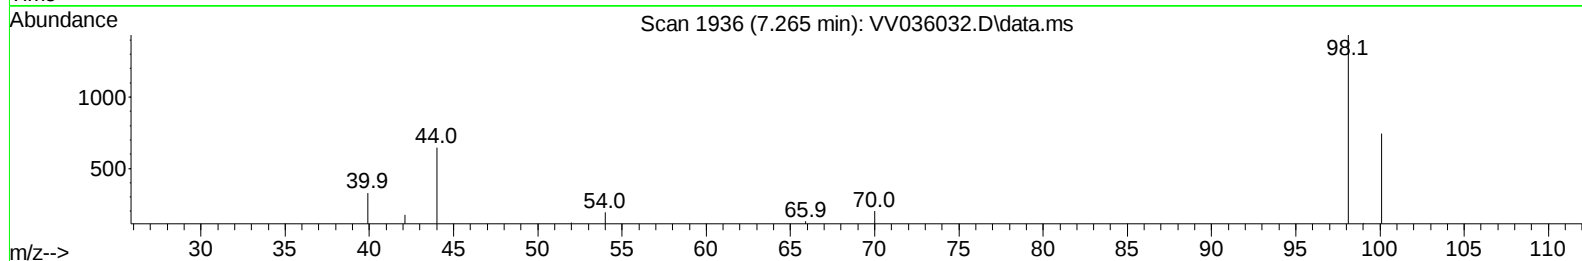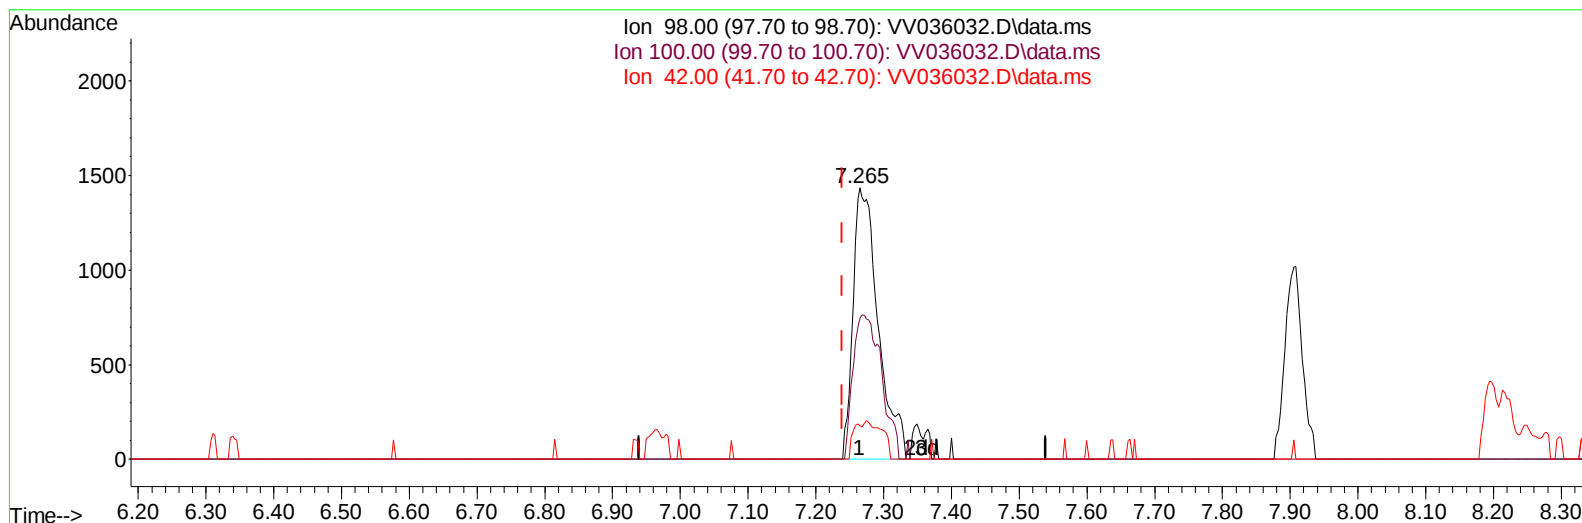

TIC: VV036032.D\data.ms

(41) Toluene-d8 (S)

7.265min (+ 0.026) 0.15 ug/L m

response 3697

Ion	Exp%	Act%
98.00	100.00	100.00
100.00	64.70	43.36#
42.00	9.90	5.14#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061124\
Data File : VV036032.D
Acq On : 11 Jun 2024 13:51
Operator : SY/MD
Sample : P2798-02
Misc : 5.35g/10.1mL/MSVOA_V/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB13

Manual IntegrationsAPPROVED

Quant Time: Jun 12 02:07:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 12 02:05:45 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/12/2024
Supervised By :Semsettin Yesilyurt 06/12/2024

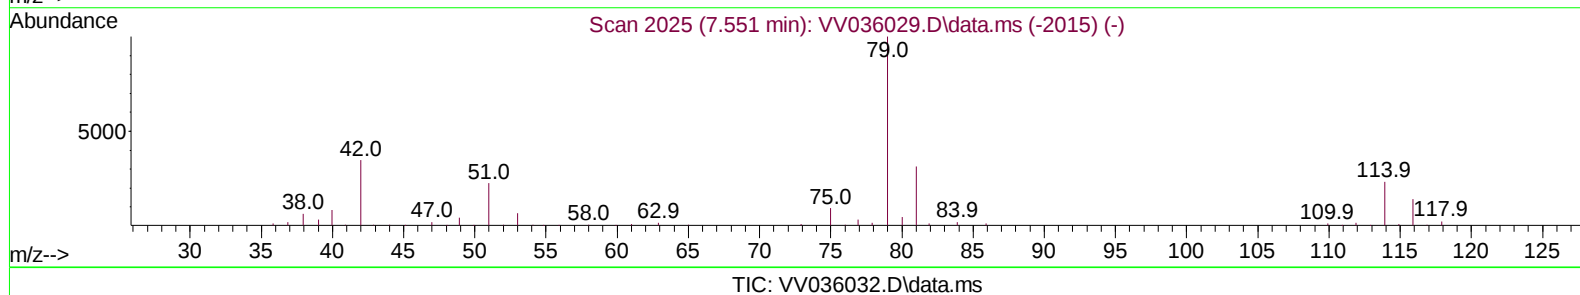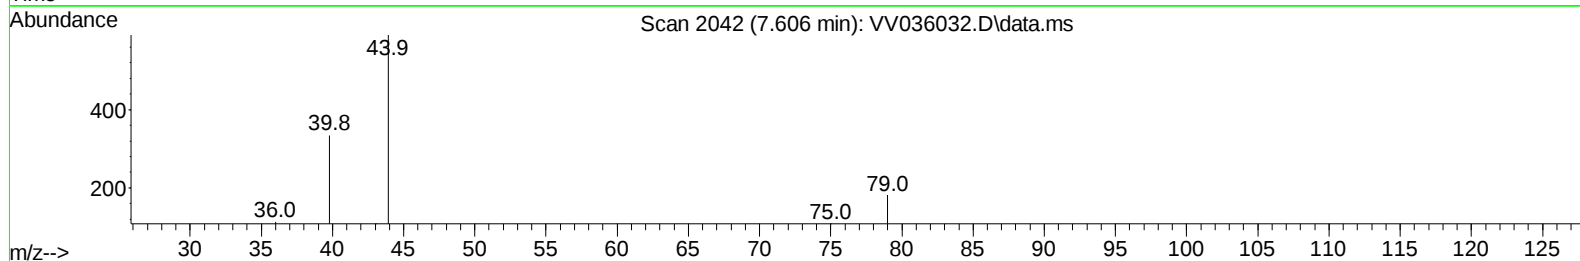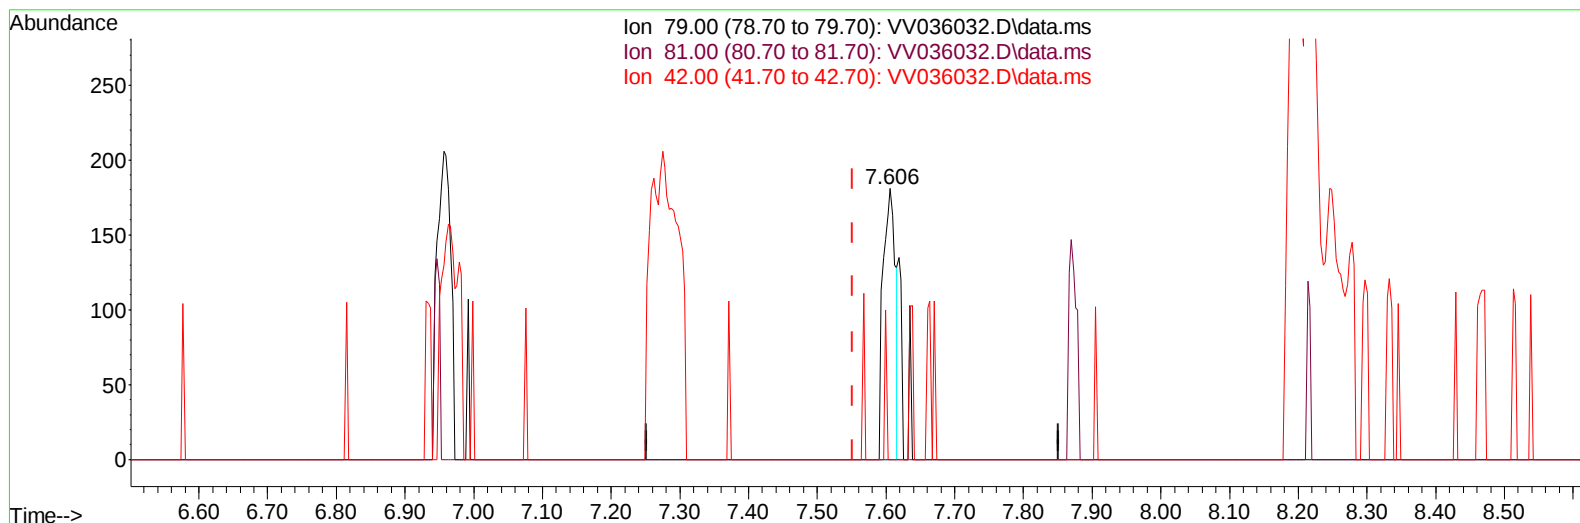

(43) trans-1,3-Dichloropropene-d4 (S)

7.606min (+ 0.055) 0.06 ug/L

response 224

Ion	Exp%	Act%
79.00	100.00	100.00
81.00	32.80	0.00#
42.00	38.70	17.86#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061124\
Data File : VV036032.D
Acq On : 11 Jun 2024 13:51
Operator : SY/MD
Sample : P2798-02
Misc : 5.35g/10.1mL/MSVOA_V/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB13

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 06/12/2024
Supervised By :Semsettin Yesilyurt 06/12/2024

Quant Time: Jun 12 02:07:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 12 02:05:45 2024
Response via : Initial Calibration

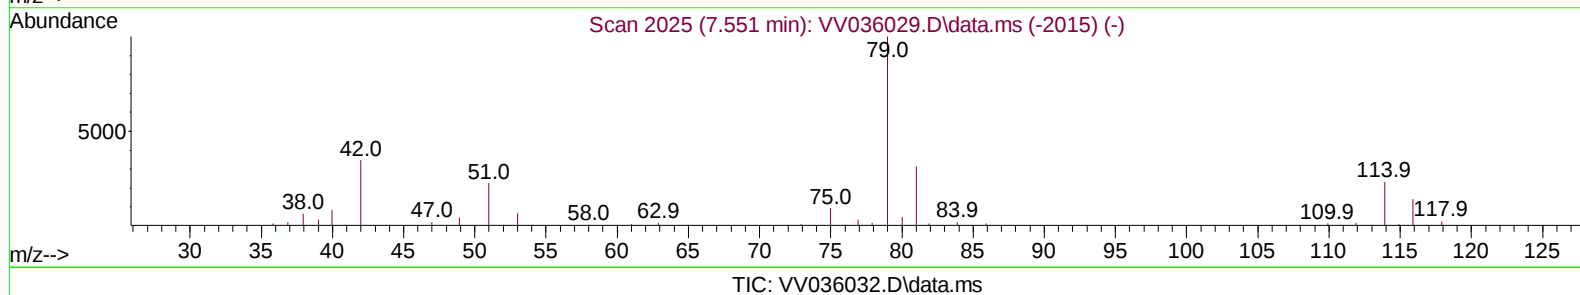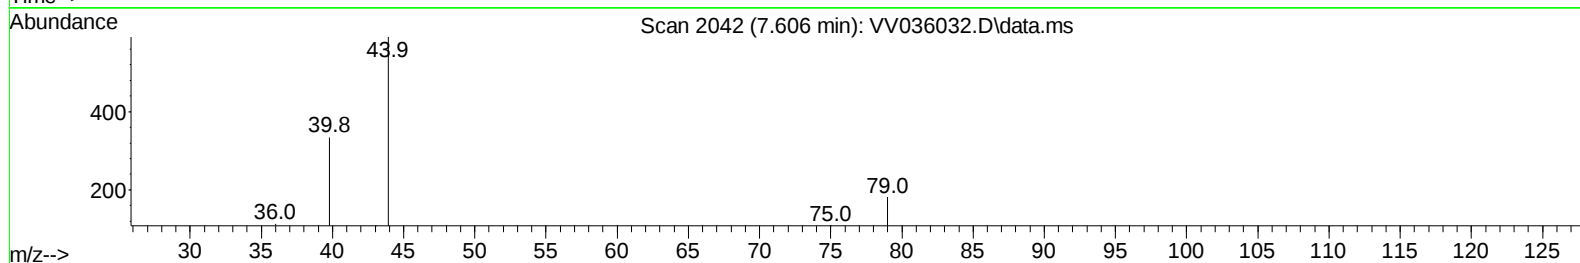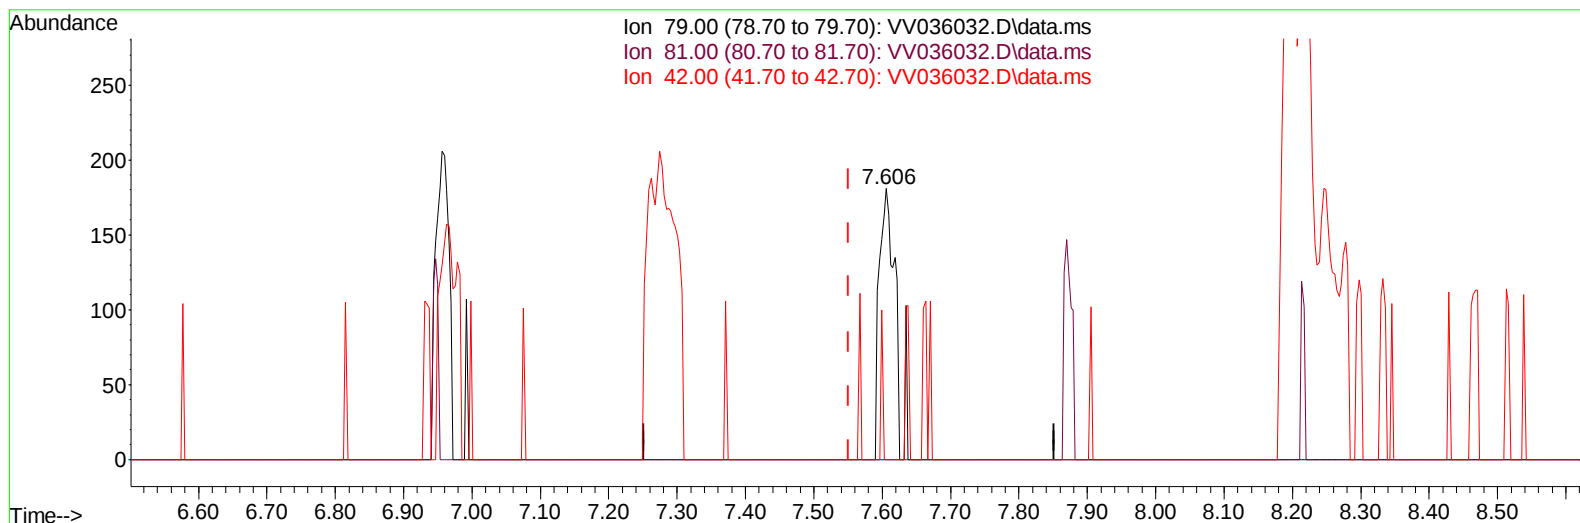**(43) trans-1,3-Dichloropropene-d4 (S)**

7.606min (+ 0.055) 0.08 ug/L m

response 273

Ion	Exp%	Act%
79.00	100.00	100.00
81.00	32.80	0.00#
42.00	38.70	14.65#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061124\
 Data File : VV036032.D
 Acq On : 11 Jun 2024 13:51
 Operator : SY/MD
 Sample : P2798-02
 Misc : 5.35g/10.1mL/MSVOA_V/SOIL/A
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB13

Manual IntegrationsAPPROVED

Quant Time: Jun 12 02:07:01 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 12 02:05:45 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/12/2024
 Supervised By :Semsettin Yesilyurt 06/12/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	492996	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	469755	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	213624	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	2282	0.252	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	1.000%#	
7) Chloroethane-d5	1.529	69	1181m	0.163	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	0.640%#	
11) 1,1-Dichloroethene-d2	2.047	65	683m	0.169	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	0.680%#	
21) 2-Butanone-d5	3.818	46	149m	0.072	ug/L	0.02
Spiked Amount 50.000	Range 20	- 135	Recovery	=	0.140%#	
24) Chloroform-d	4.256	84	1492m	0.095	ug/L	0.01
Spiked Amount 25.000	Range 40	- 150	Recovery	=	0.400%#	
26) 1,2-Dichloroethane-d4	4.973	65	903m	0.110	ug/L	0.04
Spiked Amount 25.000	Range 70	- 130	Recovery	=	0.440%#	
32) Benzene-d6	4.989	84	3450m	0.124	ug/L	0.04
Spiked Amount 25.000	Range 20	- 135	Recovery	=	0.480%#	
36) 1,2-Dichloropropane-d6	6.005	67	1041m	0.118	ug/L	0.02
Spiked Amount 25.000	Range 70	- 120	Recovery	=	0.480%#	
41) Toluene-d8	7.265	98	3697m	0.150	ug/L	0.03
Spiked Amount 25.000	Range 30	- 130	Recovery	=	0.600%#	
43) trans-1,3-Dichloroprop...	7.606	79	273m	0.076	ug/L	0.05
Spiked Amount 25.000	Range 30	- 135	Recovery	=	0.320%#	
47) 2-Hexanone-d5	0.000	63	0	0.000	ug/L	
Spiked Amount 50.000	Range 20	- 135	Recovery	=	0.000%#	
56) 1,1,2,2-Tetrachloroeth...	10.159	84	1215	0.185	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	0.720%#	
66) 1,2-Dichlorobenzene-d4	11.564	152	3820	0.488	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	1.960%#	
Target Compounds						
					Qvalue	
5) vinyl chloride	1.281	62	169478	15.780	ug/L	98
13) Acetone	2.124	43	8832	2.726	ug/L #	47
16) Methylene chloride	2.442	84	31980	2.867	ug/L	98
20) cis-1,2-Dichloroethene	3.809	96	685060	81.297	ug/L	99
34) Trichloroethene	5.834	95	51424	5.461	ug/L	98
42) Toluene	7.326	91	13167	0.419	ug/L	95
46) Tetrachloroethene	7.905	164	29738	4.318	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061124\
Data File : VV036032.D
Acq On : 11 Jun 2024 13:51
Operator : SY/MD
Sample : P2798-02
Misc : 5.35g/10.1mL/MSVOA_V/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB13

Manual IntegrationsAPPROVED

Quant Time: Jun 12 02:07:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 12 02:05:45 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/12/2024
Supervised By :Semsettin Yesilyurt 06/12/2024

