

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061219\
Quantitation Report (QT Reviewed)


Data File : VV011484.D
Acq On : 14 Jun 2019 03:32
Operator : SY/MD
Sample : K3313-09
Misc : 25ML/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COLY9

Manual Integrations
APPROVED

MMDadoda
6/14/2019 4:59:18 PM

Quant Time: Jun 14 07:05:33 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 14 06:06:48 2019
Response via : Initial Calibration

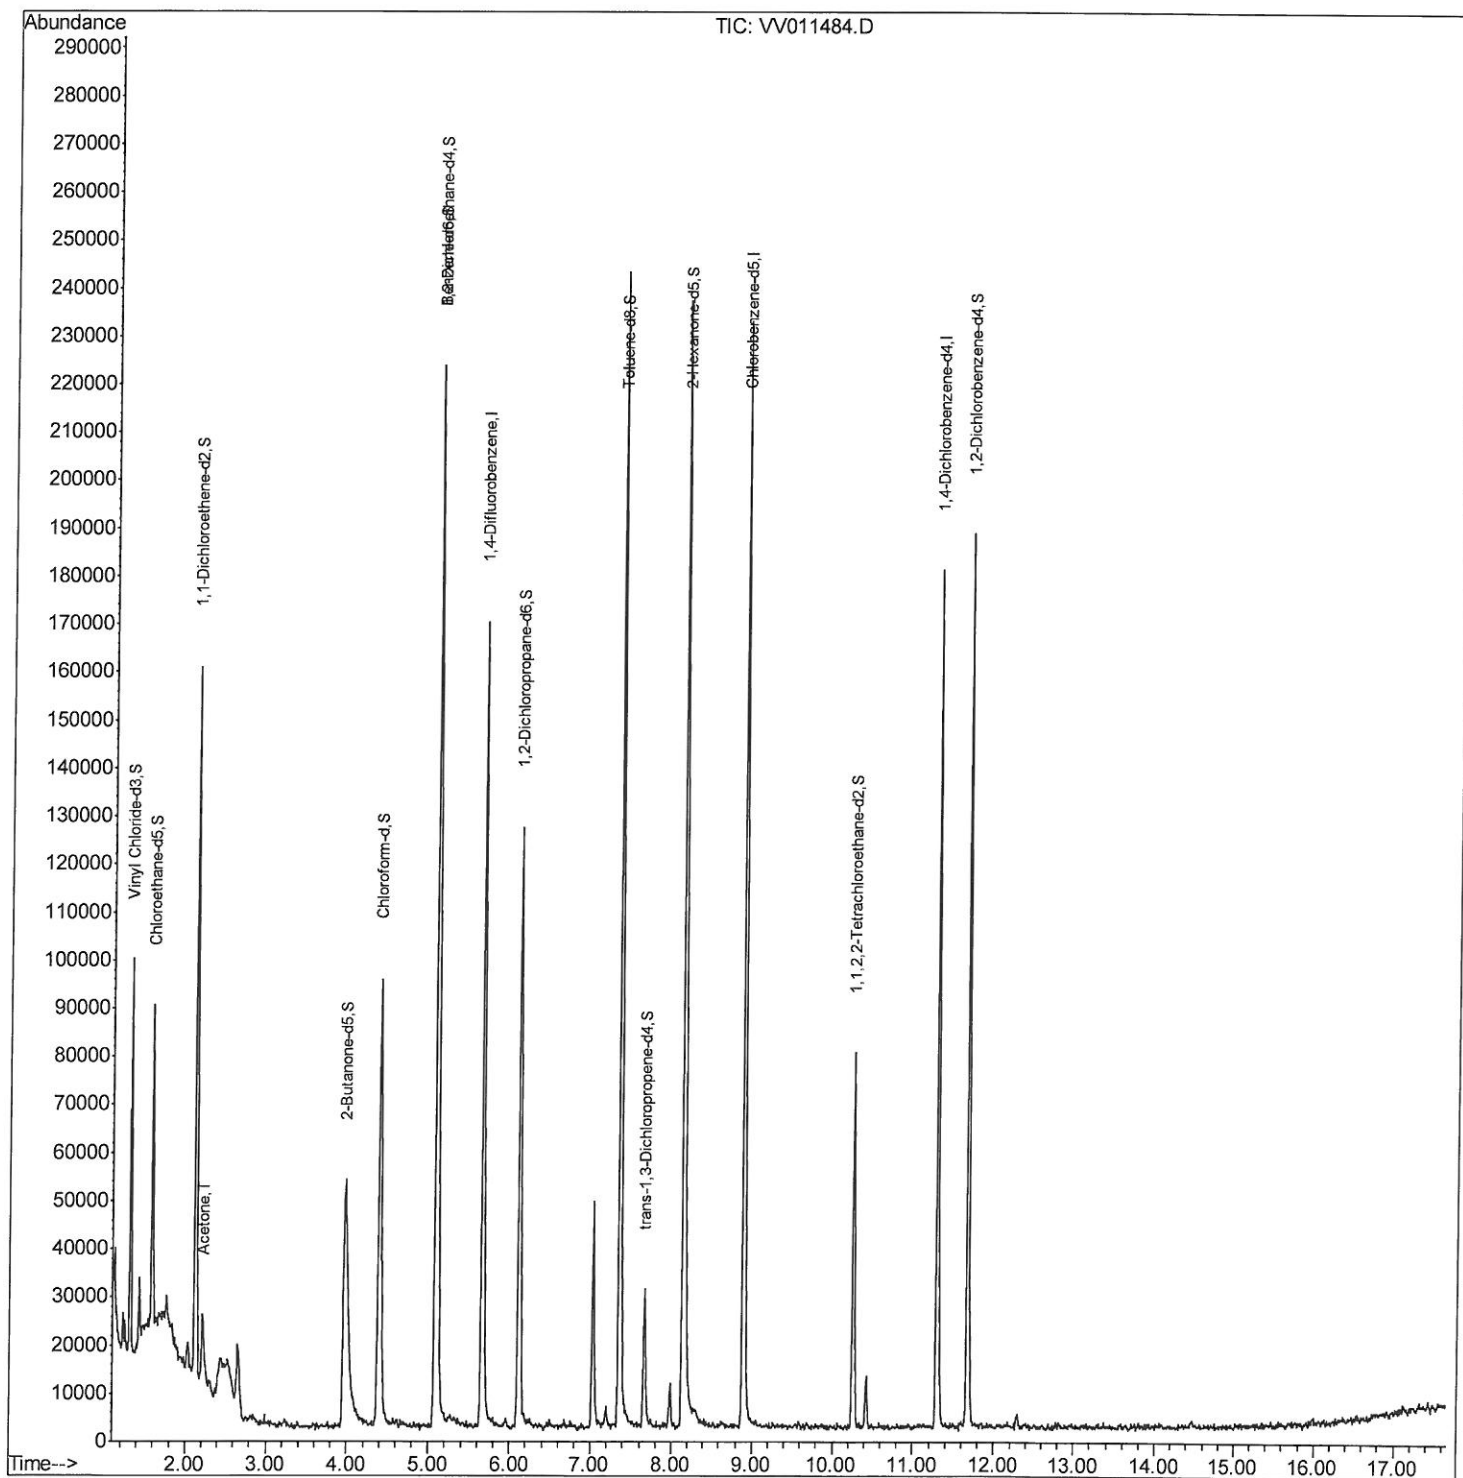

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061219\
Quantitation Report (Qedit)




Data File : VV011484.D
Acq On : 14 Jun 2019 03:32
Operator : SY/MD
Sample : K3313-09
Misc : 25ML/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COLY9

Manual Integrations
APPROVED

MMDadoda
6/14/2019 4:59:18 PM

Quant Time: Jun 14 06:10:53 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 14 06:06:48 2019
Response via : Initial Calibration

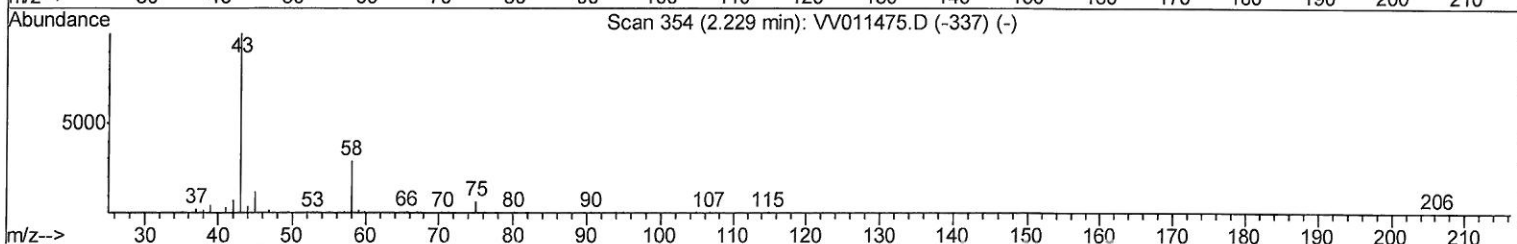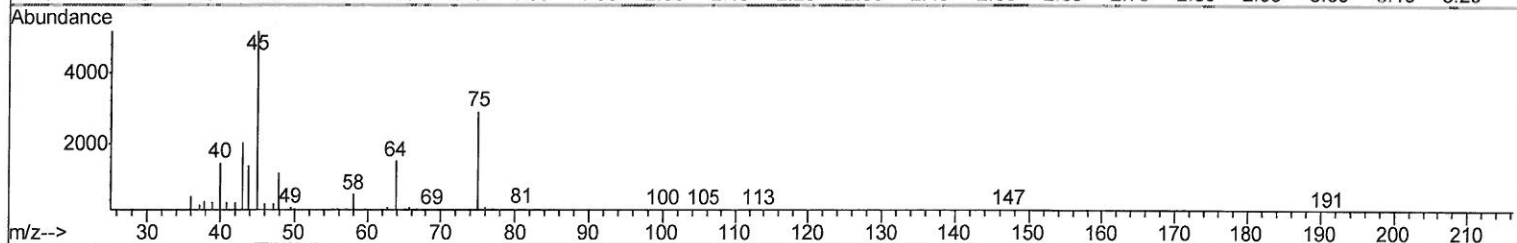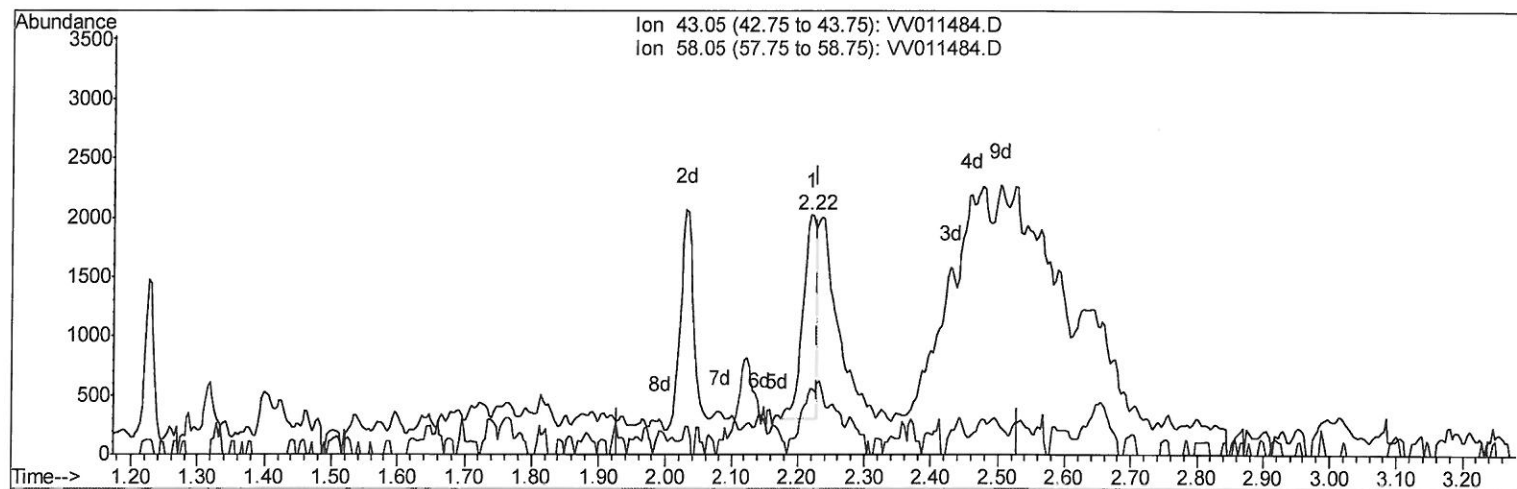

TIC: VV011484.D

(13) Acetone (T)

2.219min (-0.010) 1.73ug/L

response 2572

Ion	Exp%	Act%
43.05	100	100
58.05	27.60	55.17
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061219\
Quantitation Report (Qedit)




Data File : VV011484.D
Acq On : 14 Jun 2019 03:32
Operator : SY/MD
Sample : K3313-09
Misc : 25ML/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COLY9

Manual Integrations
APPROVED

MMDadoda
6/14/2019 4:59:18 PM

Quant Time: Jun 14 06:10:53 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 14 06:06:48 2019
Response via : Initial Calibration

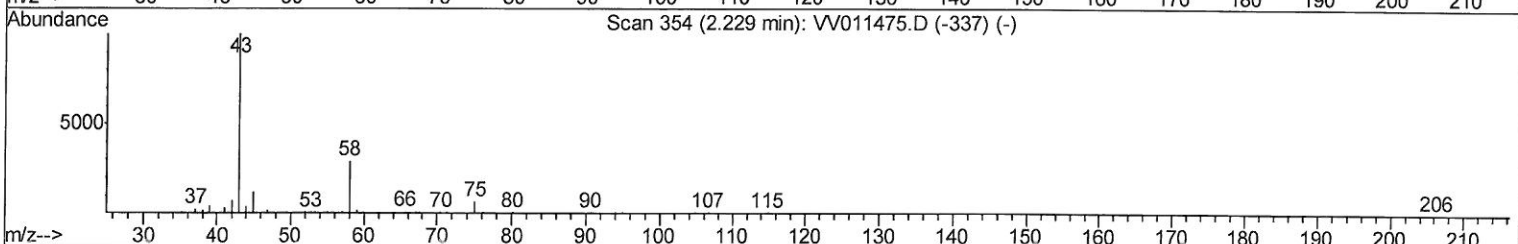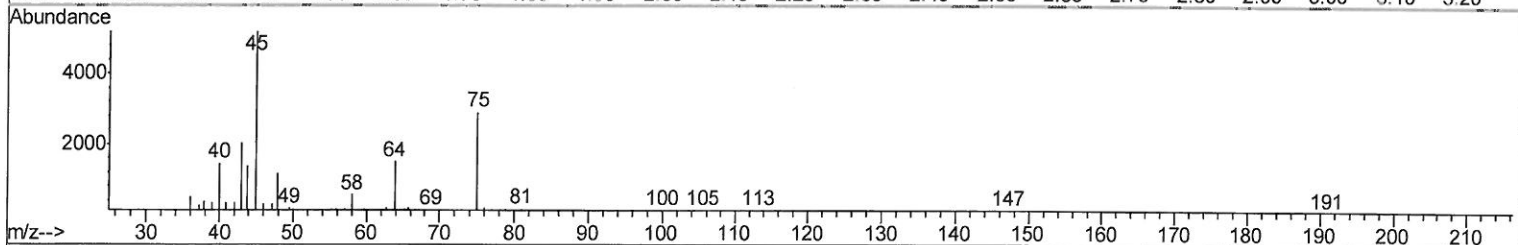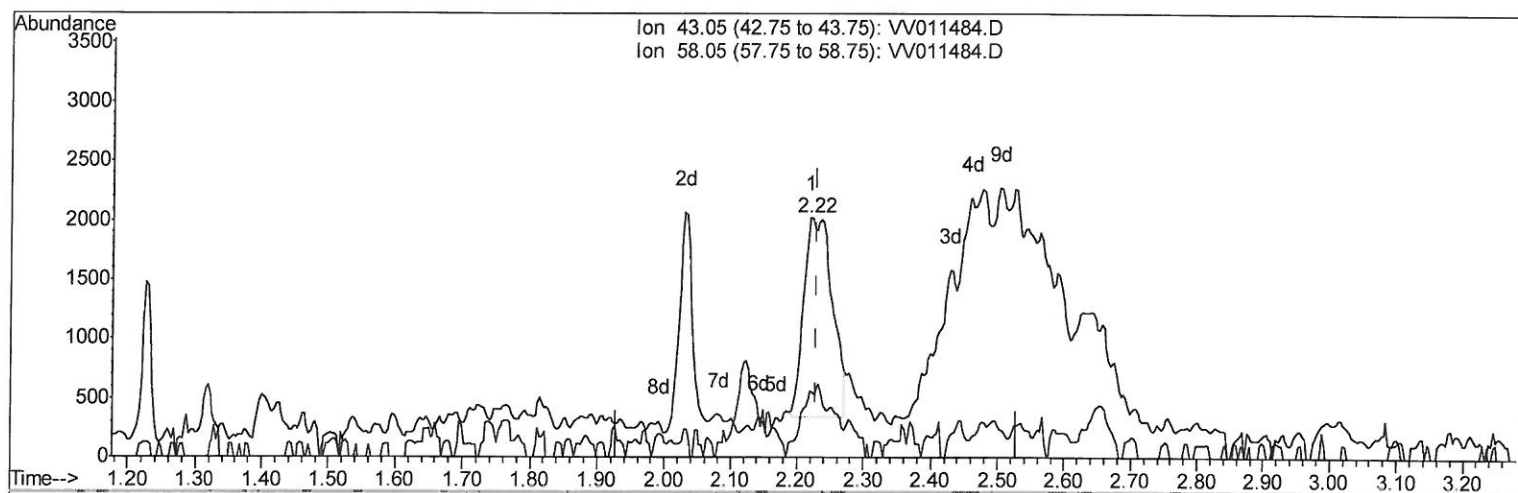

TIC: VV011484.D

(13) Acetone (T)

2.219min (-0.010) 3.38ug/L m

response 5018

Ion	Exp%	Act%
43.05	100	100
58.05	27.60	28.28
0.00	0.00	0.00
0.00	0.00	0.00

7 MD
6/17/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061219\
Quantitation Report (QT Reviewed)

Data File : VV011484.D
Acq On : 14 Jun 2019 03:32
Operator : SY/MD
Sample : K3313-09
Misc : 25ML/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COLY9

Manual Integrations
APPROVED

MMDadoda
6/14/2019 4:59:18 PM

Quant Time: Jun 14 07:05:33 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 14 06:06:48 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	129656	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	117889	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	42787	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	48450	4.93	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.60%
7) Chloroethane-d5	1.58	69	40132	4.91	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.20%
11) 1,1-Dichloroethene-d2	2.12	63	78535	4.00	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	80.00%
20) 2-Butanone-d5	3.97	46	113826	51.46	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.92%
24) Chloroform-d	4.40	84	86711	5.02	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.40%
26) 1,2-Dichloroethane-d4	5.08	65	49594	5.31	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.20%
32) Benzene-d6	5.10	84	176857	5.01	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.20%
36) 1,2-Dichloropropane-d6	6.12	67	52587	4.84	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.80%
41) Toluene-d8	7.36	98	152354	4.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.00%
43) trans-1,3-Dichloropropene-	7.67	79	14266	3.44	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	68.80%
46) 2-Hexanone-d5	8.14	63	85800	49.04	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.08%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	34793	4.70	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	44690	5.29	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.80%

Target Compounds

13) Acetone	2.22	43	5018m	3.384	ug/L	Qvalue
-------------	------	----	-------	-------	------	--------

7MR
6/17/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed