

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061219\
 Data File : VV011416.D
 Acq On : 12 Jun 2019 11:37
 Operator : SY/MD
 Sample : K3286-01
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JQ4

Quant Time: Jun 13 08:57:25 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jun 13 01:13:22 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	136563	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	128032	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	49116	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	30129	2.91	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	58.20%
7) Chloroethane-d5	1.55	69	29822	3.47	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	69.40%
11) 1,1-Dichloroethene-d2	2.11	63	52128	2.52	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	50.40%#
20) 2-Butanone-d5	3.95	46	133500	57.30	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.60%
24) Chloroform-d	4.39	84	78380	4.31	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.20%
26) 1,2-Dichloroethane-d4	5.08	65	43678	4.44	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.80%
32) Benzene-d6	5.08	84	141207	3.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	73.80%
36) 1,2-Dichloropropane-d6	6.11	67	46313	3.93	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	78.60%
41) Toluene-d8	7.35	98	119651	3.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	68.00%#
43) trans-1,3-Dichloropropene-	7.66	79	11841	2.63	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	52.60%#
46) 2-Hexanone-d5	8.14	63	85022	44.75	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.50%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	36645	4.55	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	42632	4.40	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	88.00%


Target Compounds					Ovalue
13) Acetone	2.19	43	4434	2.839 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061219\
Data File : VV011416.D
Acq On : 12 Jun 2019 11:37
Operator : SY/MD
Sample : K3286-01
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JQ4

Quant Time: Jun 13 08:57:25 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jun 13 01:13:22 2019
Response via : Initial Calibration

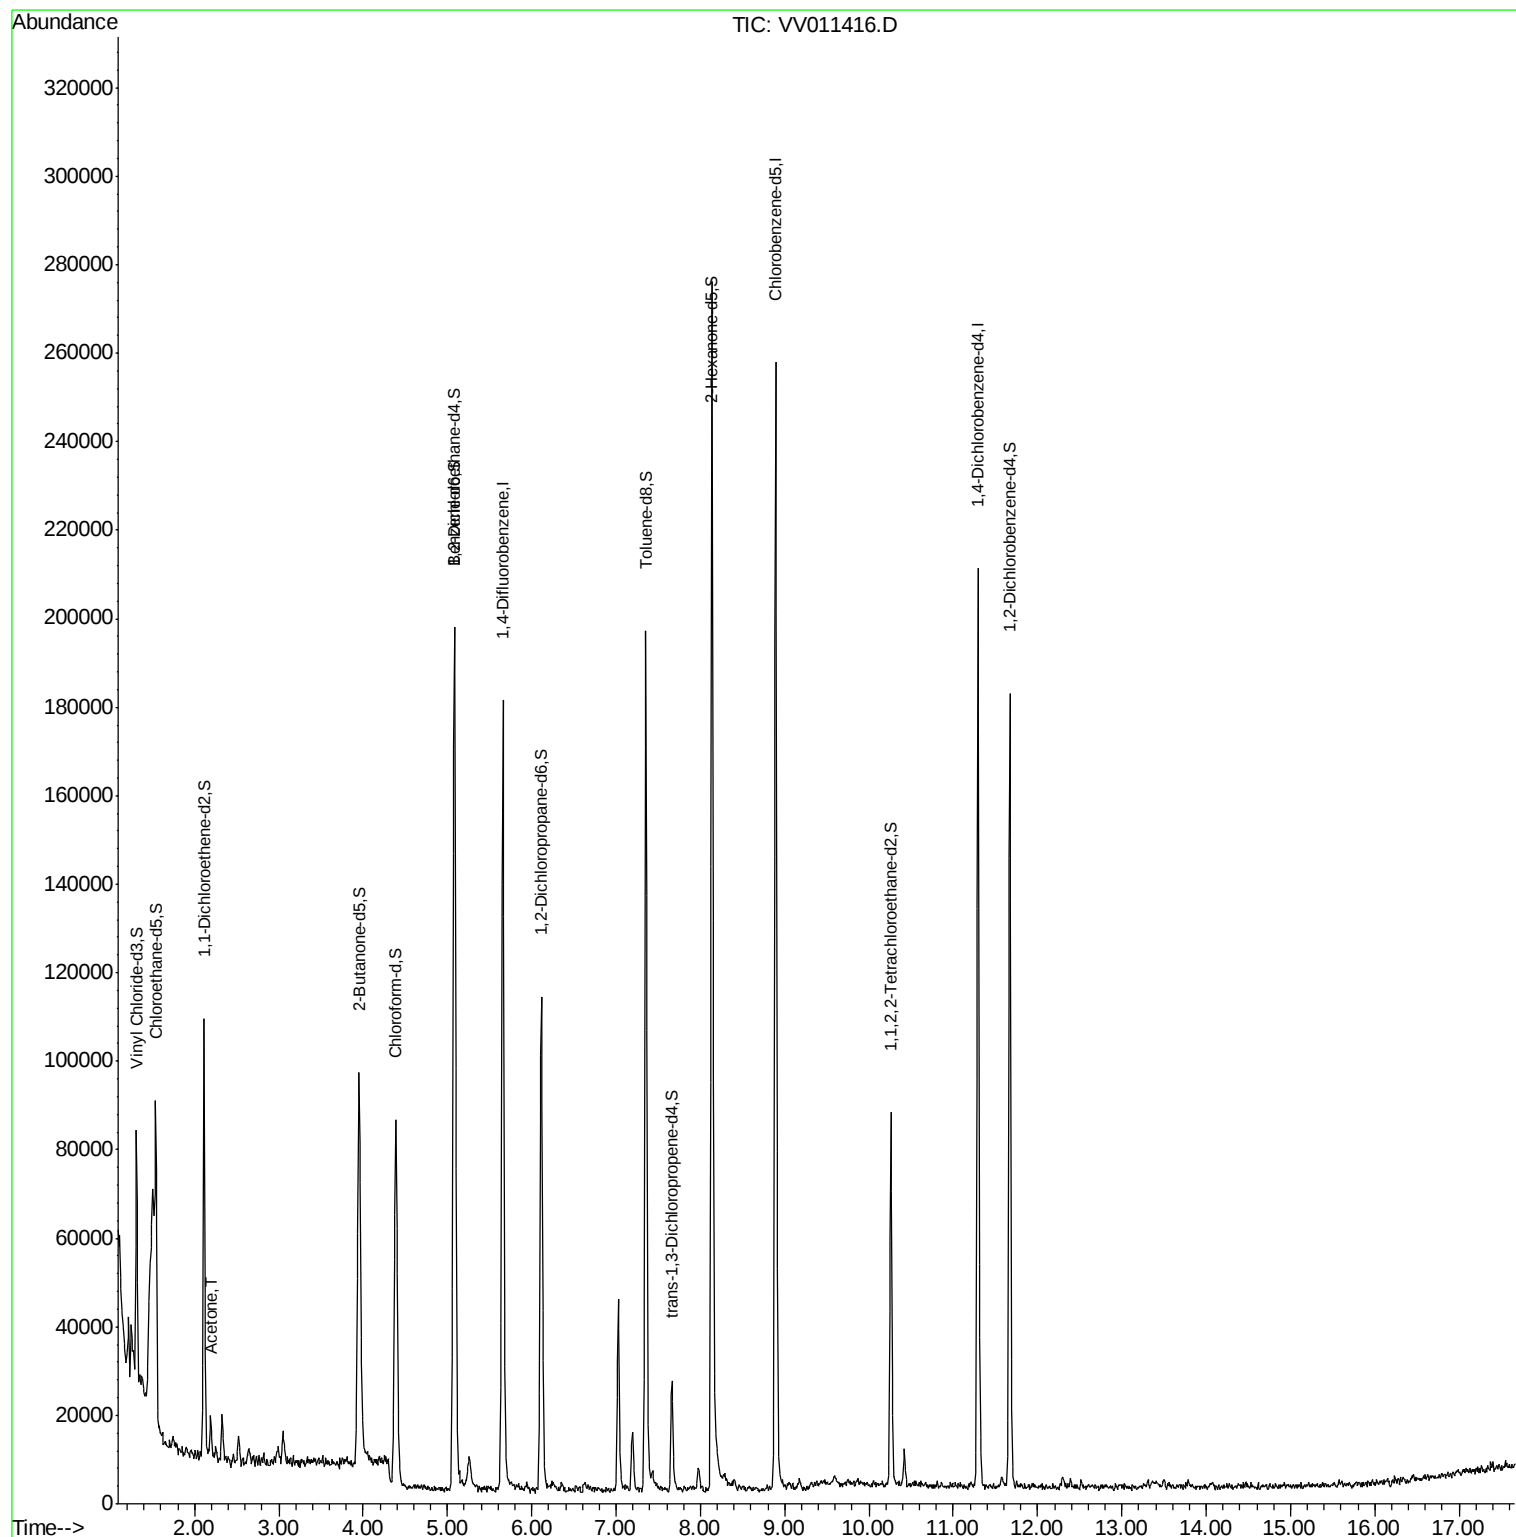

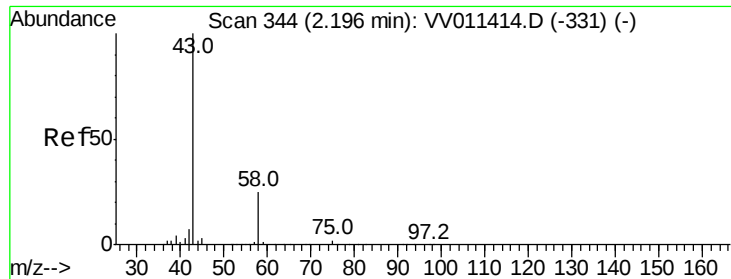

#13

Acetone

Concen: 2.839 ug/L

RT: 2.19 min Scan# 342

Delta R.T. -0.01 min

Lab File: VV011416.D

Acq: 12 Jun 2019 11:37

Instrument :
MSVOA_V
ClientSampleId :
C0JQ4

Tot Ion: 43 Resp: 4434

Ion Ratio Lower Upper

43 100

58 28.8 0.0 55.2

