

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061219\
 Data File : VV011470.D
 Acq On : 13 Jun 2019 19:41
 Operator : SY/MD
 Sample : K3314-10
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COM42

Quant Time: Jun 14 05:54:20 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 14 04:38:08 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	125043	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	108946	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	40639	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	50631	5.34	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	106.80%
7) Chloroethane-d5	1.58	69	44030	5.59	ug/L	0.03
Spiked Amount	5.000	Range	65 - 130	Recovery	=	111.80%
11) 1,1-Dichloroethene-d2	2.12	63	83538	4.41	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	88.20%
20) 2-Butanone-d5	3.96	46	113952	53.42	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.84%
24) Chloroform-d	4.40	84	90228	5.41	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.20%
26) 1,2-Dichloroethane-d4	5.08	65	51261	5.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	113.80%
32) Benzene-d6	5.10	84	183000	5.61	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	112.20%
36) 1,2-Dichloropropane-d6	6.12	67	55800	5.56	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	111.20%
41) Toluene-d8	7.36	98	155130	5.18	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.60%
43) trans-1,3-Dichloropropene-	7.66	79	15463	4.04	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.80%
46) 2-Hexanone-d5	8.14	63	87045	53.84	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	107.68%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	35936	5.25	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	46163	5.75	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	115.00%


Target Compounds					Ovalue
13) Acetone	2.21	43	5594	3.911 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061219\
Data File : VV011470.D
Acq On : 13 Jun 2019 19:41
Operator : SY/MD
Sample : K3314-10
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COM42

Quant Time: Jun 14 05:54:20 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 14 04:38:08 2019
Response via : Initial Calibration

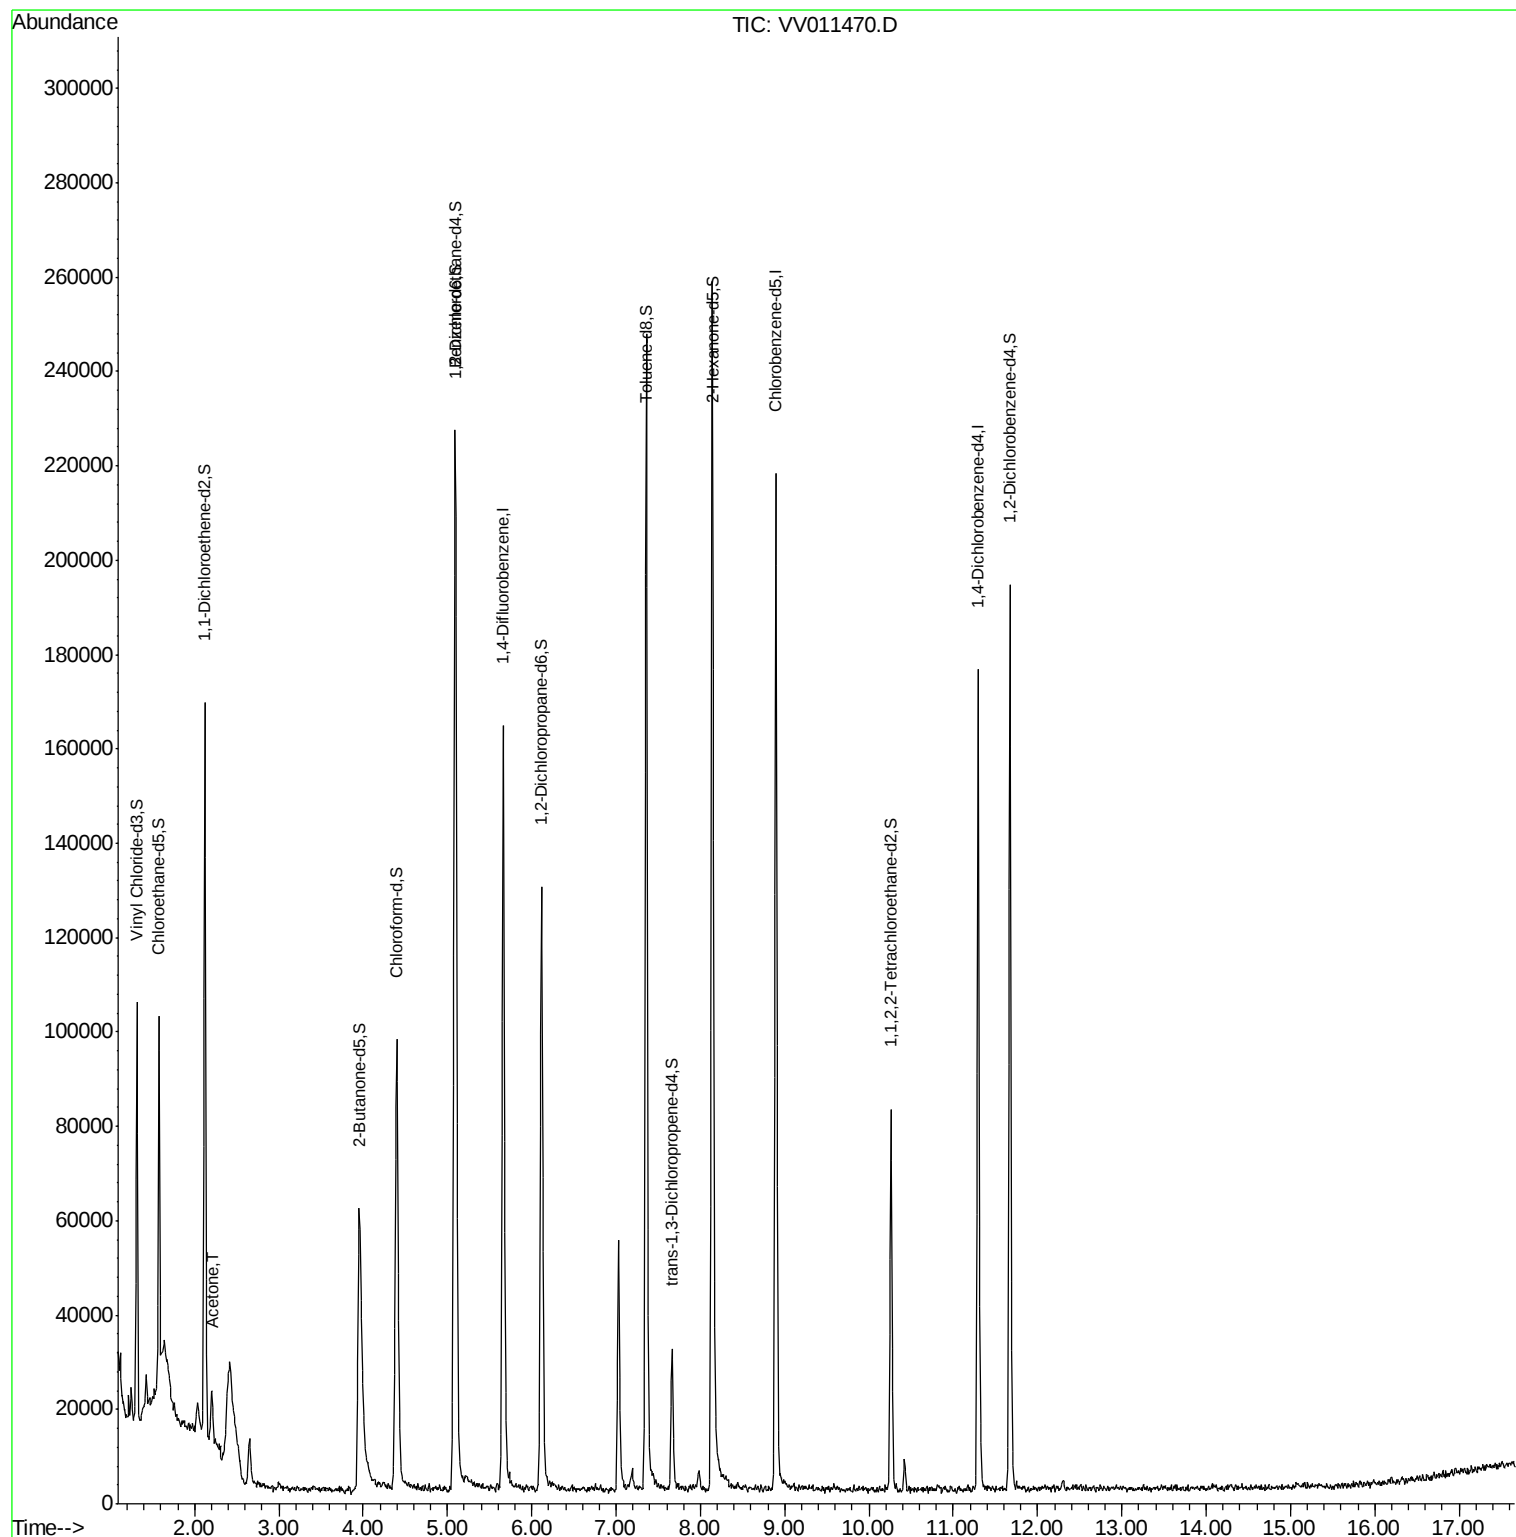

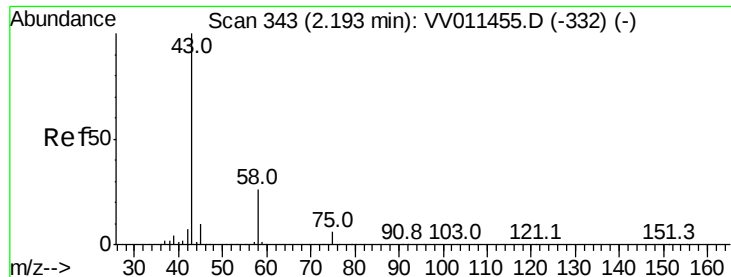

#13

Acetone

Concen: 3.911 ug/L

RT: 2.21 min Scan# 349

Delta R.T. 0.02 min

Lab File: VV011470.D

Acq: 13 Jun 2019 19:41


Instrument :
MSVOA_V
ClientSampleId :
COM42

Tot Ion: 43 Resp: 5594

Ion Ratio Lower Upper

43 100

58 32.0 0.0 55.2

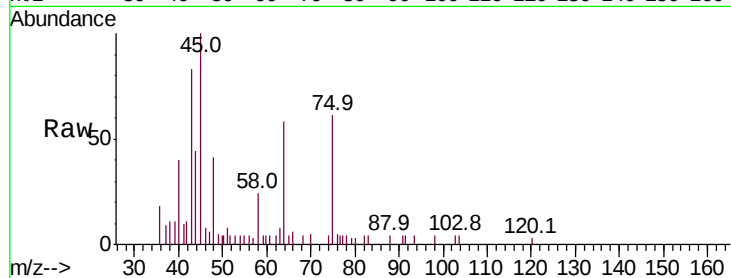

Abundance

Scan 349 (2.212 min): VV011470.D (-250) (-)

