

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061219\
 Data File : VV011486.D
 Acq On : 14 Jun 2019 04:28
 Operator : SY/MD
 Sample : K3313-11
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COLZ1

Quant Time: Jun 14 07:10:41 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 14 06:06:48 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	132727	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	119672	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	43140	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	48775	4.85	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.00%
7) Chloroethane-d5	1.58	69	42782	5.12	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.40%
11) 1,1-Dichloroethene-d2	2.13	63	77420	3.85	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.00%
20) 2-Butanone-d5	3.96	46	111237	49.13	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.26%
24) Chloroform-d	4.40	84	87088	4.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.40%
26) 1,2-Dichloroethane-d4	5.08	65	48655	5.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.60%
32) Benzene-d6	5.10	84	175418	4.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.00%
36) 1,2-Dichloropropane-d6	6.12	67	54410	4.93	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.60%
41) Toluene-d8	7.36	98	154254	4.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.80%
43) trans-1,3-Dichloropropene-	7.67	79	14361	3.42	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	68.40%
46) 2-Hexanone-d5	8.14	63	86481	48.70	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.40%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	34935	4.65	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	44611	5.24	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.80%


Target Compounds					Ovalue
13) Acetone	2.22	43	48225	31.766 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061219\
Data File : VV011486.D
Acq On : 14 Jun 2019 04:28
Operator : SY/MD
Sample : K3313-11
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0LZ1

Quant Time: Jun 14 07:10:41 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 14 06:06:48 2019
Response via : Initial Calibration

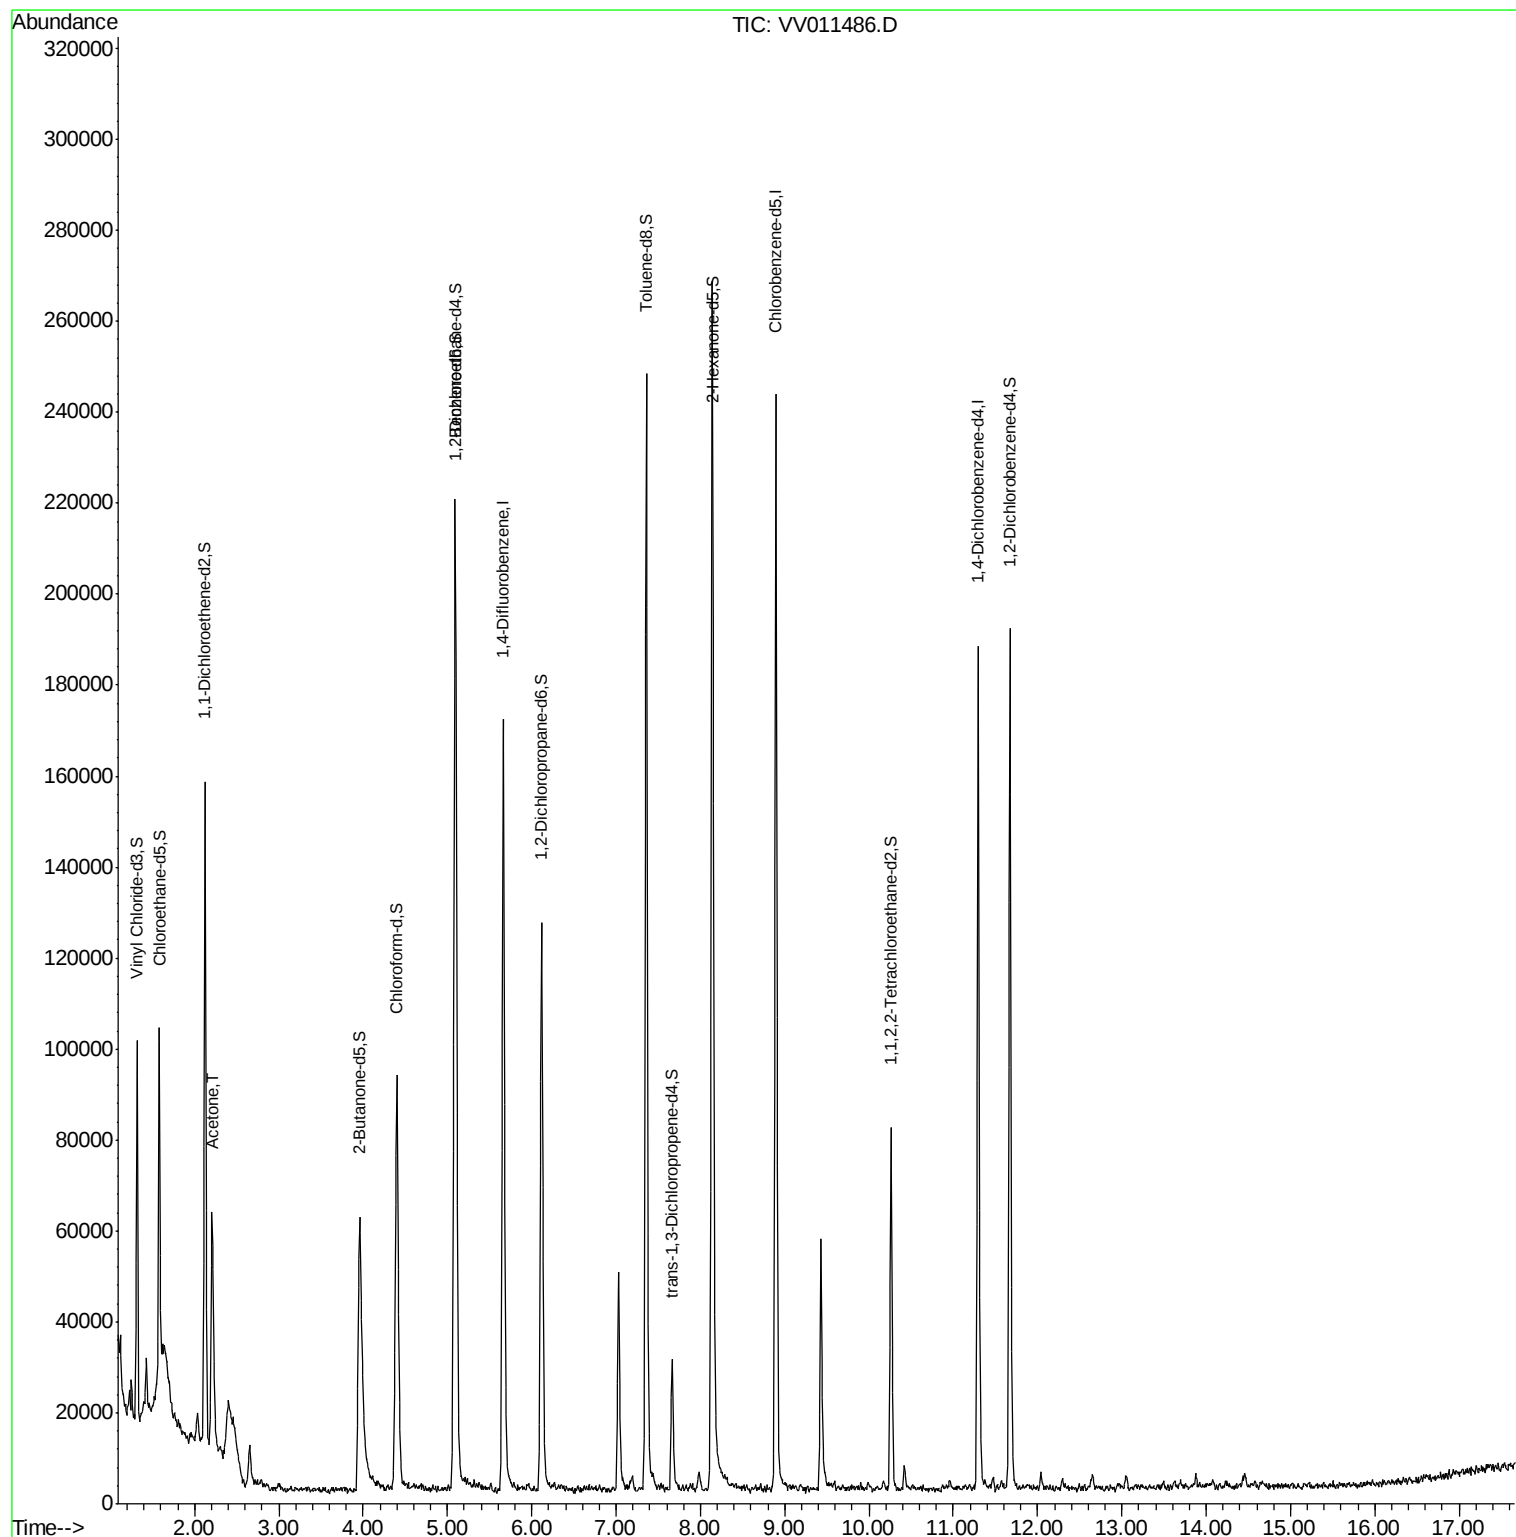

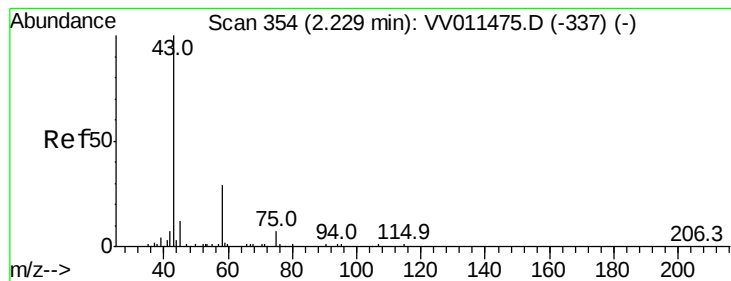

#13

Acetone

Concen: 31.766 ug/L

RT: 2.22 min Scan# 350

Delta R.T. -0.01 min

Lab File: VV011486.D

Acq: 14 Jun 2019 04:28

Instrument :
MSVOA_V
ClientSampleId :
COLZ1

Tot Ion: 43 Resp: 48225

Ion Ratio Lower Upper

43 100

58 25.4 0.0 55.2

