

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061219\
 Data File : VV011490.D
 Acq On : 14 Jun 2019 06:19
 Operator : SY/MD
 Sample : K3313-15
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COLZ5

Quant Time: Jun 14 07:23:11 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 14 06:06:48 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	127799	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	114484	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	41702	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	45678	4.72	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.40%
7) Chloroethane-d5	1.58	69	37507	4.66	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.20%
11) 1,1-Dichloroethene-d2	2.12	63	75166	3.88	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.60%
20) 2-Butanone-d5	3.98	46	110910	50.87	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.74%
24) Chloroform-d	4.40	84	85271	5.00	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.00%
26) 1,2-Dichloroethane-d4	5.08	65	50464	5.48	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.60%
32) Benzene-d6	5.10	84	171319	5.00	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.00%
36) 1,2-Dichloropropane-d6	6.12	67	52856	5.01	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.20%
41) Toluene-d8	7.36	98	145844	4.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.80%
43) trans-1,3-Dichloropropene-	7.66	79	13822	3.44	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	68.80%
46) 2-Hexanone-d5	8.14	63	84943	50.00	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.00%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	35130	4.88	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.60%
64) 1,2-Dichlorobenzene-d4	11.67	152	41936	5.09	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.80%


Target Compounds					Ovalue
16) Methylene chloride	2.53	84	3170	0.382 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061219\
Data File : VV011490.D
Acq On : 14 Jun 2019 06:19
Operator : SY/MD
Sample : K3313-15
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0LZ5

Quant Time: Jun 14 07:23:11 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 14 06:06:48 2019
Response via : Initial Calibration

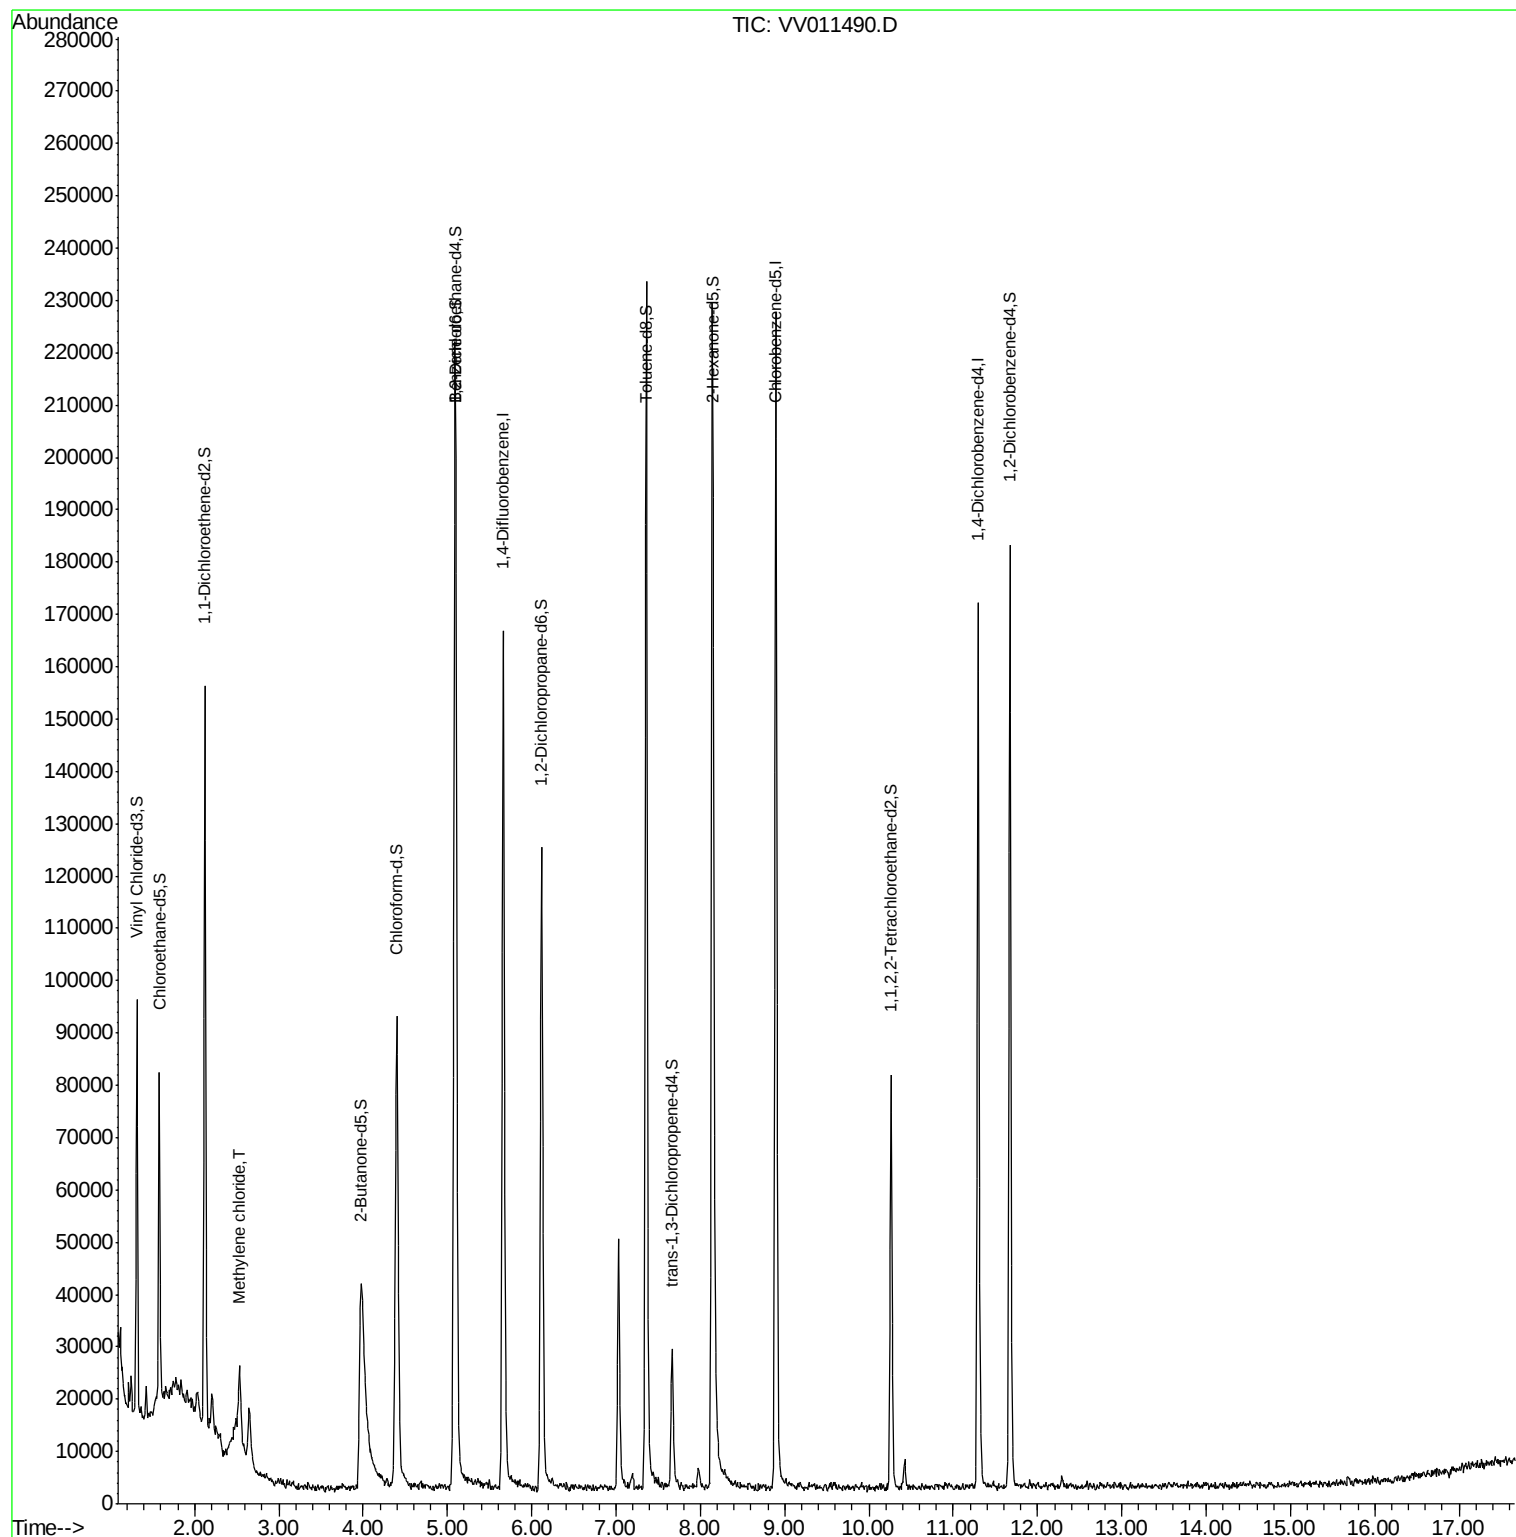

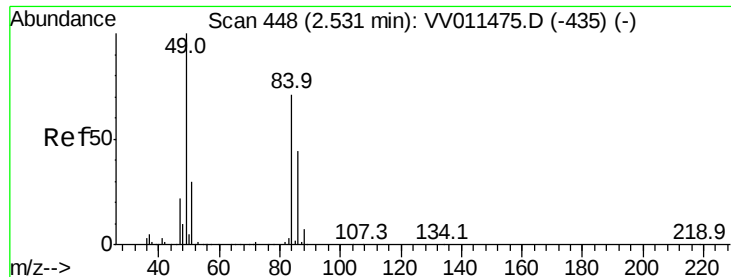

#16
Methylene chloride
Concen: 0.382 ug/L
RT: 2.53 min Scan# 448
Delta R.T. 0.00 min
Lab File: VV011490.D
Acq: 14 Jun 2019 06:19

Instrument :
MSVOA_V
ClientSampleId :
COLZ5

Tot Ion: 84 Resp: 3170
Ion Ratio Lower Upper
84 100
86 65.2 44.9 83.3
49 150.1 102.1 189.5

