


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV061219\
Data File : VV011413.D
Acq On : 12 Jun 2019 09:37
Operator : SY/MD
Sample : BFB47
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB47

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Jun 14 09:13:02 2019

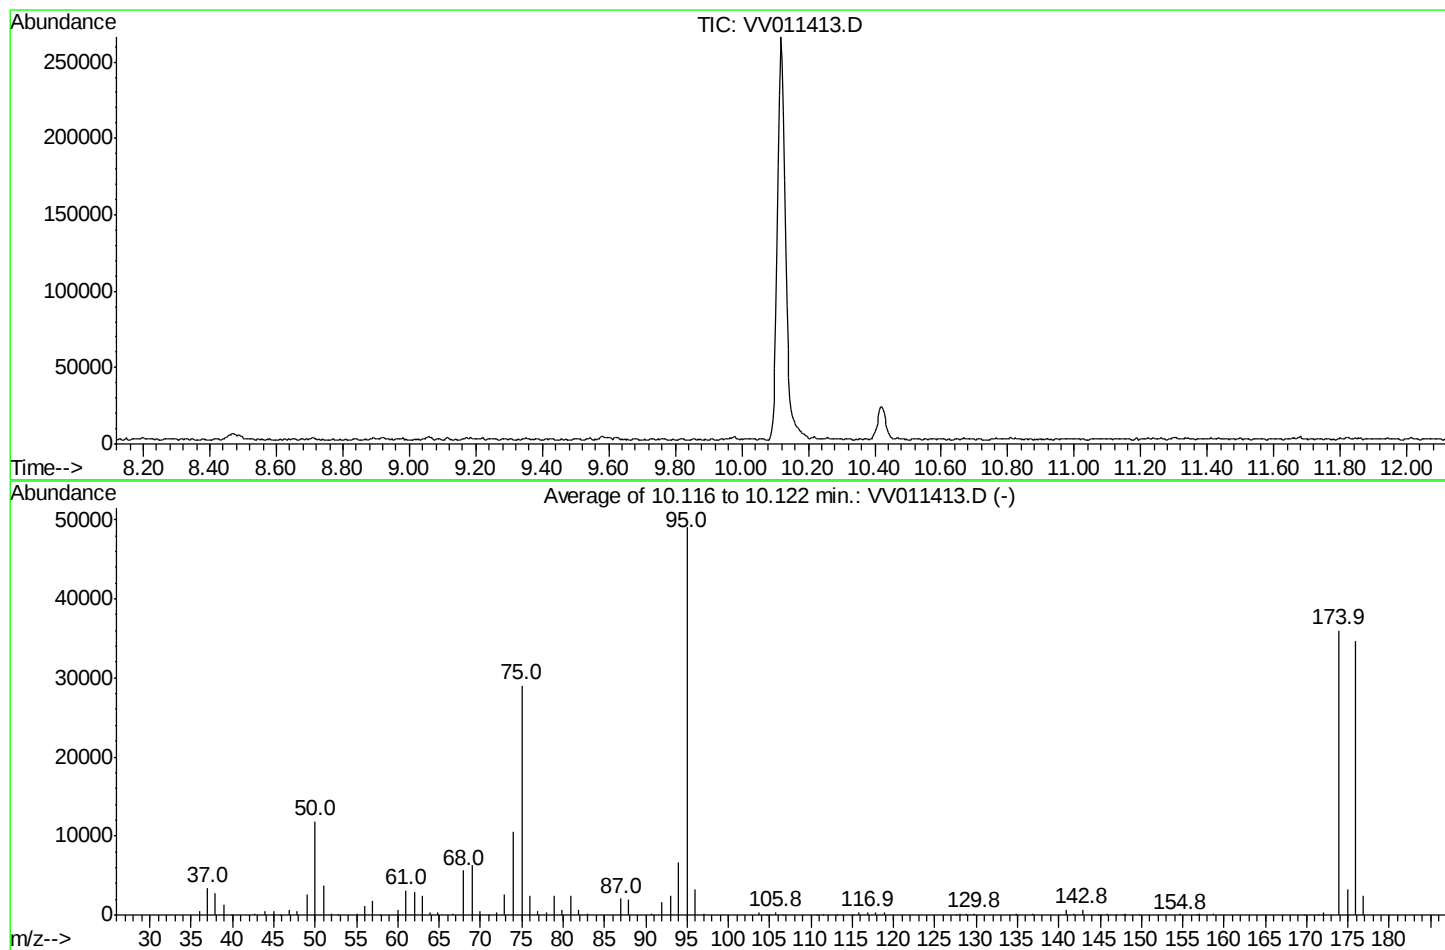

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.3	11897	PASS
75	95	30	80	59.2	29024	PASS
95	95	100	100	100.0	49050	PASS
96	95	5	9	6.7	3278	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.3	35978	PASS
175	174	5	9	8.8	3167	PASS
176	174	95	101	96.4	34680	PASS
177	176	5	9	7.2	2493	PASS

Scan 2793 (10.071 min): VV011413.D
BFB47

m/z	Abundance
36.00	142.0
37.90	136.0
39.90	1173.0
42.00	140.0
43.10	125.0
43.80	370.0
45.00	114.0
49.00	134.0
51.50	117.0
72.60	102.0
79.00	110.0
91.20	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB47

m/z	Abundance
36.00	597.0
37.00	3526.0
38.00	2866.0
38.90	1257.0
39.90	1176.0
41.90	123.0
42.70	131.0
43.90	833.0
44.90	721.0
45.70	153.0
46.90	794.0
47.90	619.0
49.00	2767.0
50.00	11981.0
51.00	3734.0
52.00	194.0
52.70	128.0
55.00	244.0
56.00	1081.0
57.00	1814.0
60.00	610.0
61.00	2953.0
62.00	3012.0
63.00	2340.0
63.90	371.0
64.80	255.0
66.80	233.0
68.00	5790.0
68.90	6481.0
70.00	515.0
71.00	103.0
71.90	370.0
72.90	2542.0
74.00	10457.0
75.00	29176.0
76.00	2511.0
76.90	411.0
78.00	319.0
78.90	2480.0
79.80	711.0
80.90	2394.0
81.90	579.0
83.00	142.0
87.00	2043.0
87.90	2037.0
90.80	240.0
92.00	1587.0
93.00	2440.0
94.00	6701.0
95.00	49128.0
96.00	3341.0
97.00	182.0
103.70	302.0
105.80	435.0
106.60	112.0
110.80	123.0
115.90	233.0
116.90	355.0
117.80	266.0
118.90	284.0
127.60	156.0
128.10	191.0
128.80	168.0
129.70	221.0
134.80	139.0
136.90	159.0
141.00	695.0
141.80	138.0
142.90	629.0
144.70	116.0
145.90	121.0
147.80	199.0
149.70	124.0
154.80	165.0
156.90	133.0
158.70	116.0
169.70	110.0
171.40	144.0
172.00	320.0
173.90	35848.0
175.00	3154.0
175.90	33432.0
176.90	2474.0

Instrument :
MSVOA_V
ClientSampleId :
BFB47

m/z	Abundance
35.90	615.0
37.00	3563.0
38.00	2966.0
38.90	1358.0
39.90	1243.0
41.80	124.0
42.80	139.0
43.90	931.0
45.00	708.0
46.90	680.0
47.90	557.0
49.00	2854.0
50.00	12409.0
51.00	3897.0
51.90	202.0
52.70	116.0
55.00	236.0
56.00	1141.0
57.00	1873.0
57.80	126.0
60.00	598.0
61.00	3194.0
62.00	3085.0
63.00	2440.0
63.90	347.0
64.80	267.0
66.70	213.0
68.00	5808.0
68.90	6371.0
70.00	524.0
70.90	104.0
71.90	347.0
72.90	2603.0
74.00	10927.0
75.00	29904.0
76.00	2478.0
77.00	423.0
77.90	327.0
78.90	2571.0
79.90	729.0
80.90	2459.0
81.90	615.0
83.00	147.0
87.00	2168.0
87.90	2003.0
90.80	232.0
92.00	1710.0
93.00	2453.0
94.00	6873.0
95.00	50336.0
96.00	3376.0
97.00	157.0
103.80	353.0
104.60	119.0
105.80	407.0
106.60	114.0
110.70	102.0
111.50	102.0
115.10	115.0
115.80	276.0
116.90	363.0
117.80	260.0
119.00	333.0
128.00	174.0
128.90	216.0
129.80	229.0
134.90	145.0
136.90	169.0
141.00	682.0
141.80	172.0
142.80	718.0
145.00	106.0
145.90	159.0
146.90	102.0
148.00	167.0
154.70	163.0
157.00	139.0
158.80	112.0
171.90	291.0
173.90	36904.0
175.00	3252.0
175.90	35808.0
176.90	2610.0

Instrument :
MSVOA_V
ClientSampleId :
BFB47

m/z	Abundance
35.90	648.0
37.00	3314.0
38.00	2821.0
38.90	1311.0
39.90	1292.0
42.70	126.0
43.90	903.0
44.90	577.0
46.90	569.0
47.80	411.0
49.00	2660.0
50.00	11302.0
51.00	3767.0
51.90	193.0
55.00	243.0
56.00	1084.0
57.00	1776.0
57.90	119.0
60.00	550.0
61.00	3111.0
62.00	2902.0
63.00	2326.0
63.90	280.0
64.80	258.0
66.70	222.0
68.00	5362.0
69.00	5941.0
70.00	476.0
71.90	305.0
72.90	2506.0
74.00	10161.0
75.00	27992.0
76.00	2231.0
77.00	398.0
77.90	294.0
78.90	2374.0
79.90	665.0
80.90	2306.0
81.80	623.0
82.90	162.0
87.00	2080.0
87.90	1847.0
90.70	224.0
92.00	1715.0
92.90	2238.0
93.90	6423.0
95.00	47688.0
96.00	3117.0
97.00	140.0
103.80	330.0
104.60	144.0
105.00	113.0
105.70	339.0
111.50	129.0
113.10	102.0
115.00	122.0
115.80	266.0
116.90	390.0
117.90	247.0
119.00	377.0
127.90	209.0
128.90	189.0
129.80	204.0
135.00	158.0
136.90	138.0
140.90	638.0
141.80	152.0
142.80	706.0
145.80	158.0
148.00	145.0
154.80	133.0
156.70	106.0
157.00	124.0
158.80	108.0
171.90	239.0
173.90	35184.0
174.90	3097.0
175.90	34800.0
176.90	2396.0

Instrument :
MSVOA_V
ClientSampleId :
BFB47