




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061324\
Data File : VV036052.D
Acq On : 13 Jun 2024 11:05
Operator : SY/MD
Sample : P2850-09
Misc : 5.31g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB10

Manual IntegrationsAPPROVED

Quant Time: Jun 14 01:16:36 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 14 01:10:24 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/20/2024
Supervised By :Semsettin Yesilyurt 06/20/2024

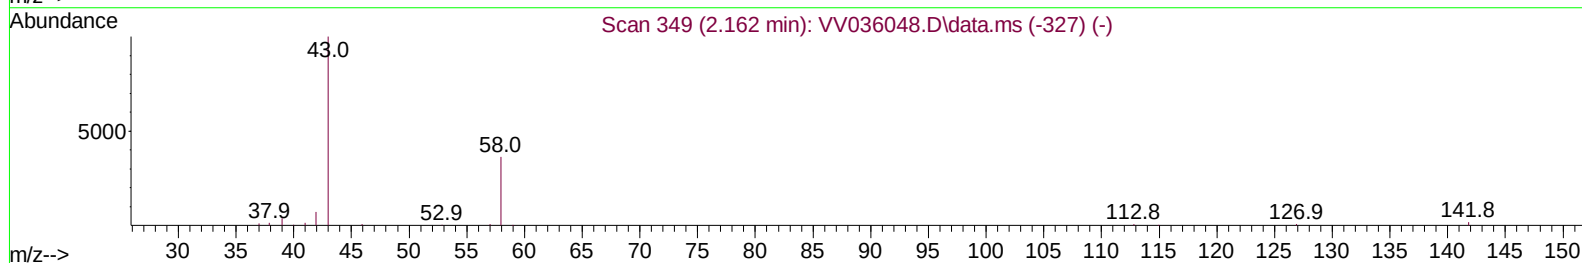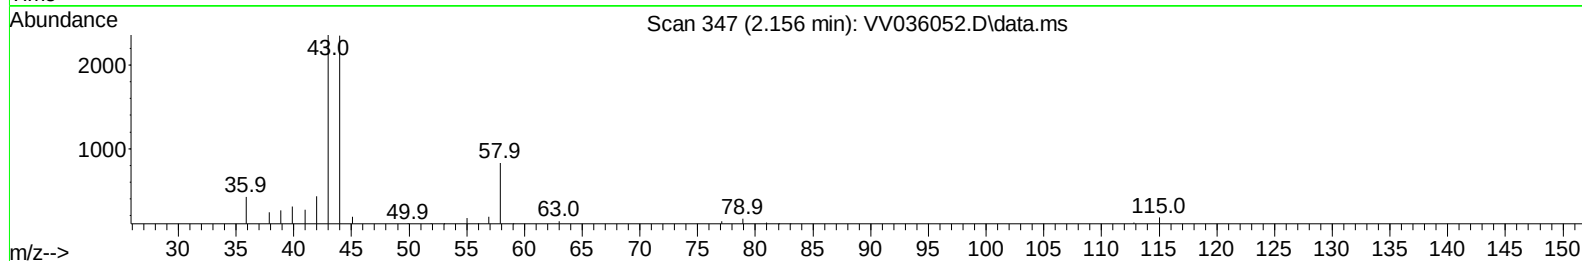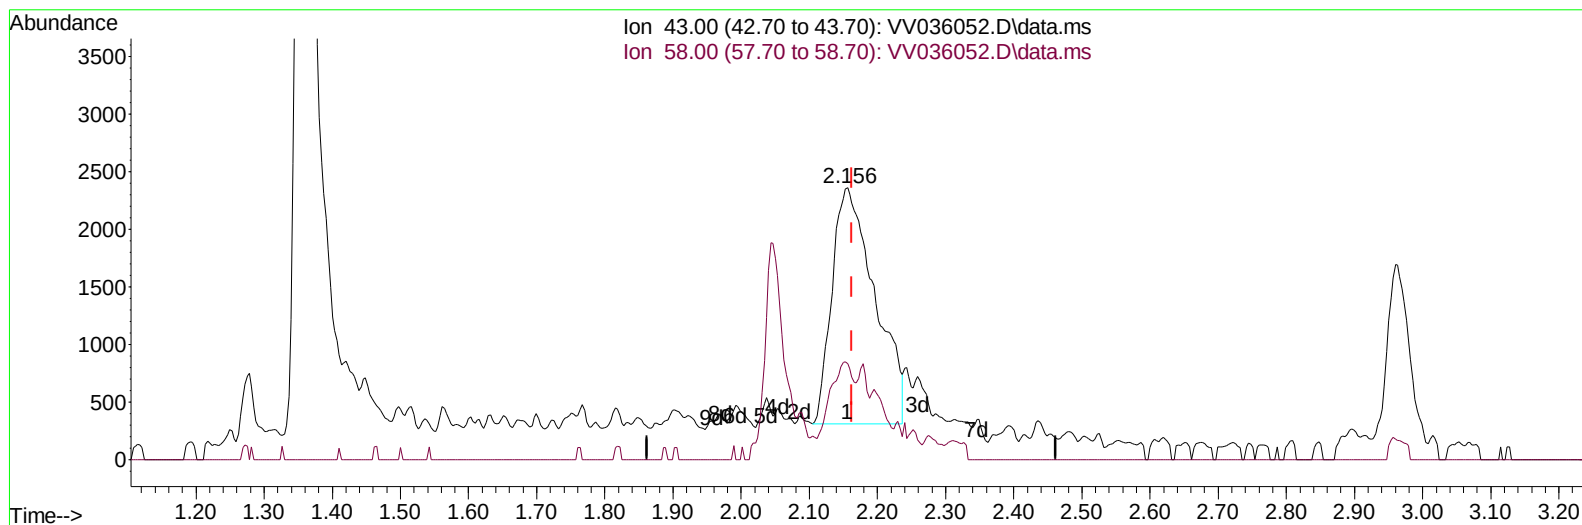

TIC: VV036052.D\data.ms

(13) Acetone (T)

2.156min (-0.006) 4.17 ug/L

response 8949

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	12.10	17.15
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061324\
Data File : VV036052.D
Acq On : 13 Jun 2024 11:05
Operator : SY/MD
Sample : P2850-09
Misc : 5.31g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB10

Manual IntegrationsAPPROVED

Quant Time: Jun 14 01:16:36 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 14 01:10:24 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/20/2024
Supervised By :Semsettin Yesilyurt 06/20/2024

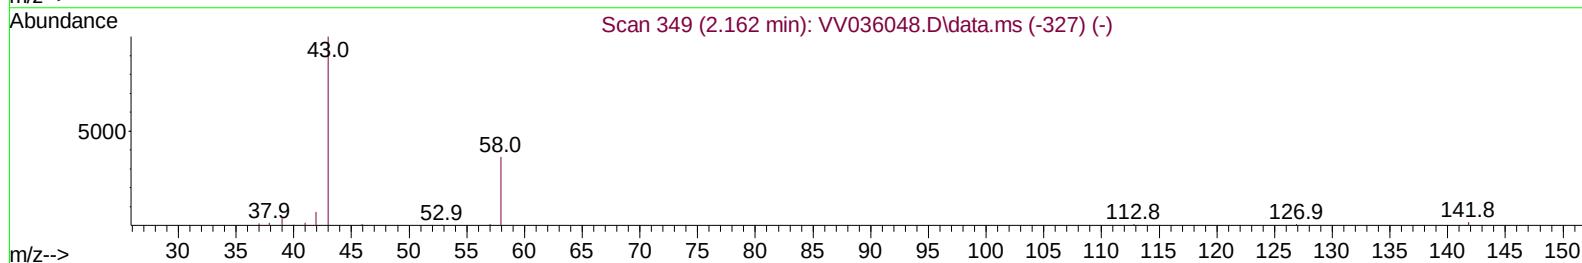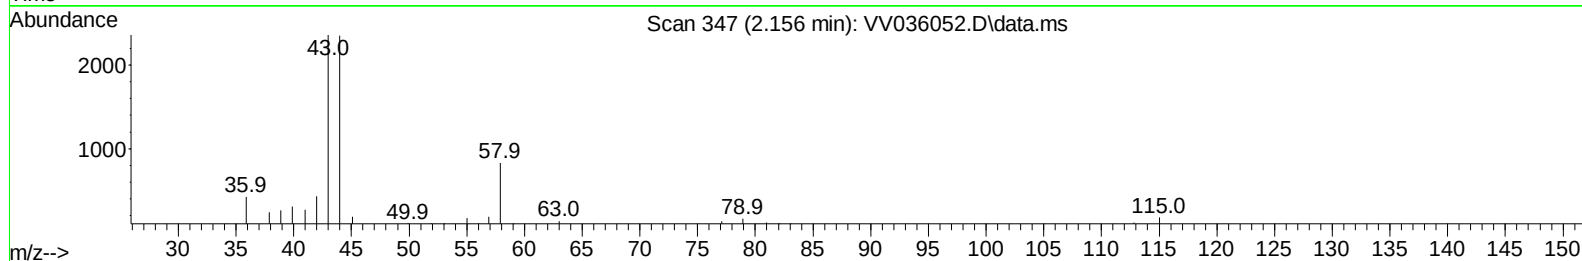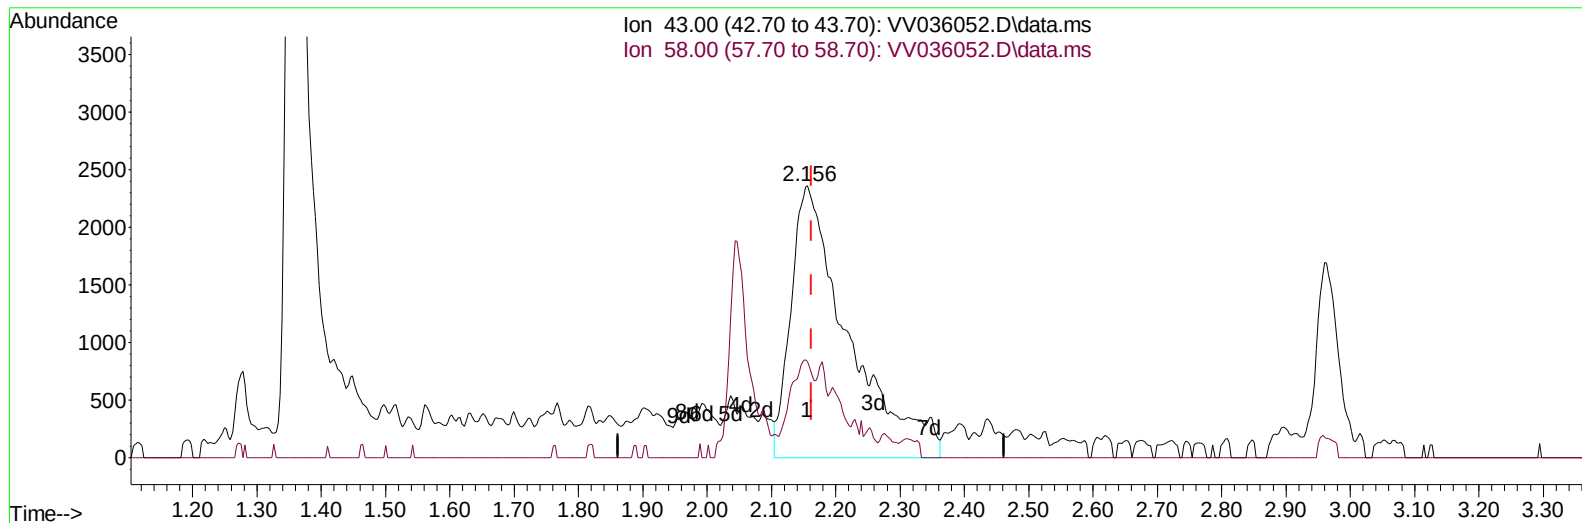

TIC: VV036052.D\data.ms

(13) Acetone (T)

2.156min (-0.006) 6.81 ug/L m

response 14602

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	12.10	10.51
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061324\
Data File : VV036052.D
Acq On : 13 Jun 2024 11:05
Operator : SY/MD
Sample : P2850-09
Misc : 5.31g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB10

Manual IntegrationsAPPROVED

Quant Time: Jun 14 01:16:36 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 14 01:10:24 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/20/2024
Supervised By :Semsettin Yesilyurt 06/20/2024

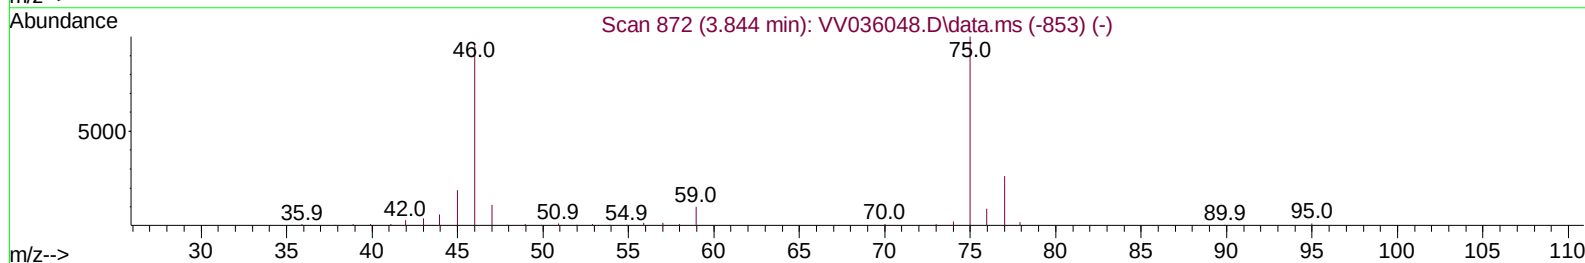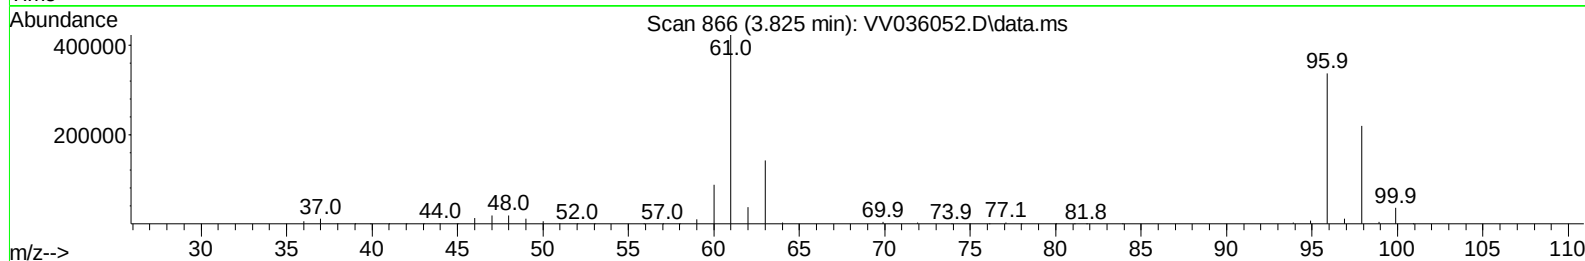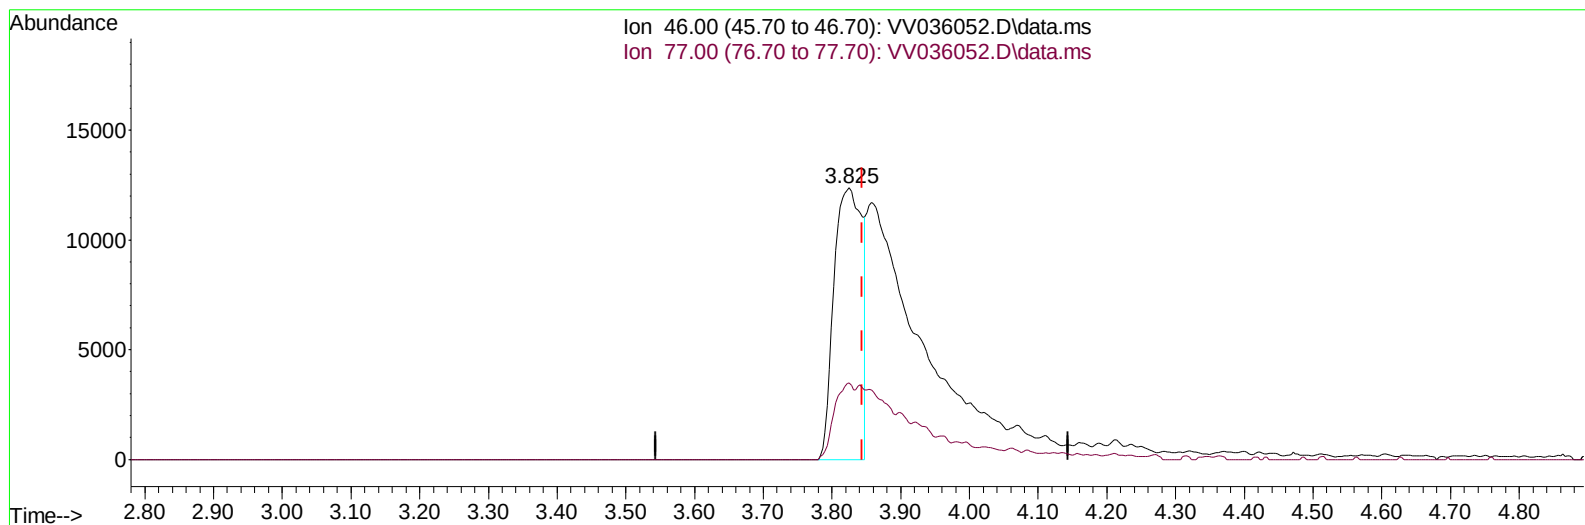

TIC: VV036052.D\data.ms

(21) 2-Butanone-d5 (S)

3.825min (-0.019) 25.61 ug/L

response 35266

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	11.90	20.63#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061324\
Data File : VV036052.D
Acq On : 13 Jun 2024 11:05
Operator : SY/MD
Sample : P2850-09
Misc : 5.31g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB10

Manual IntegrationsAPPROVED

Quant Time: Jun 14 01:16:36 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 14 01:10:24 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/20/2024
Supervised By :Semsettin Yesilyurt 06/20/2024

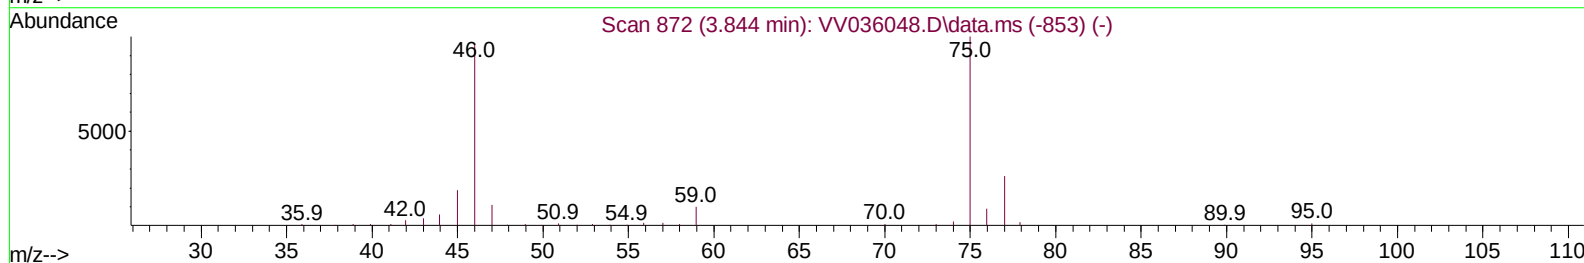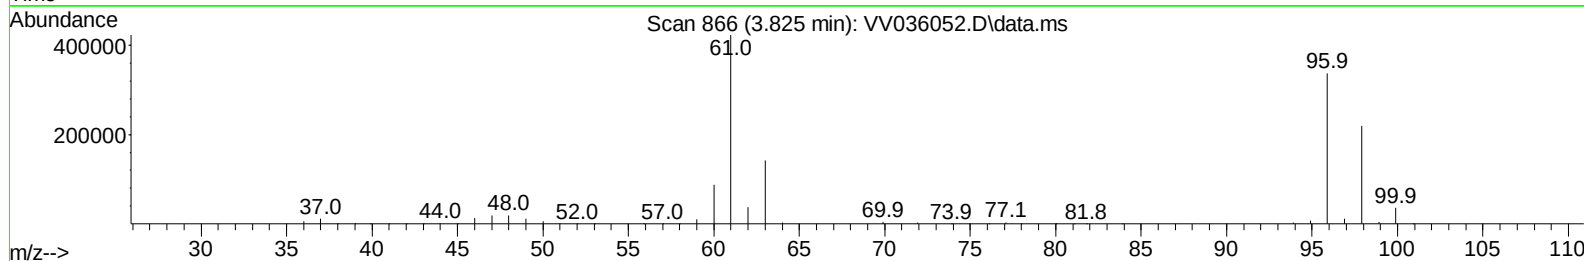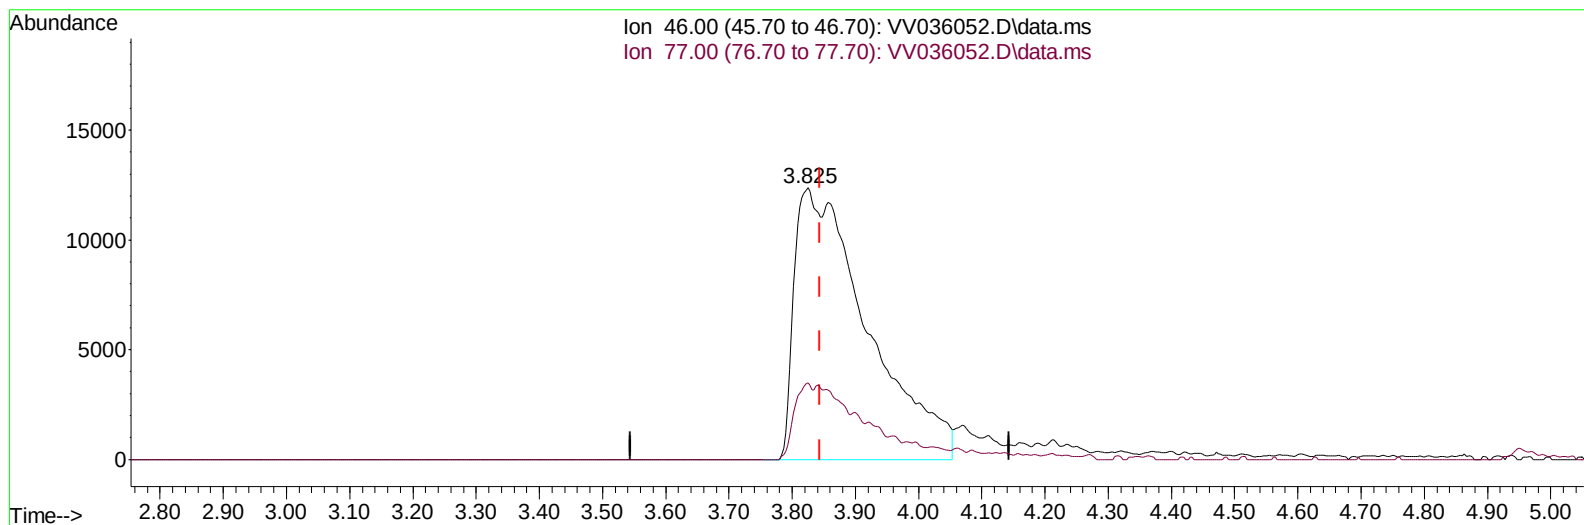

TIC: VV036052.D\data.ms

(21) 2-Butanone-d5 (S)

3.825min (-0.019) 71.96 ug/L m

response 99100

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	11.90	7.34#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061324\
 Data File : VV036052.D
 Acq On : 13 Jun 2024 11:05
 Operator : SY/MD
 Sample : P2850-09
 Misc : 5.31g/10.0mL/MSVOA_V/SOIL/A
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB10

Manual IntegrationsAPPROVED

Quant Time: Jun 14 01:16:36 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 14 01:10:24 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/20/2024
 Supervised By :Semsettin Yesilyurt 06/20/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.532	114		326462	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117		345138	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152		163262	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.275	65		163356	27.217	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	108.880%	
7) Chloroethane-d5	1.529	69		128428	26.835	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	107.360%	
11) 1,1-Dichloroethene-d2	2.053	65		69183	25.892	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	103.560%	
21) 2-Butanone-d5	3.825	46		99100m	71.964	ug/L	-0.02
Spiked Amount 50.000	Range 20	- 135		Recovery	=	143.920%#	
24) Chloroform-d	4.246	84		261896	25.233	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	100.920%	
26) 1,2-Dichloroethane-d4	4.941	65		149281	27.433	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	109.720%	
32) Benzene-d6	4.957	84		512153	24.964	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	99.840%	
36) 1,2-Dichloropropane-d6	5.986	67		169191	26.188	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	104.760%	
41) Toluene-d8	7.240	98		415300	22.942	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	91.760%	
43) trans-1,3-Dichloroprop...	7.555	79		60125	22.697	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	90.800%	
47) 2-Hexanone-d5	8.030	63		63080	72.064	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	144.120%#	
56) 1,1,2,2-Tetrachloroeth...	10.149	84		158705	32.873	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	131.480%#	
66) 1,2-Dichlorobenzene-d4	11.558	152		163117	27.245	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	109.000%	
Target Compounds							
							Qvalue
13) Acetone	2.156	43		14602m	6.807	ug/L	
16) Methylene chloride	2.442	84		52602	7.121	ug/L	98
17) trans-1,2-Dichloroethene	2.696	96		2639	0.475	ug/L	96
19) 1,1-Dichloroethane	3.111	63		6922	0.655	ug/L	98
20) cis-1,2-Dichloroethene	3.806	96		1596362	286.080	ug/L	99
34) Trichloroethene	5.834	95		36907	5.335	ug/L	100
42) Toluene	7.326	91		11298	0.490	ug/L	88
46) Tetrachloroethene	7.902	164		272078	53.772	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061324\
Data File : VV036052.D
Acq On : 13 Jun 2024 11:05
Operator : SY/MD
Sample : P2850-09
Misc : 5.31g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB10

Manual IntegrationsAPPROVED

Quant Time: Jun 14 01:16:36 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 14 01:10:24 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/20/2024
Supervised By :Semsettin Yesilyurt 06/20/2024

