




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061324\
Data File : VV036059.D
Acq On : 13 Jun 2024 13:45
Operator : SY/MD
Sample : P2798-07RE
Misc : 5.54g/10.0mL/MSVOA_V/SOIL/B
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB58RE

Manual IntegrationsAPPROVED

Quant Time: Jun 14 01:18:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 14 01:10:24 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/20/2024
Supervised By :Semsettin Yesilyurt 06/20/2024

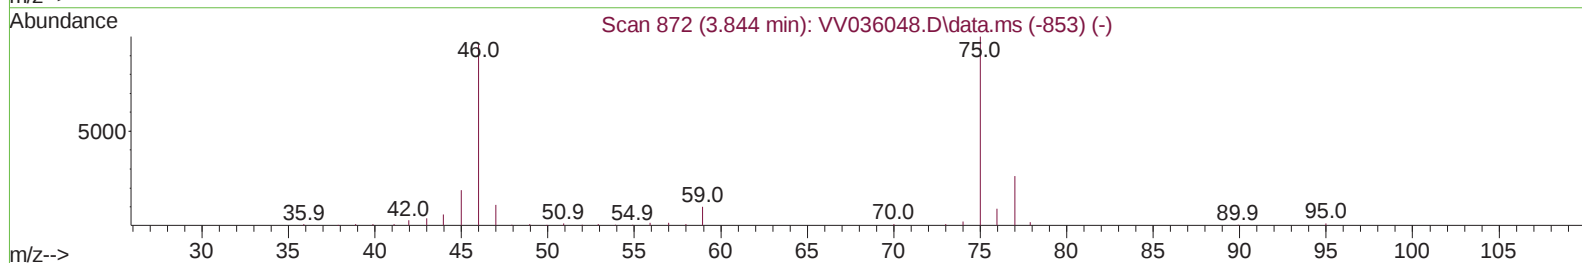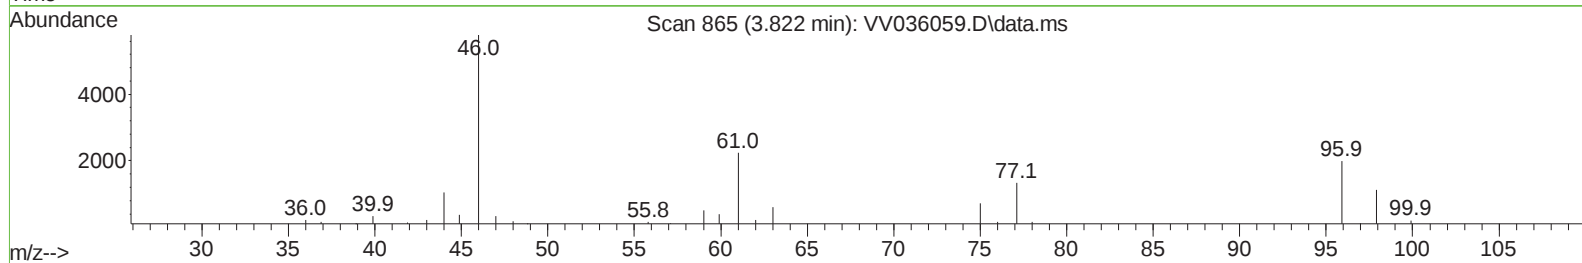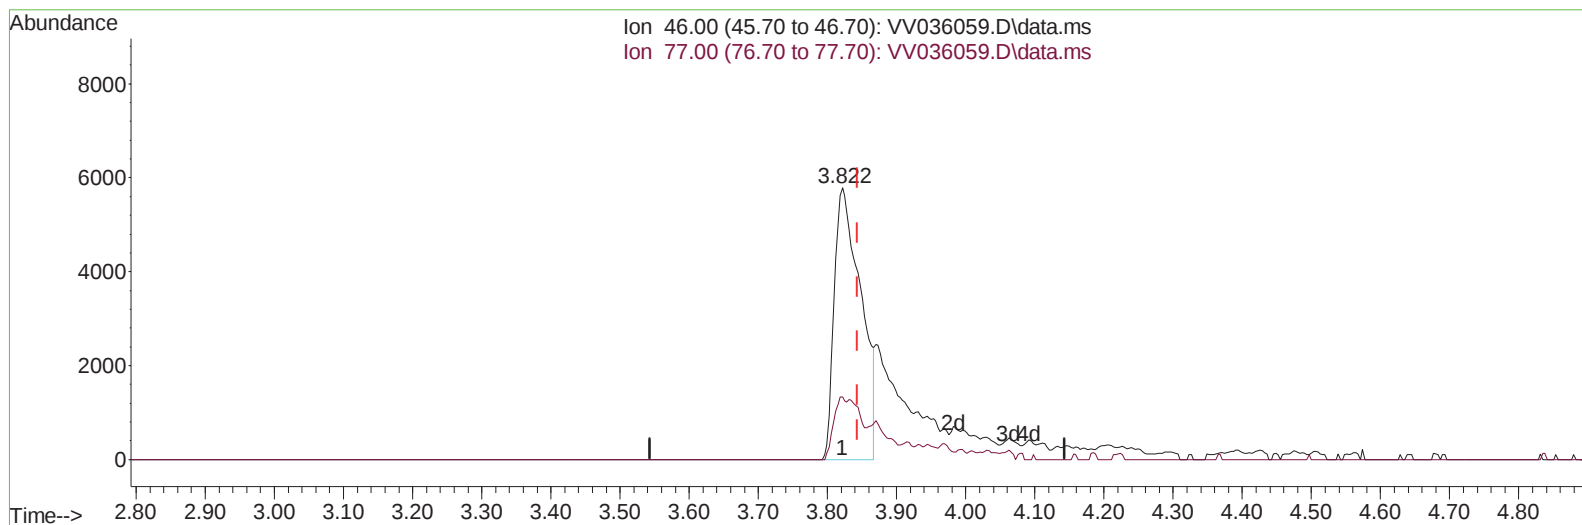

TIC: VV036059.D\data.ms

(21) 2-Butanone-d5 (S)

3.822min (-0.022) 15.30 ug/L

response 15524

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	11.90	11.30
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061324\
Data File : VV036059.D
Acq On : 13 Jun 2024 13:45
Operator : SY/MD
Sample : P2798-07RE
Misc : 5.54g/10.0mL/MSVOA_V/SOIL/B
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB58RE

Manual IntegrationsAPPROVED

Quant Time: Jun 14 01:18:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 14 01:10:24 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/20/2024
Supervised By :Semsettin Yesilyurt 06/20/2024

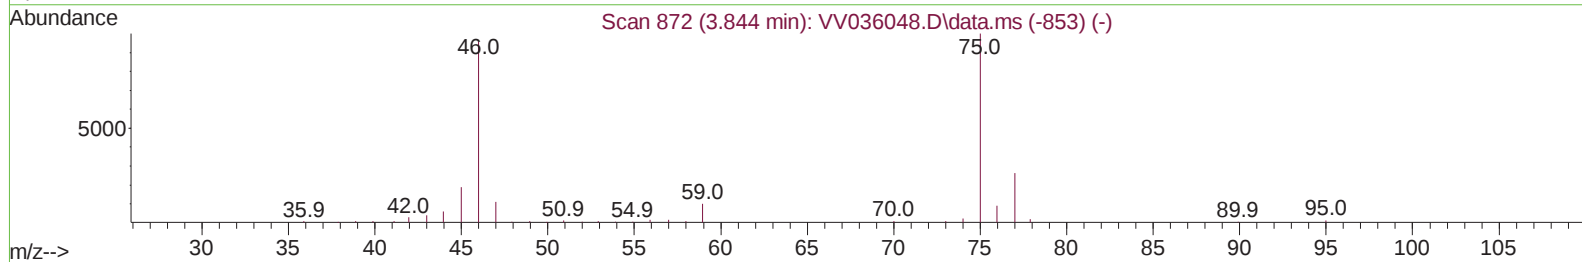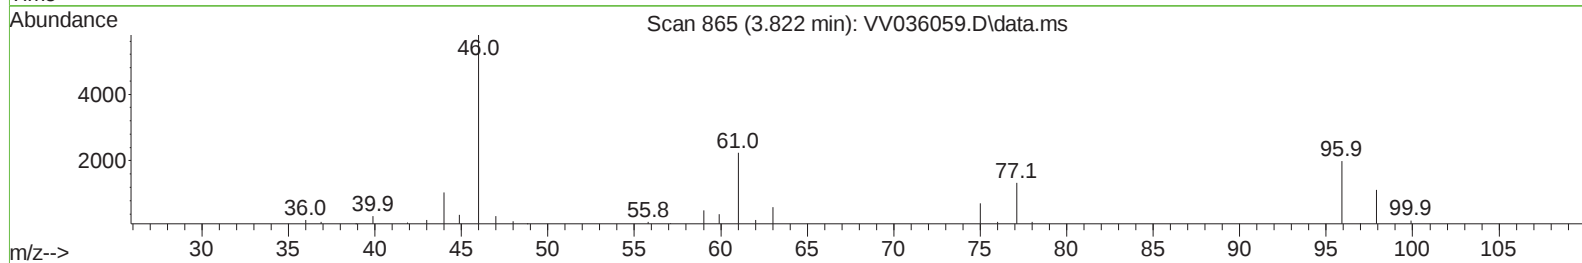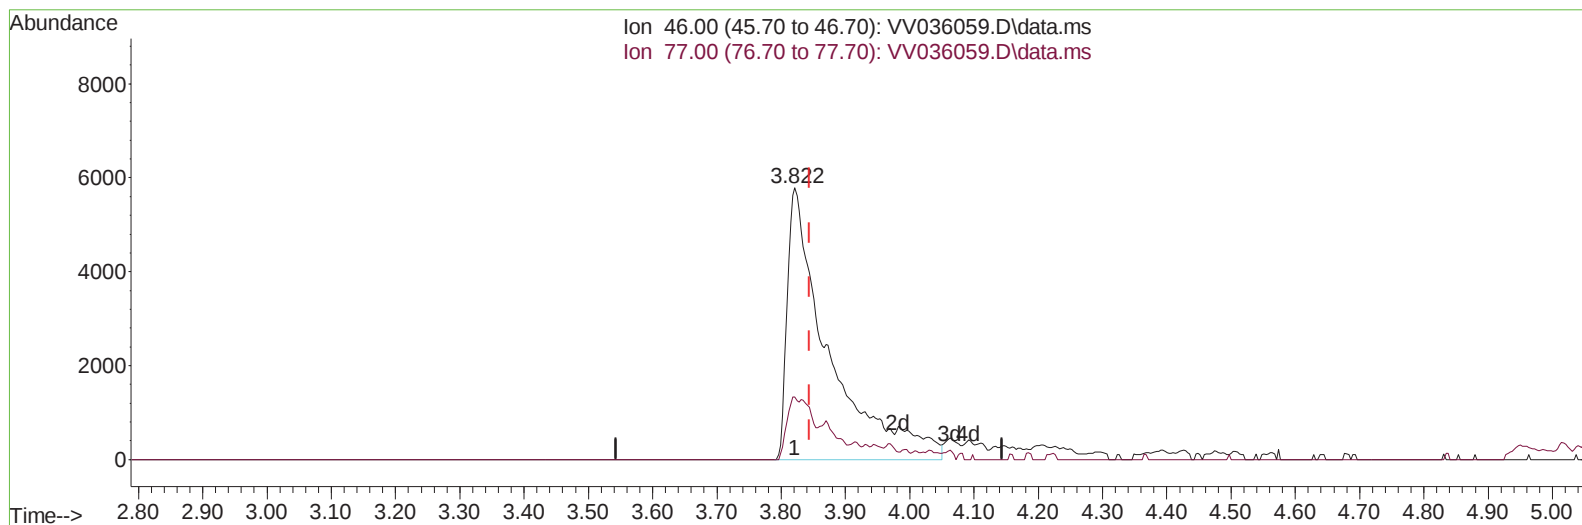

TIC: VV036059.D\data.ms

(21) 2-Butanone-d5 (S)

3.822min (-0.022) 25.39 ug/L m

response 25752

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	11.90	6.81#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061324\
 Data File : VV036059.D
 Acq On : 13 Jun 2024 13:45
 Operator : SY/MD
 Sample : P2798-07RE
 Misc : 5.54g/10.0mL/MSVOA_V/SOIL/B
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB58RE

Manual IntegrationsAPPROVED

Quant Time: Jun 14 01:18:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 14 01:10:24 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/20/2024
 Supervised By :Semsettin Yesilyurt 06/20/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	240486	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	228078	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	89454	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	105929	23.959	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	95.840%	
7) Chloroethane-d5	1.529	69	92388	26.206	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	104.840%	
11) 1,1-Dichloroethene-d2	2.056	65	50026	25.416	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	101.680%	
21) 2-Butanone-d5	3.822	46	25752m	25.386	ug/L	-0.02
Spiked Amount 50.000	Range 20	- 135	Recovery	=	50.780%	
24) Chloroform-d	4.249	84	184355	24.113	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	96.440%	
26) 1,2-Dichloroethane-d4	4.940	65	77578	19.353	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	77.400%	
32) Benzene-d6	4.957	84	347368	25.622	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	102.480%	
36) 1,2-Dichloropropane-d6	5.989	67	106835	25.023	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	100.080%	
41) Toluene-d8	7.243	98	268118	22.414	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	89.640%	
43) trans-1,3-Dichloroprop...	7.561	79	25462	14.545	ug/L	0.01
Spiked Amount 25.000	Range 30	- 135	Recovery	=	58.200%	
47) 2-Hexanone-d5	8.034	63	13848	23.940	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	47.880%	
56) 1,1,2,2-Tetrachloroeth...	10.152	84	68233	21.387	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	85.560%	
66) 1,2-Dichlorobenzene-d4	11.558	152	82266	25.078	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	100.320%	
Target Compounds						
16) Methylene chloride	2.445	84	22069	4.056	ug/L	98
20) cis-1,2-Dichloroethene	3.825	96	5230	1.272	ug/L	87
46) Tetrachloroethene	7.905	164	4973	1.487	ug/L	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061324\
Data File : VV036059.D
Acq On : 13 Jun 2024 13:45
Operator : SY/MD
Sample : P2798-07RE
Misc : 5.54g/10.0mL/MSVOA_V/SOIL/B
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB58RE

Manual IntegrationsAPPROVED

Quant Time: Jun 14 01:18:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 14 01:10:24 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/20/2024
Supervised By :Semsettin Yesilyurt 06/20/2024

