

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061424\
 Data File : VV036085.D
 Acq On : 14 Jun 2024 11:33
 Operator : SY/MD
 Sample : P2850-13
 Misc : 5.51g/10.0mL/MSVOA_V/SOIL/B
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB56

Quant Time: Jun 15 01:31:57 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 15 01:30:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	369420	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	354070	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	130808	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	165777	24.408	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	97.640%
7) Chloroethane-d5	1.529	69	128297	23.691	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	94.760%
11) 1,1-Dichloroethene-d2	2.056	65	69709	23.055	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	92.240%
21) 2-Butanone-d5	3.809	46	18551	11.905	ug/L	-0.03
Spiked Amount	50.000	Range	20 - 135	Recovery	=	23.800%
24) Chloroform-d	4.246	84	227185	19.344	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	77.360%
26) 1,2-Dichloroethane-d4	4.940	65	93039	15.109	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	60.440%#
32) Benzene-d6	4.957	84	464274	22.059	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	88.240%
36) 1,2-Dichloropropane-d6	5.985	67	135690	20.473	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	81.880%
41) Toluene-d8	7.243	98	390297	21.017	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	84.080%
43) trans-1,3-Dichloroprop...	7.558	79	38483	14.161	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	56.640%
47) 2-Hexanone-d5	8.037	63	14742	16.417	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	32.840%
56) 1,1,2,2-Tetrachloroeth...	10.152	84	69385	14.009	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	56.040%
66) 1,2-Dichlorobenzene-d4	11.558	152	97346	20.294	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	81.160%
Target Compounds						Qvalue
5) Vinyl chloride	1.281	62	5894	0.732	ug/L #	52
20) cis-1,2-Dichloroethene	3.809	96	270943	42.909	ug/L	99
34) Trichloroethene	5.834	95	35944	5.064	ug/L	97
46) Tetrachloroethene	7.902	164	355827	68.550	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061424\
Data File : VV036085.D
Acq On : 14 Jun 2024 11:33
Operator : SY/MD
Sample : P2850-13
Misc : 5.51g/10.0mL/MSVOA_V/SOIL/B
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHB56

Quant Time: Jun 15 01:31:57 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 15 01:30:52 2024
Response via : Initial Calibration




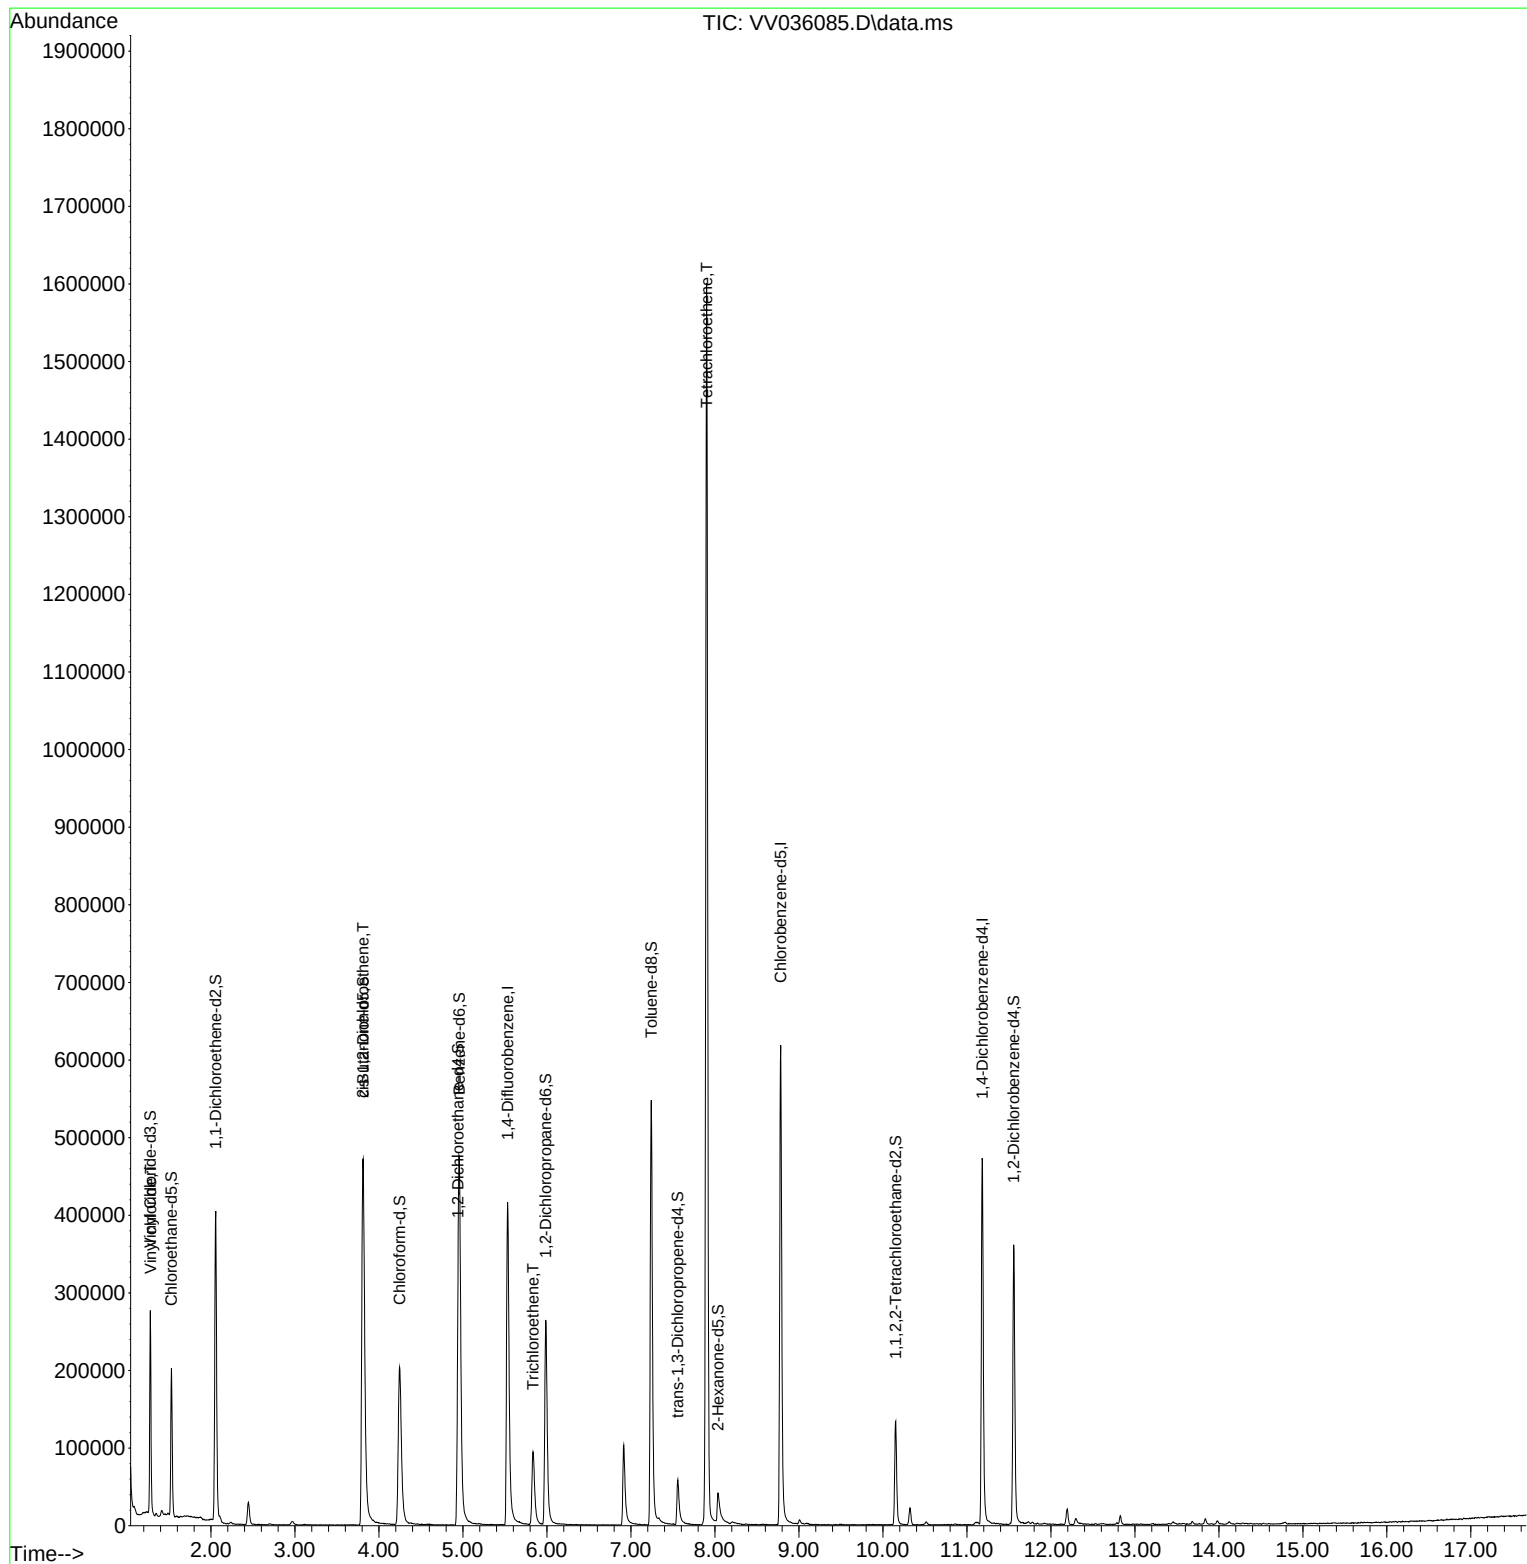


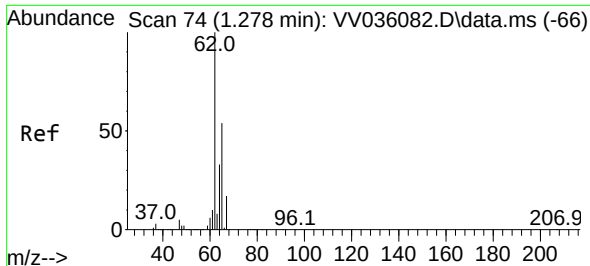

#5
 Vinyl chloride
 Concen: 0.732 ug/L
 RT: 1.281 min Scan# 74
 Delta R.T. 0.003 min
 Lab File: VV036085.D
 Acq: 14 Jun 2024 11:33




Instrument :
 MSVOA_V
 ClientSampleId :
 BHB56


Tgt Ion: 62 Resp: 5894
 Ion Ratio Lower Upper
 62 100
 64 60.0 22.9 42.5#

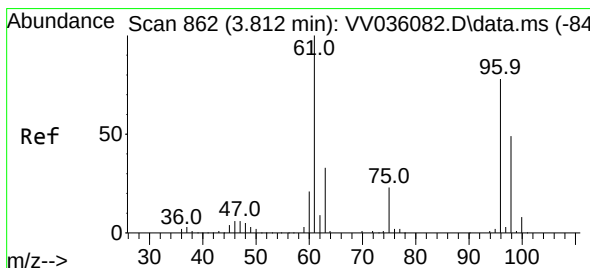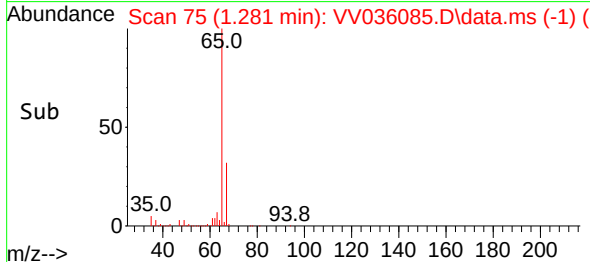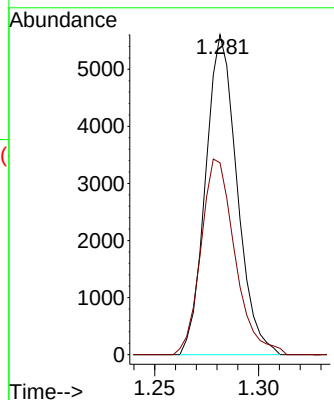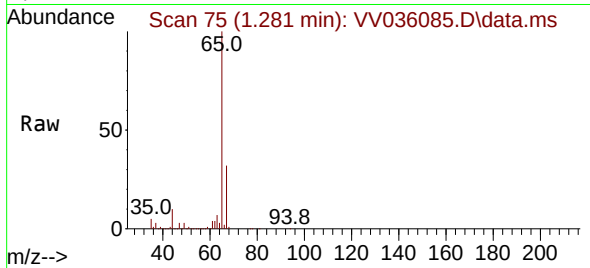

#20
 cis-1,2-Dichloroethene
 Concen: 42.909 ug/L
 RT: 3.809 min Scan# 861
 Delta R.T. -0.003 min
 Lab File: VV036085.D
 Acq: 14 Jun 2024 11:33

Tgt Ion: 96 Resp: 270943
 Ion Ratio Lower Upper
 96 100
 61 127.1 87.9 163.3
 98 62.7 44.4 82.5

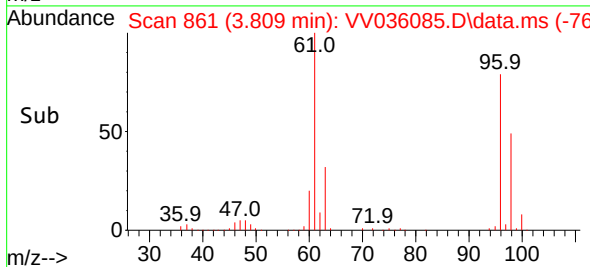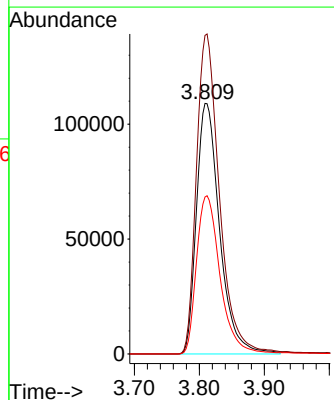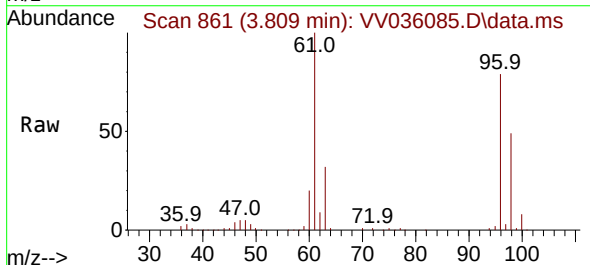




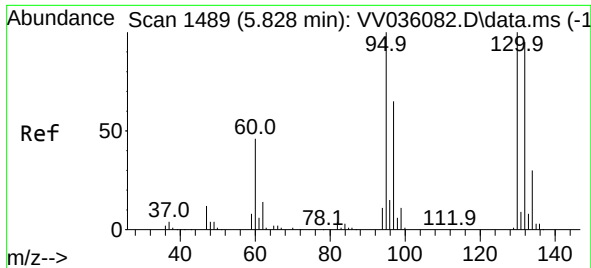


#34
 Trichloroethene
 Concen: 5.064 ug/L
 RT: 5.834 min Scan# 1491
 Delta R.T. 0.006 min
 Lab File: VV036085.D
 Acq: 14 Jun 2024 11:33

Instrument :
 MSVOA_V
 ClientSampleId :
 BHB56

Tgt Ion: 95 Resp: 35944

Ion	Ratio	Lower	Upper
95	100		
97	63.1	44.8	83.2
132	91.7	66.8	124.2
130	96.8	70.0	130.0

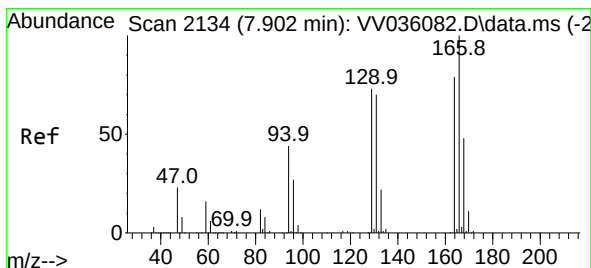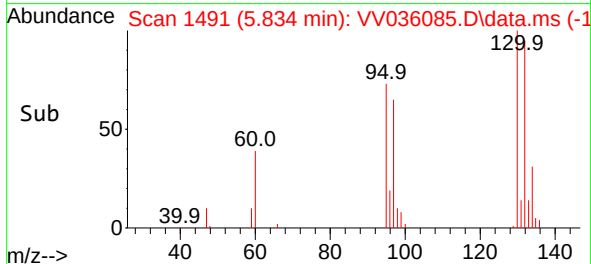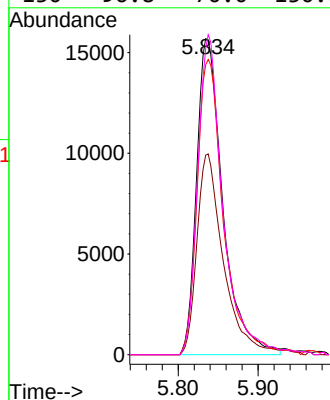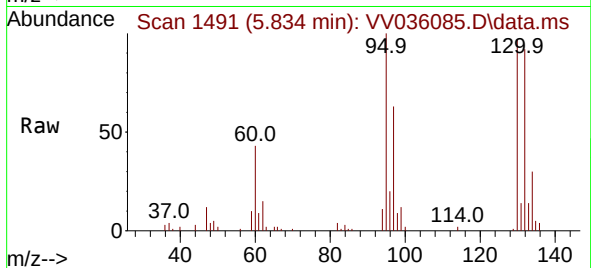

#46
 Tetrachloroethene
 Concen: 68.550 ug/L
 RT: 7.902 min Scan# 2134
 Delta R.T. -0.000 min
 Lab File: VV036085.D
 Acq: 14 Jun 2024 11:33

Tgt Ion: 164 Resp: 355827

Ion	Ratio	Lower	Upper
164	100		
129	94.0	64.6	120.0
131	88.9	63.2	117.4
166	126.4	89.5	166.3

