




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
 Data File : VV026279.D
 Acq On : 15 Jun 2022 15:45
 Operator : SY/MD
 Sample : N3275-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BC4

Manual IntegrationsAPPROVED

Quant Time: Jun 16 01:40:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jun 16 01:38:03 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/17/2022
 Supervised By :Mahesh Dadoda 06/17/2022

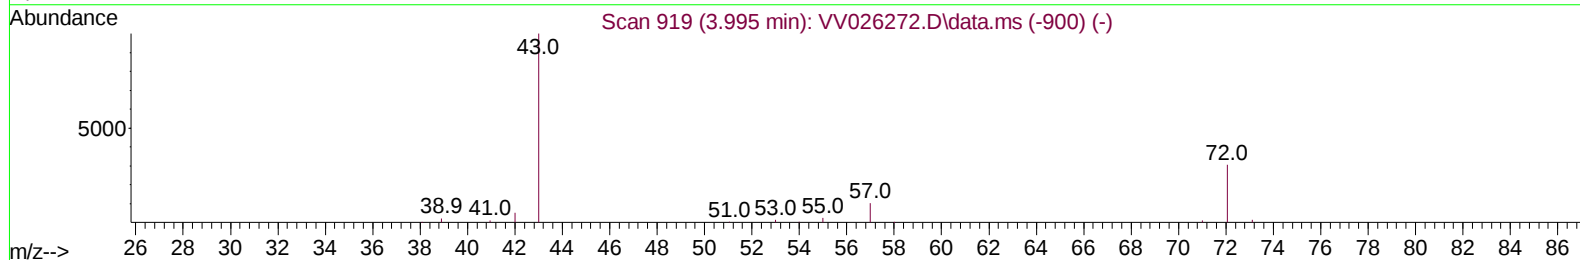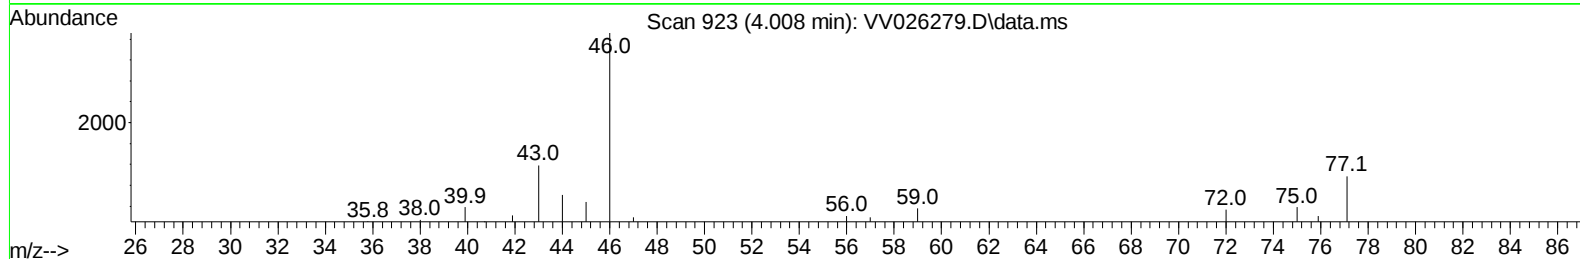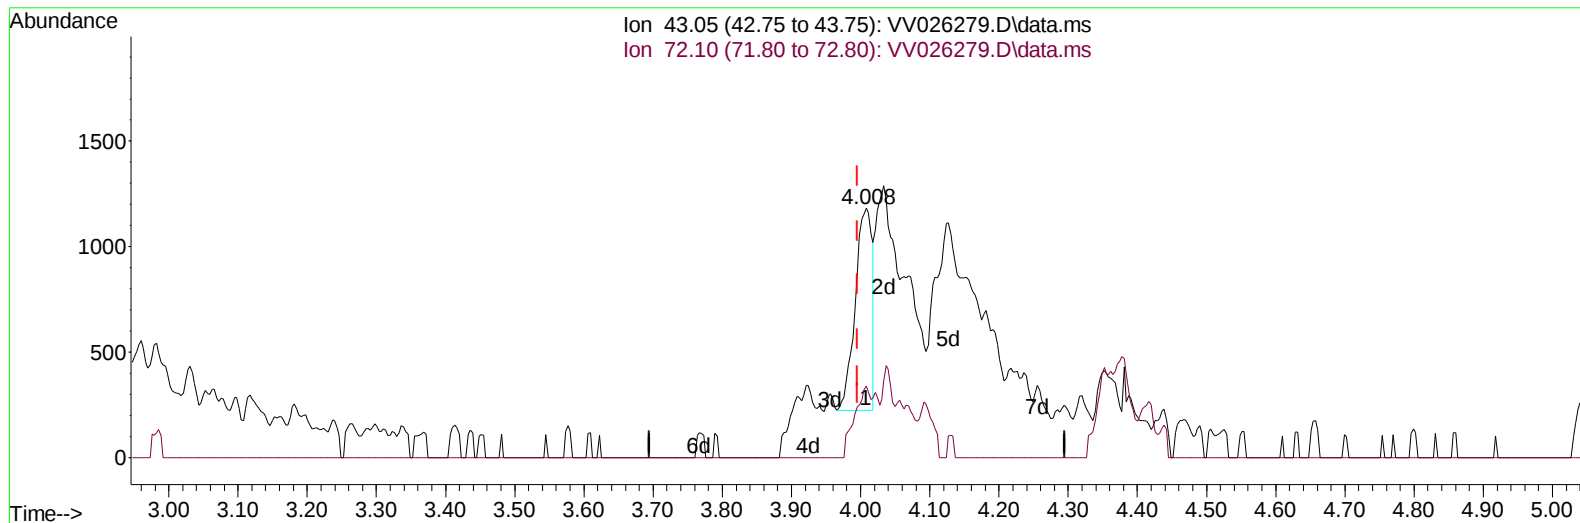

TIC: VV026279.D\data.ms

(21) 2-Butanone (T)

4.008min (+ 0.013) 0.97 ug/L

response 1620

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	25.30	32.65
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026279.D
Acq On : 15 Jun 2022 15:45
Operator : SY/MD
Sample : N3275-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BC4

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 06/17/2022
Supervised By :Mahesh Dadoda 06/17/2022

Quant Time: Jun 16 01:40:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jun 16 01:38:03 2022
Response via : Initial Calibration

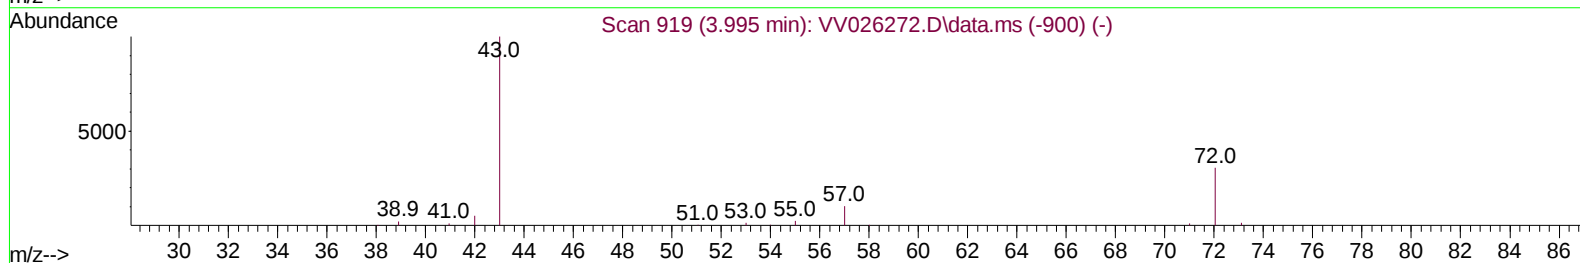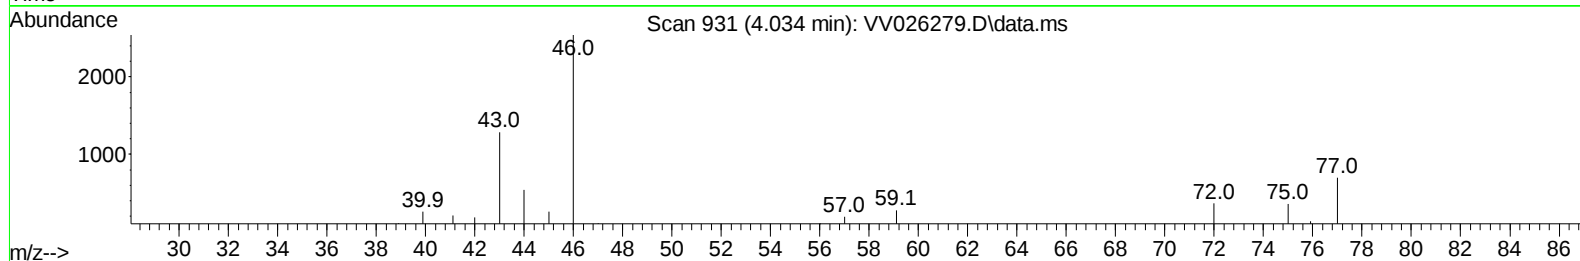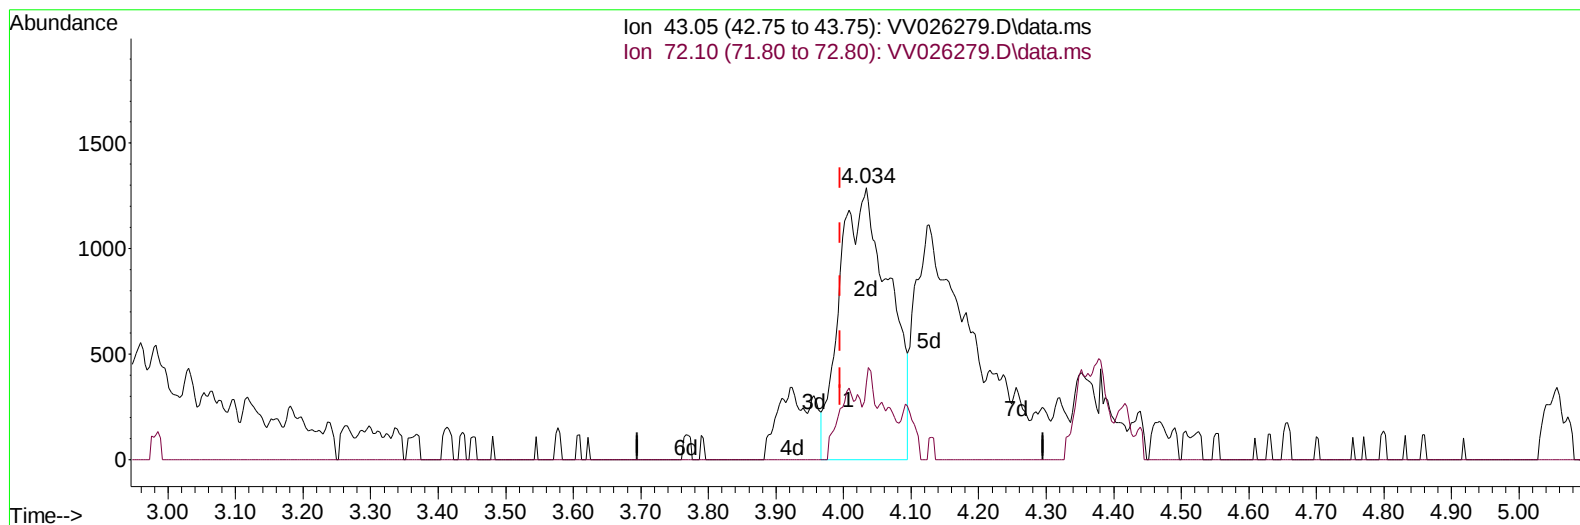

TIC: VV026279.D\data.ms

(21) 2-Butanone (T)

4.034min (+ 0.038) 3.92 ug/L m

response 6518

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	25.30	8.12#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
 Data File : VV026279.D
 Acq On : 15 Jun 2022 15:45
 Operator : SY/MD
 Sample : N3275-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BC4

Manual IntegrationsAPPROVED

Quant Time: Jun 16 01:40:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jun 16 01:38:03 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/17/2022
 Supervised By :Mahesh Dadoda 06/17/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	195835	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	189319	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	79470	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.317	65	82210	4.833	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	96.600%	
7) Chloroethane-d5	1.577	69	66713	4.988	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	99.800%	
11) 1,1-Dichloroethene-d2	2.117	63	112874	3.864	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	77.200%	
20) 2-Butanone-d5	3.918	46	100389	60.485	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	120.960%	
24) Chloroform-d	4.358	84	129520	5.195	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	104.000%	
26) 1,2-Dichloroethane-d4	5.040	65	55266	5.240	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	104.800%	
32) Benzene-d6	5.056	84	257003	5.078	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	101.600%	
36) 1,2-Dichloropropane-d6	6.075	67	78901	5.341	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	106.800%	
41) Toluene-d8	7.316	98	209390	4.537	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	90.800%	
43) trans-1,3-Dichloroprop...	7.628	79	20463	4.272	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	85.400%	
46) 2-Hexanone-d5	8.091	63	72595	50.170	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	100.340%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	47217	5.189	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	103.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	69570	5.683	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	113.600%	
Target Compounds						
						Qvalue
9) Trichlorofluoromethane	1.764	101	11111	0.476	ug/L	99
13) Acetone	2.201	43	517645	402.444	ug/L	87
21) 2-Butanone	4.034	43	6518m	3.916	ug/L	
22) cis-1,2-Dichloroethene	3.924	96	3834	0.316	ug/L	88
34) Trichloroethene	5.927	95	4067	0.307	ug/L	94
47) Tetrachloroethene	7.982	164	2389	0.243	ug/L #	75

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061522\
Data File : VV026279.D
Acq On : 15 Jun 2022 15:45
Operator : SY/MD
Sample : N3275-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BC4

Manual IntegrationsAPPROVED

Quant Time: Jun 16 01:40:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jun 16 01:38:03 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/17/2022
Supervised By :Mahesh Dadoda 06/17/2022

